

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110220\
Data File : P0072987.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2020 18:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 03:41:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.950	4.027	1091350	699138	23.670	19.948
2)	SA Decachlor...	10.984	9.308	744912	609732	20.163	18.283

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110220\
Data File : PO072987.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2020 18:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 03:41:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

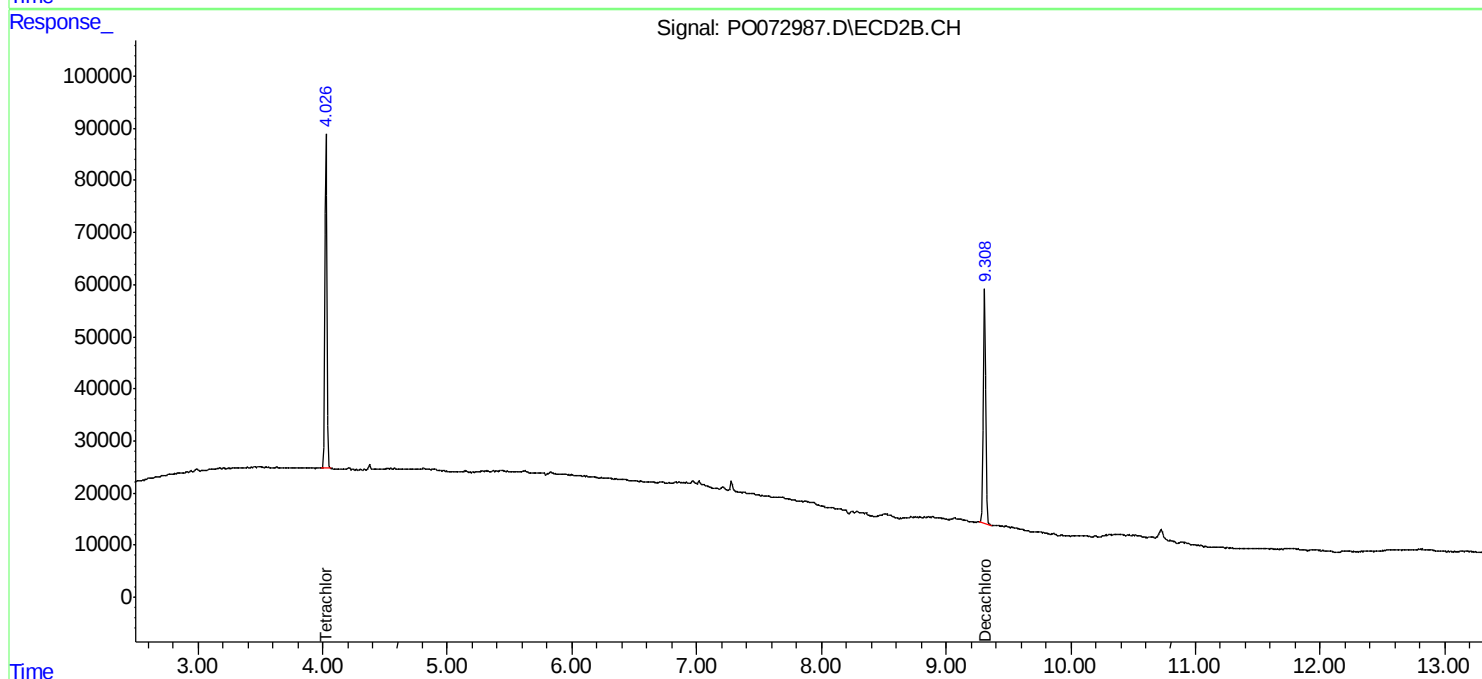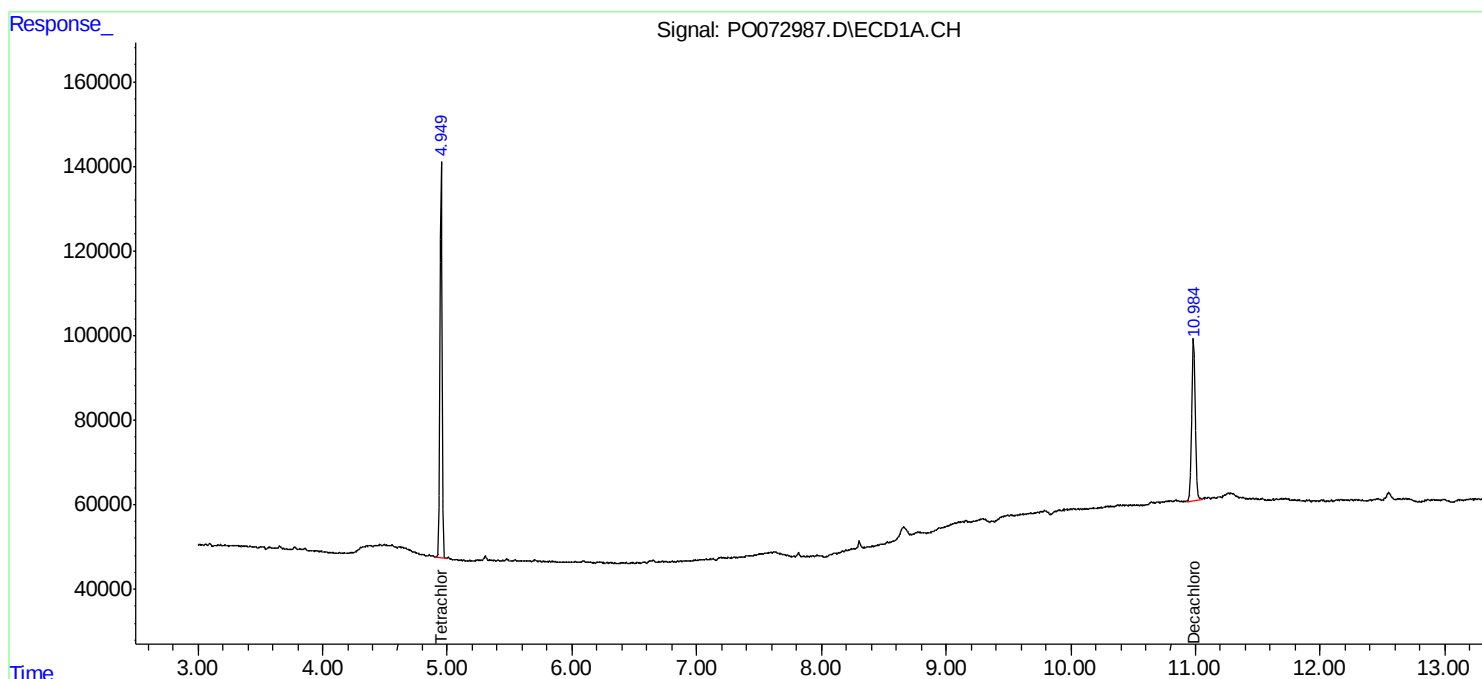


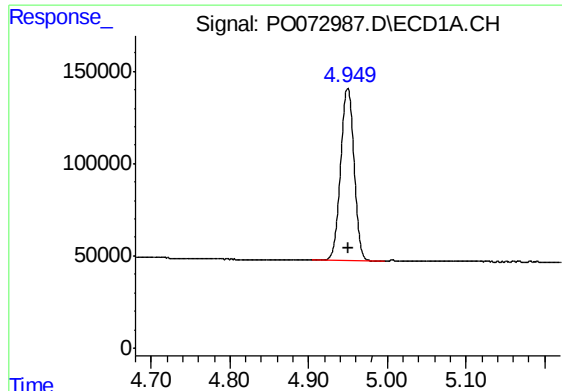

#1 Tetrachloro-m-xylene


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 1091350
Conc: 23.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

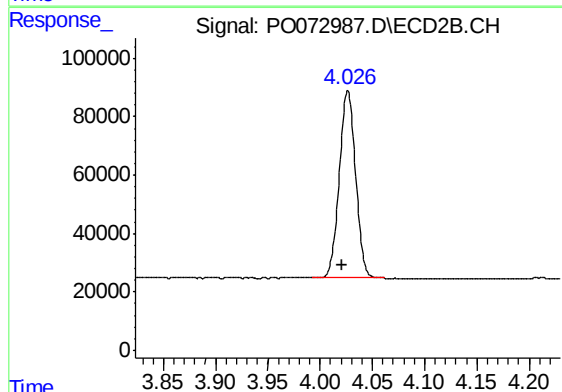


#1 Tetrachloro-m-xylene

R.T.: 4.027 min
Delta R.T.: 0.005 min
Response: 699138
Conc: 19.95 ng/ml

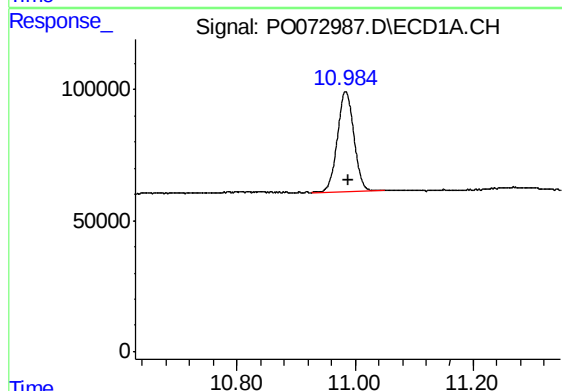

#2 Decachlorobiphenyl

R.T.: 10.984 min
Delta R.T.: -0.005 min
Response: 744912
Conc: 20.16 ng/ml

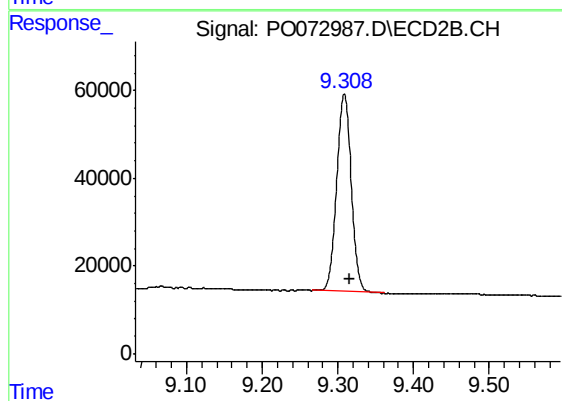

#2 Decachlorobiphenyl

R.T.: 9.308 min
Delta R.T.: -0.008 min
Response: 609732
Conc: 18.28 ng/ml