

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110220\
 Data File : PO072966.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2020 8:56
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 11/3/2020 3:33:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 03:30:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.952	4.025	1168941	831316	25.353	23.720
2) SA Decachlor...	10.990	9.309	1018371	761582	27.564m	22.837

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110220\
Data File : PO072966.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2020 8:56
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
11/3/2020 3:33:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 03:30:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

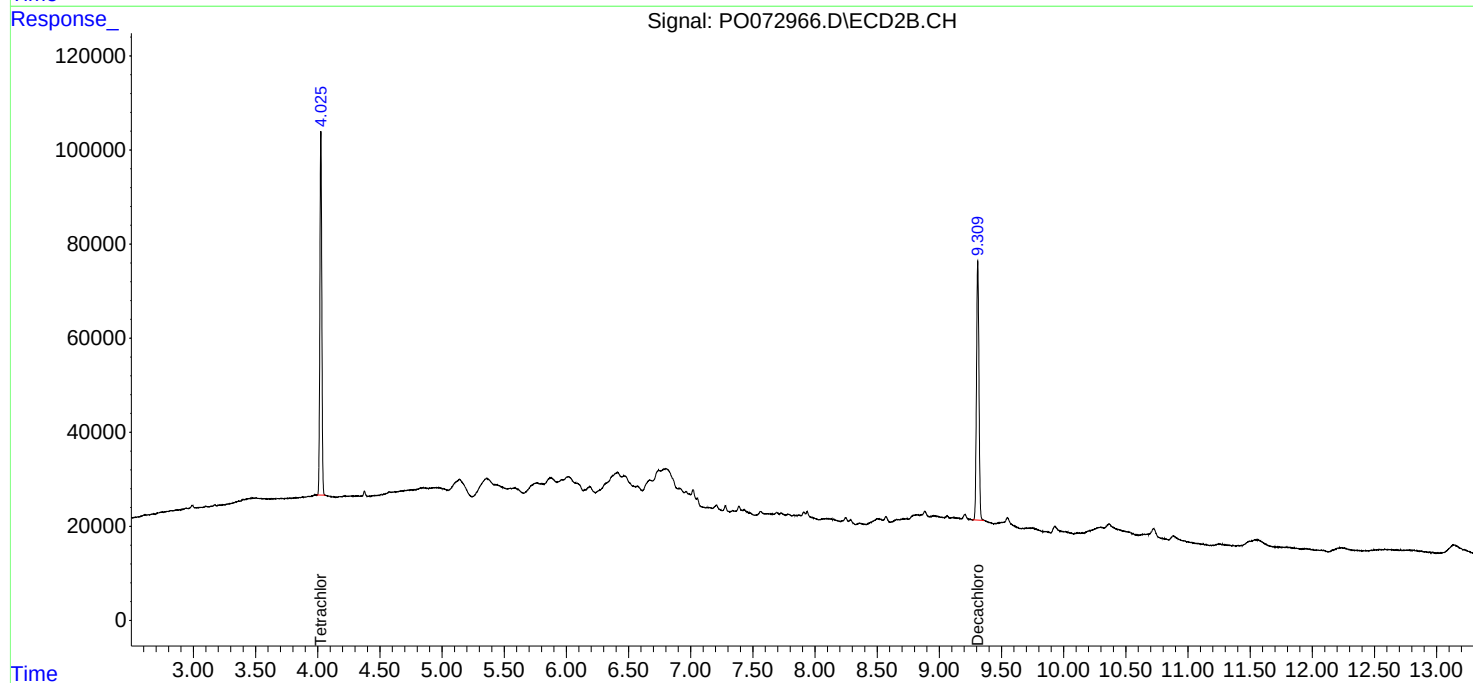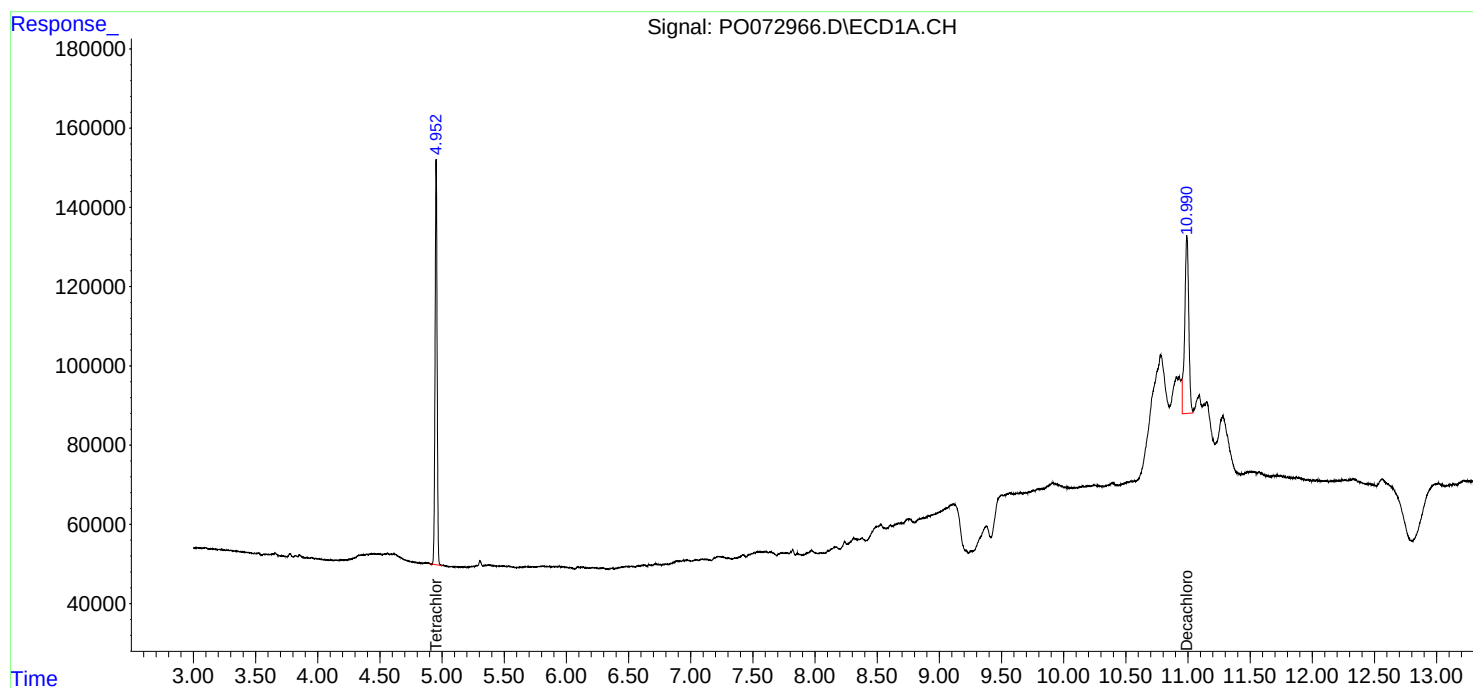

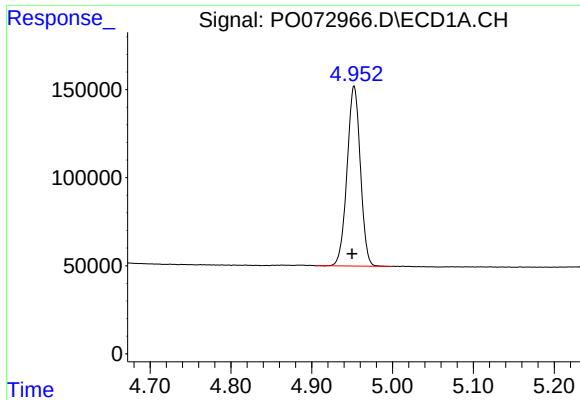


#1 Tetrachloro-m-xylene

R.T.: 4.952 min
Delta R.T.: 0.002 min
Response: 1168941
Conc: 25.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
11/3/2020 3:33:25 PM

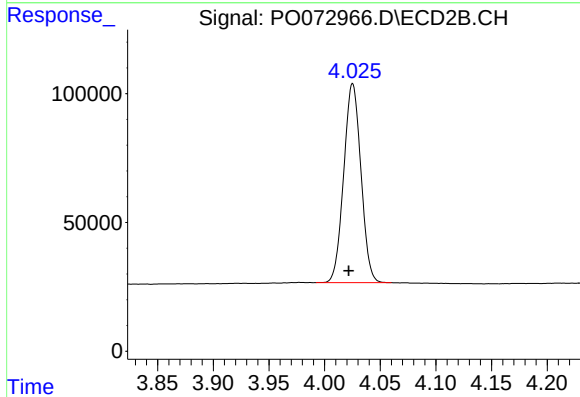


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.004 min
Response: 831316
Conc: 23.72 ng/ml

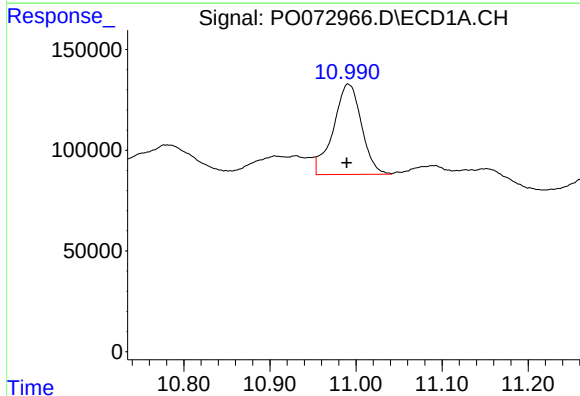

#2 Decachlorobiphenyl

R.T.: 10.990 min
Delta R.T.: 0.000 min
Response: 1018371
Conc: 27.56 ng/ml m

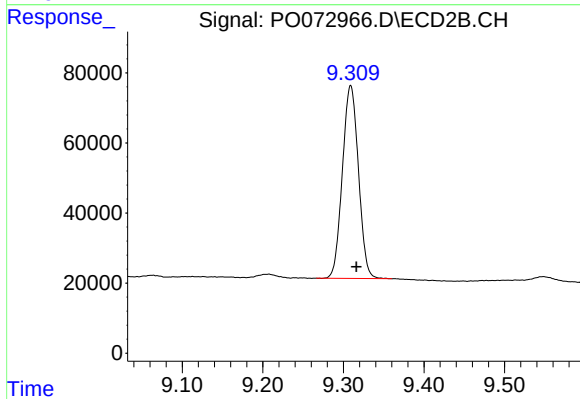

#2 Decachlorobiphenyl

R.T.: 9.309 min
Delta R.T.: -0.007 min
Response: 761582
Conc: 22.84 ng/ml