

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO110220\
 Data File : PO072991.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2020 20:07
 Operator : DD\AJ
 Sample : L4570-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MW-PIER-S

Manual Integrations
 APPROVED

Ankita
 11/3/2020 3:33:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 03:44:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.950	4.026	1437173	949924	31.171	27.104
2) SA Decachlor...	10.984	9.309	986423	790494	26.700	23.704
Target Compounds						
26) L6 AR-1254-1	7.187	6.147	21774	24034	12.564m	10.678
27) L6 AR-1254-2	7.417	6.306	67161	24754	25.136m	12.324 #
28) L6 AR-1254-3	7.801	6.723	50895	39150	18.832	12.323 #
29) L6 AR-1254-4	8.097	6.961	46778	37826	21.346	17.392
30) L6 AR-1254-5	8.527	7.389	42214	63328	19.531	22.753

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110220\
Data File : PO072991.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2020 20:07
Operator : DD\AJ
Sample : L4570-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
MW-PIER-S


Manual Integrations
APPROVED

Ankita
11/3/2020 3:33:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 03:44:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

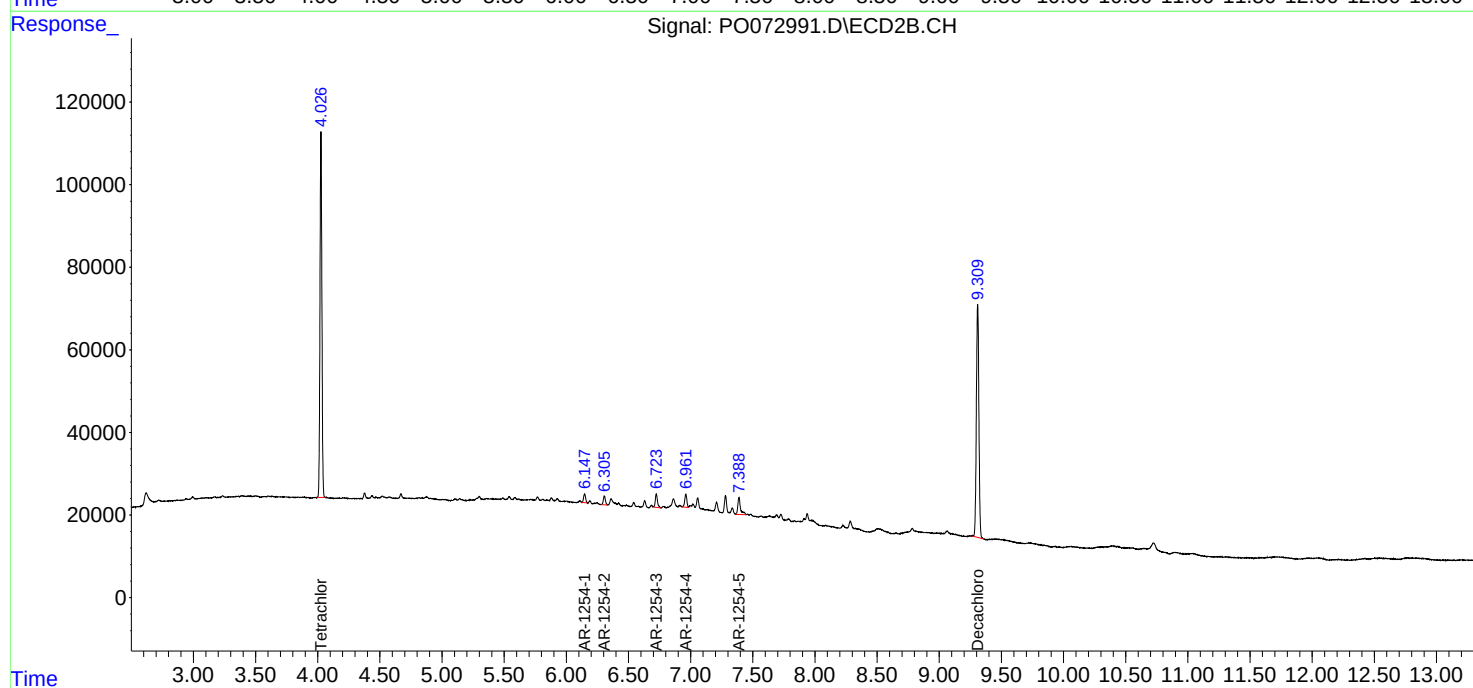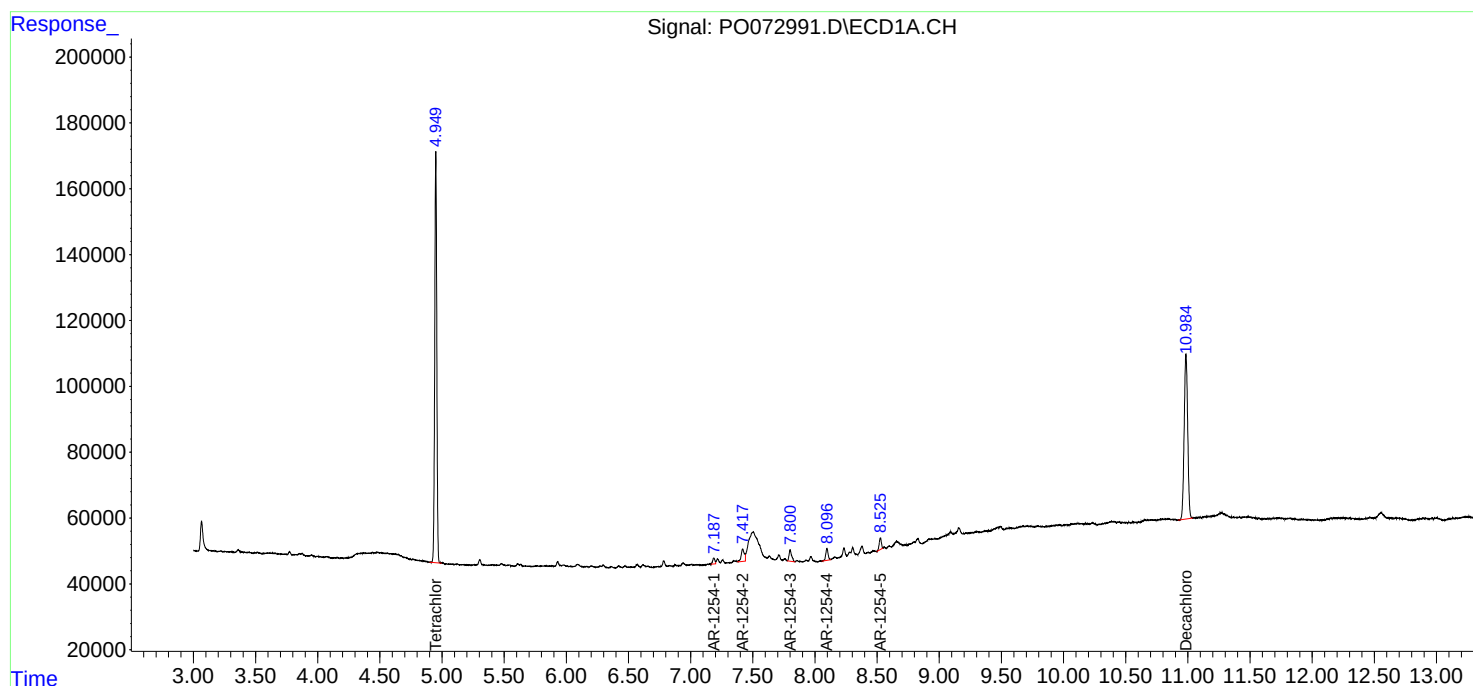

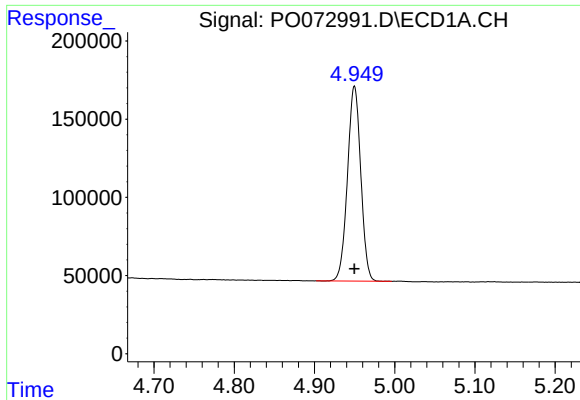


#1 Tetrachloro-m-xylene

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 1437173
Conc: 31.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-PIER-S


Manual Integrations
APPROVED

Ankita
11/3/2020 3:33:36 PM

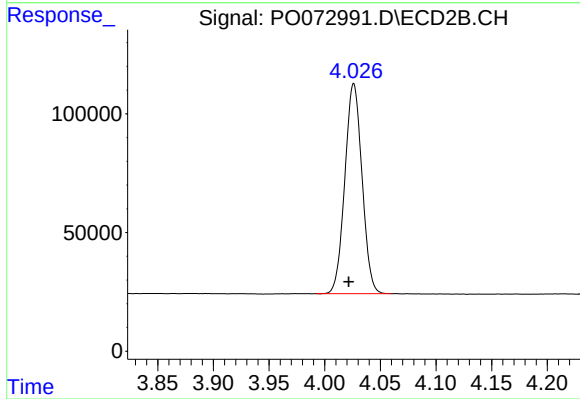


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.005 min
Response: 949924
Conc: 27.10 ng/ml

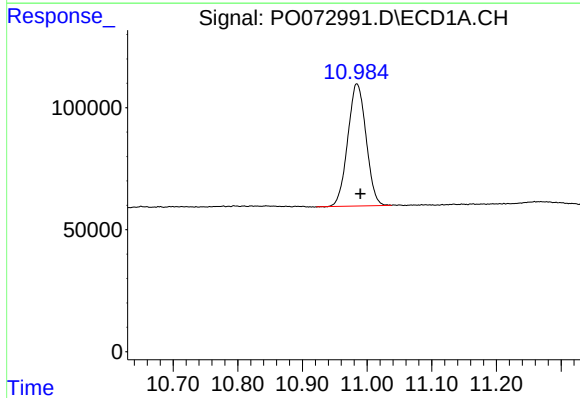


#2 Decachlorobiphenyl

R.T.: 10.984 min
Delta R.T.: -0.005 min
Response: 986423
Conc: 26.70 ng/ml

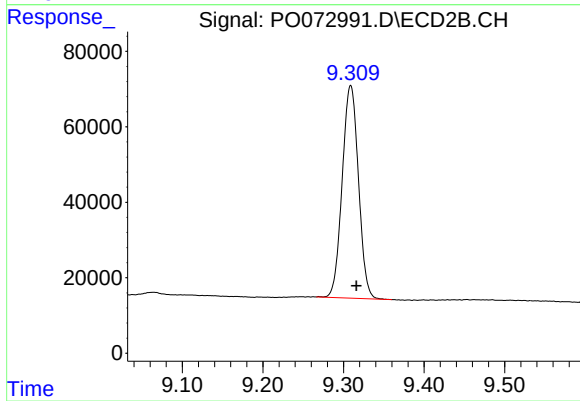

#2 Decachlorobiphenyl

R.T.: 9.309 min
Delta R.T.: -0.007 min
Response: 790494
Conc: 23.70 ng/ml

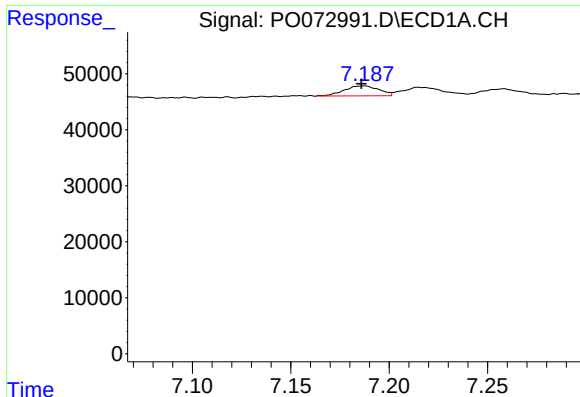


#26 AR-1254-1

R.T.: 7.187 min
Delta R.T.: 0.002 min
Response: 21774
Conc: 12.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MW-PIER-S


Manual Integrations
APPROVED

Ankita
11/3/2020 3:33:36 PM

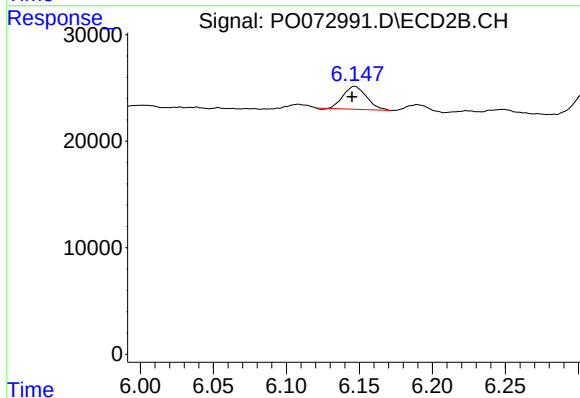


#26 AR-1254-1

R.T.: 6.147 min
Delta R.T.: 0.002 min
Response: 24034
Conc: 10.68 ng/ml

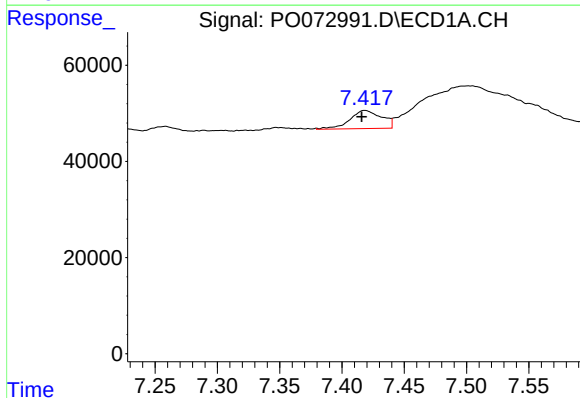


#27 AR-1254-2

R.T.: 7.417 min
Delta R.T.: 0.001 min
Response: 67161
Conc: 25.14 ng/ml m

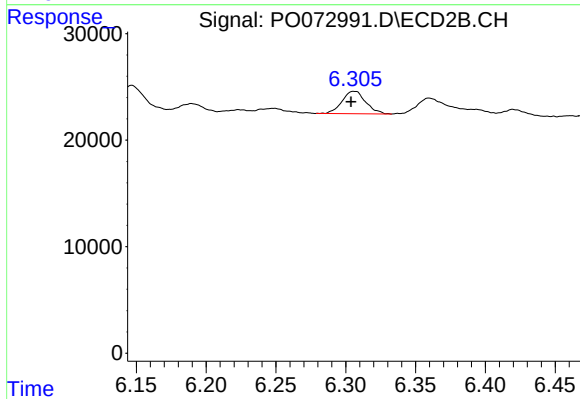

#27 AR-1254-2

R.T.: 6.306 min
Delta R.T.: 0.002 min
Response: 24754
Conc: 12.32 ng/ml

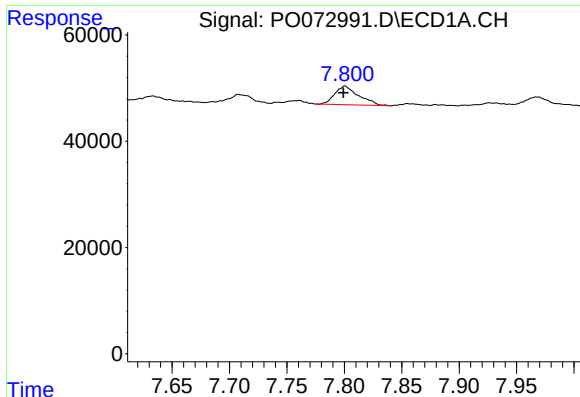


#28 AR-1254-3

R.T.: 7.801 min
Delta R.T.: 0.001 min
Response: 50895
Conc: 18.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-PIER-S


Manual Integrations
APPROVED

Ankita
11/3/2020 3:33:36 PM

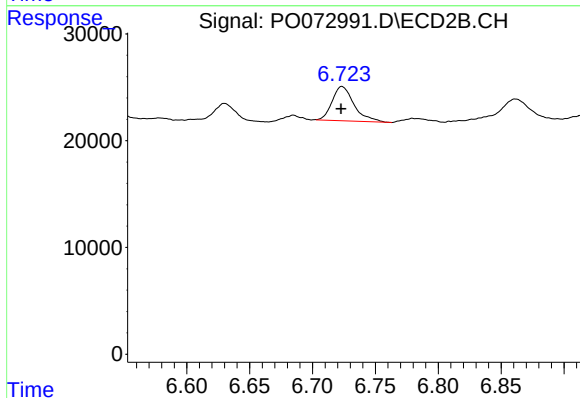


#28 AR-1254-3

R.T.: 6.723 min
Delta R.T.: 0.000 min
Response: 39150
Conc: 12.32 ng/ml

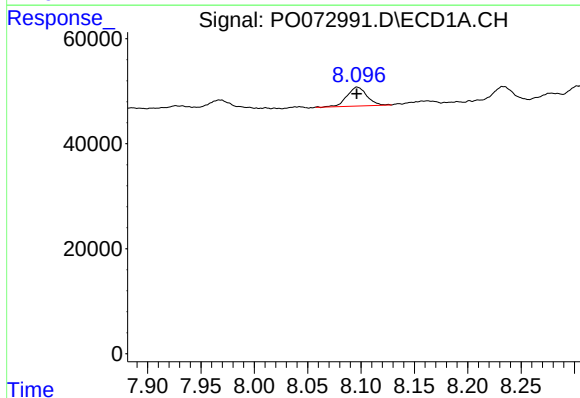


#29 AR-1254-4

R.T.: 8.097 min
Delta R.T.: 0.000 min
Response: 46778
Conc: 21.35 ng/ml

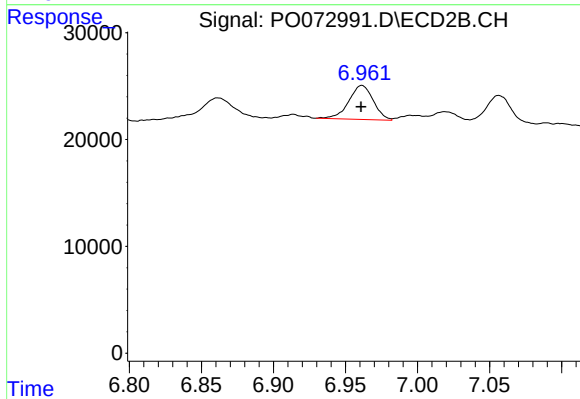

#29 AR-1254-4

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 37826
Conc: 17.39 ng/ml

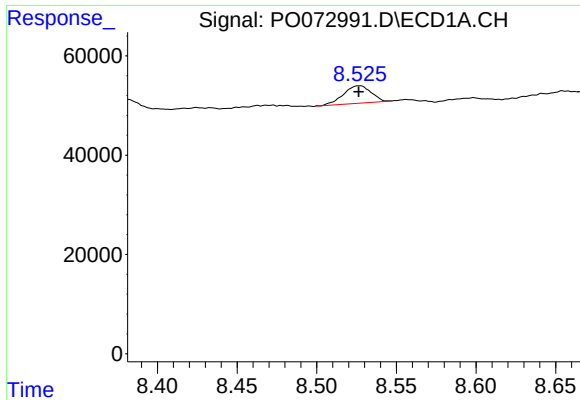


#30 AR-1254-5

R.T.: 8.527 min
Delta R.T.: 0.000 min
Response: 42214
Conc: 19.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-PIER-S

Manual Integrations
APPROVED

Ankita
11/3/2020 3:33:36 PM

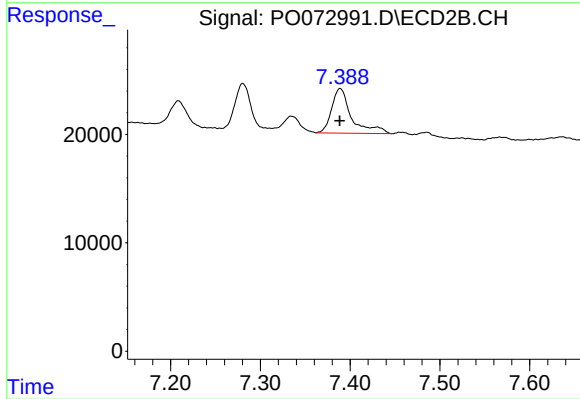

#30 AR-1254-5

R.T.: 7.389 min
Delta R.T.: 0.000 min
Response: 63328
Conc: 22.75 ng/ml