

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110220\
 Data File : PO072992.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2020 20:24
 Operator : DD\AJ
 Sample : L4570-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-FOUND-T1

Manual Integrations
 APPROVED

Ankita
 11/3/2020 3:33:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 03:45:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.950	4.028	1197853	788726	25.980	22.505
2) SA Decachlor...	10.985	9.309	983424	790267	26.619	23.697

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110220\
Data File : PO072992.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2020 20:24
Operator : DD\AJ
Sample : L4570-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MW-FOUND-T1


Manual Integrations
APPROVED

Ankita
11/3/2020 3:33:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 03:45:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

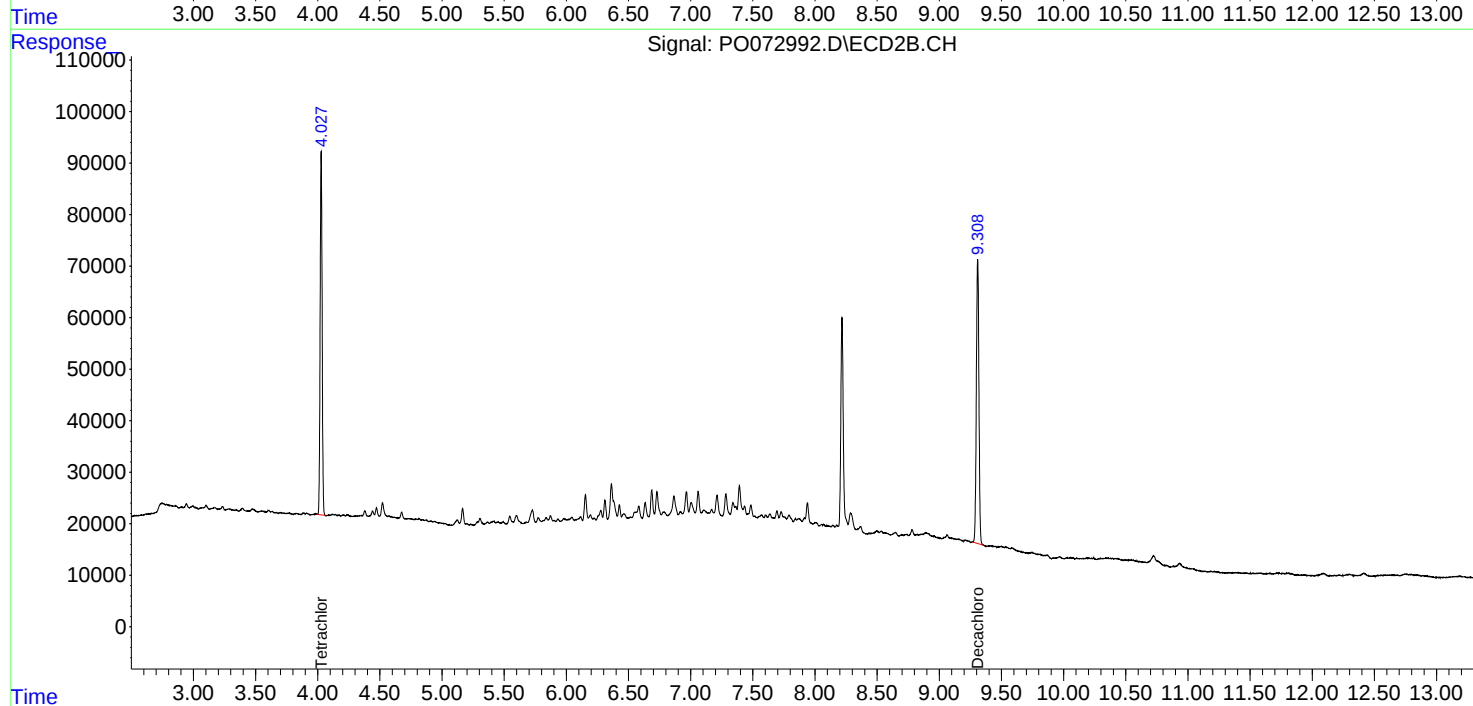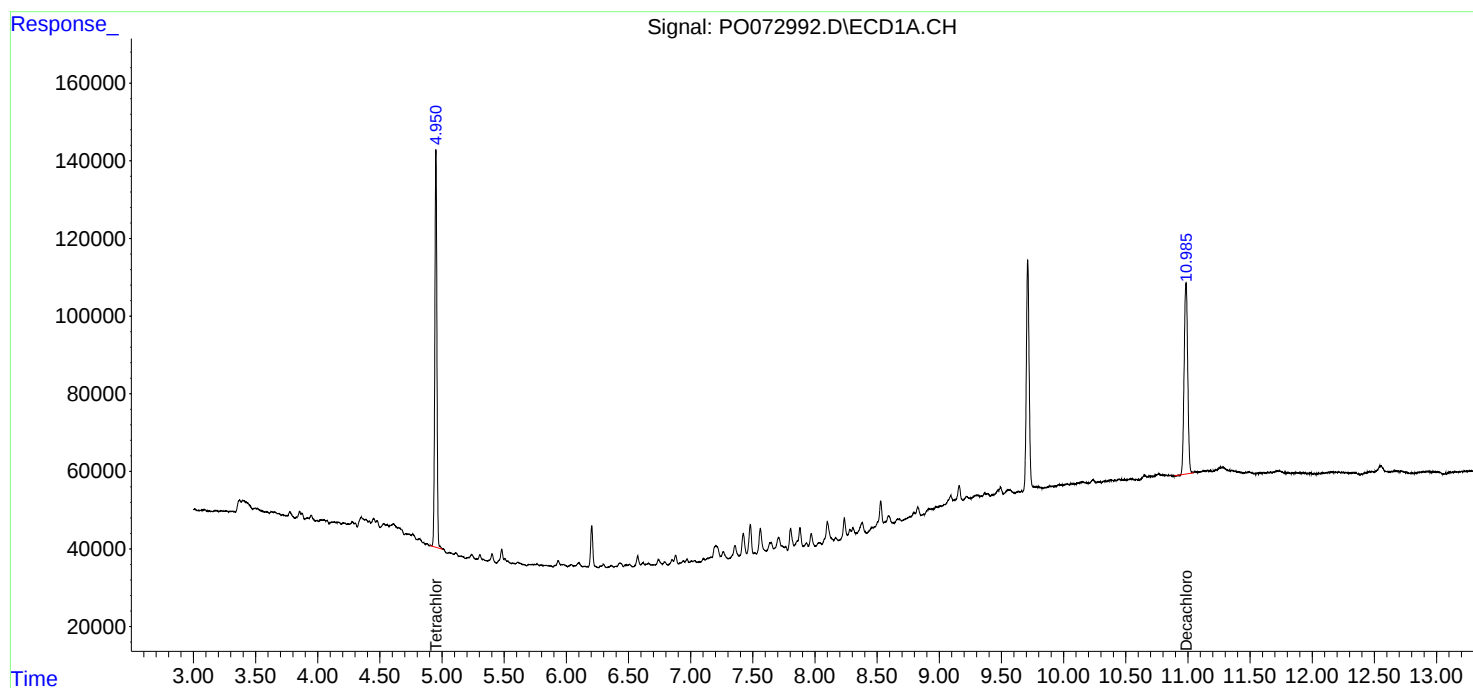

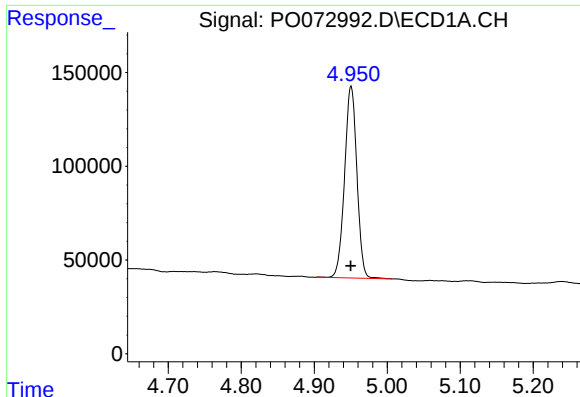


#1 Tetrachloro-m-xylene

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 1197853
Conc: 25.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-FOUND-T1


Manual Integrations
APPROVED

Ankita
11/3/2020 3:33:38 PM

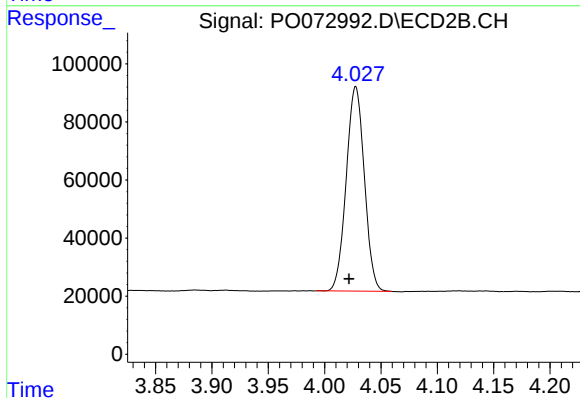


#1 Tetrachloro-m-xylene

R.T.: 4.028 min
Delta R.T.: 0.006 min
Response: 788726
Conc: 22.50 ng/ml

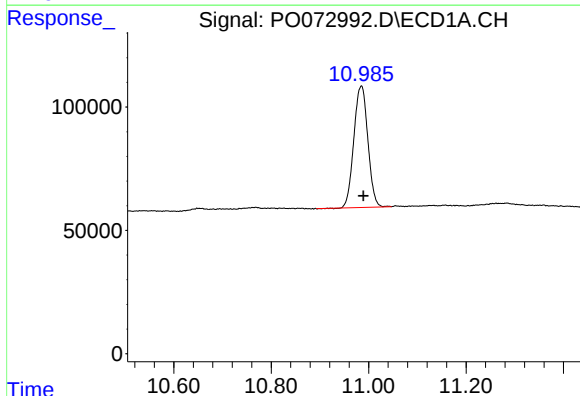

#2 Decachlorobiphenyl

R.T.: 10.985 min
Delta R.T.: -0.004 min
Response: 983424
Conc: 26.62 ng/ml

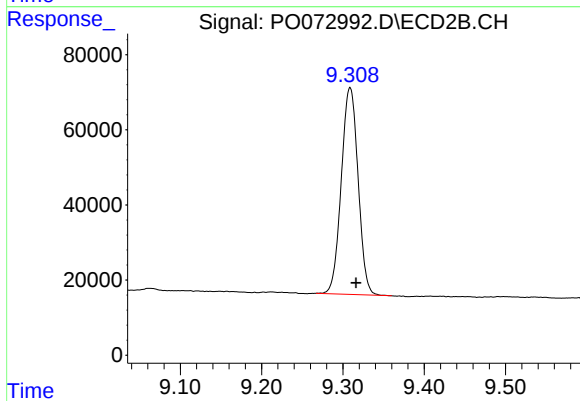

#2 Decachlorobiphenyl

R.T.: 9.309 min
Delta R.T.: -0.007 min
Response: 790267
Conc: 23.70 ng/ml