

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110221\
 Data File : PO082413.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2021 11:29
 Operator : AJ\MA
 Sample : M4427-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FDR-BH-6-20211029-7.5-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:34:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 29 11:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.972	3.969	1018339	368077	12.603	12.475
2) SA Decachlor...	11.079f	9.287	550900	250177	9.912	9.822

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110221\
Data File : PO082413.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2021 11:29
Operator : AJ\MA
Sample : M4427-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FDR-BH-6-20211029-7.5-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:34:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

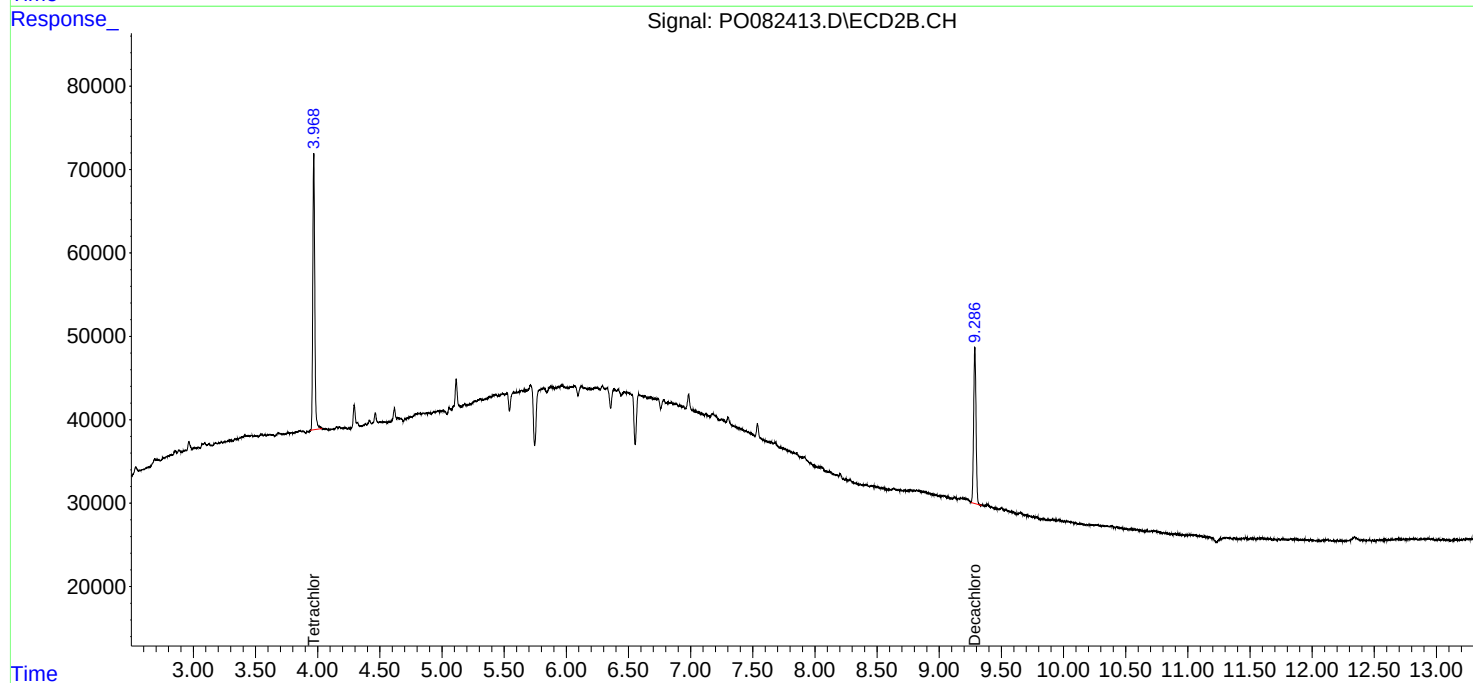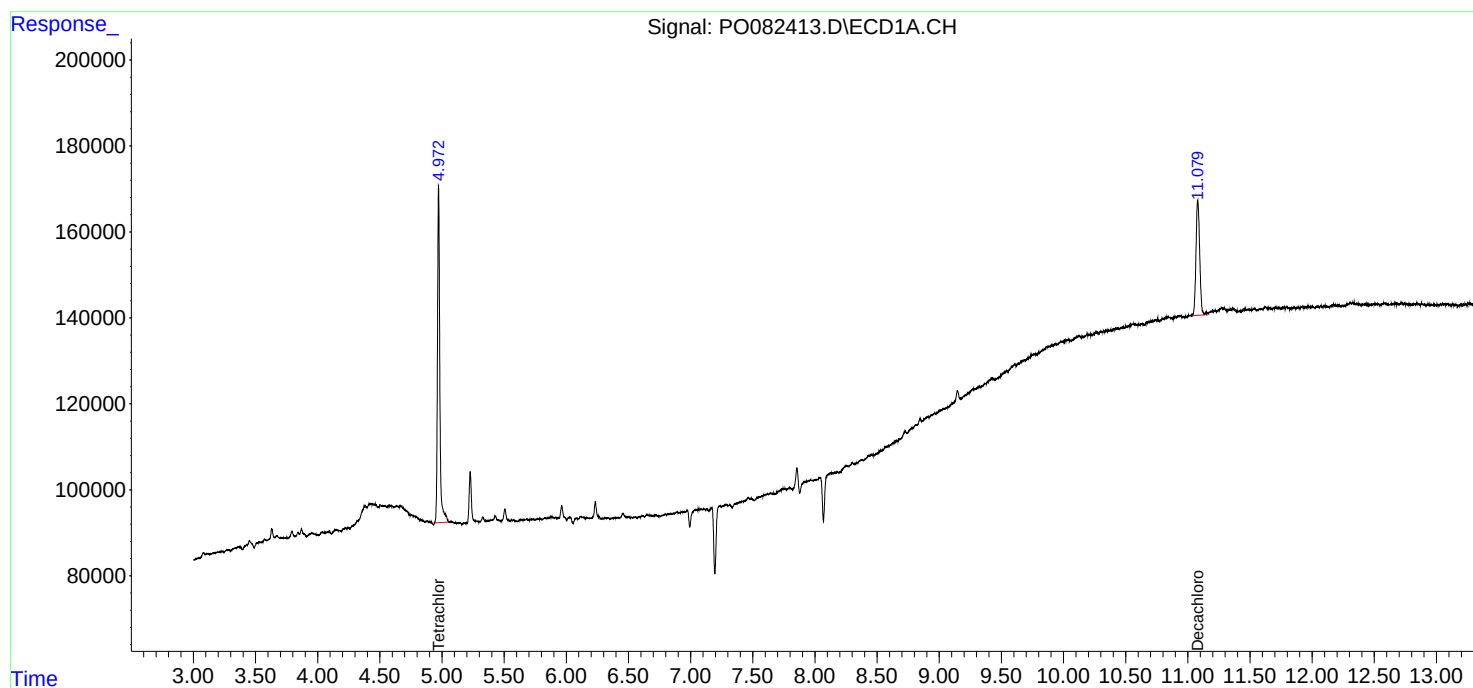


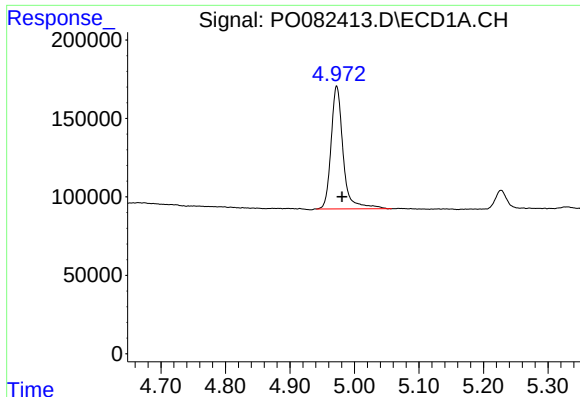

#1 Tetrachloro-m-xylene


R.T.: 4.972 min
Delta R.T.: -0.009 min
Response: 1018339
Conc: 12.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDR-BH-6-20211029-7.5-8

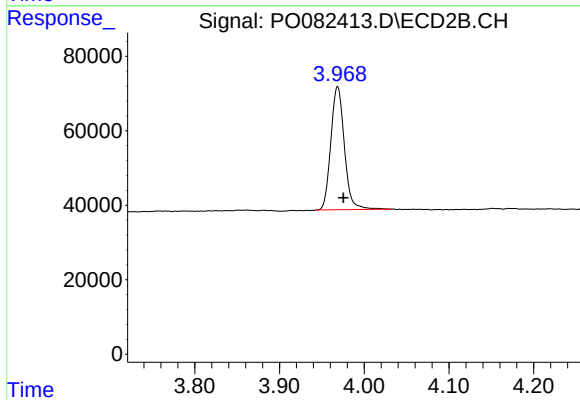


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.007 min
Response: 368077
Conc: 12.48 ng/ml

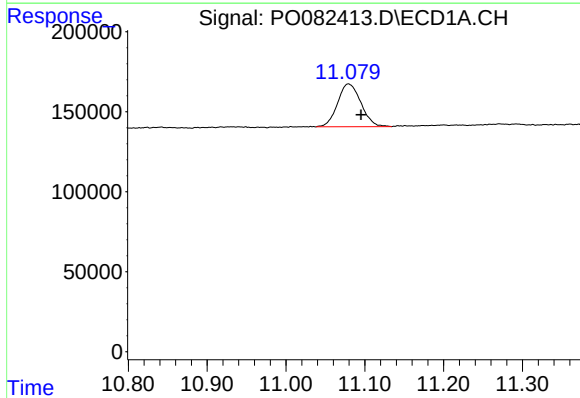

#2 Decachlorobiphenyl

R.T.: 11.079 min
Delta R.T.: -0.016 min
Response: 550900
Conc: 9.91 ng/ml

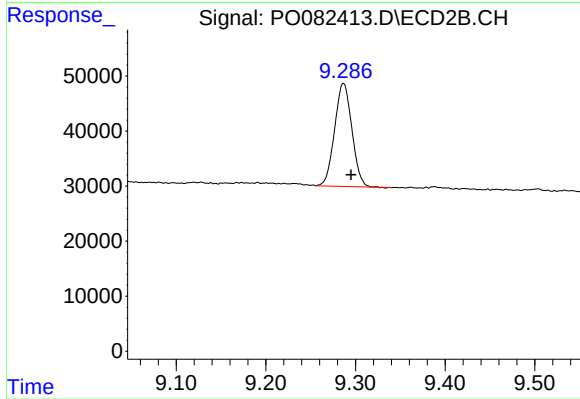

#2 Decachlorobiphenyl

R.T.: 9.287 min
Delta R.T.: -0.008 min
Response: 250177
Conc: 9.82 ng/ml