

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO110221\  
 Data File : PO082416.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Nov 2021 12:21  
 Operator : AJ\MA  
 Sample : M4427-04  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 FDR-BH-4-20211029-7.5-8M

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 03 01:35:52 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO101821.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Oct 29 11:08:21 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|--------|--------|--------|
| -----                       |        |       |         |        |        |        |
| System Monitoring Compounds |        |       |         |        |        |        |
| 1) SA Tetrachlo...          | 4.974  | 3.971 | 1599037 | 576769 | 19.789 | 19.549 |
| 2) SA Decachlor...          | 11.084 | 9.288 | 1437697 | 546446 | 25.868 | 21.454 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO110221\  
Data File : PO082416.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Nov 2021 12:21  
Operator : AJ\MA  
Sample : M4427-04  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
FDR-BH-4-20211029-7.5-8M

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 03 01:35:52 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO101821.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Oct 29 11:08:21 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

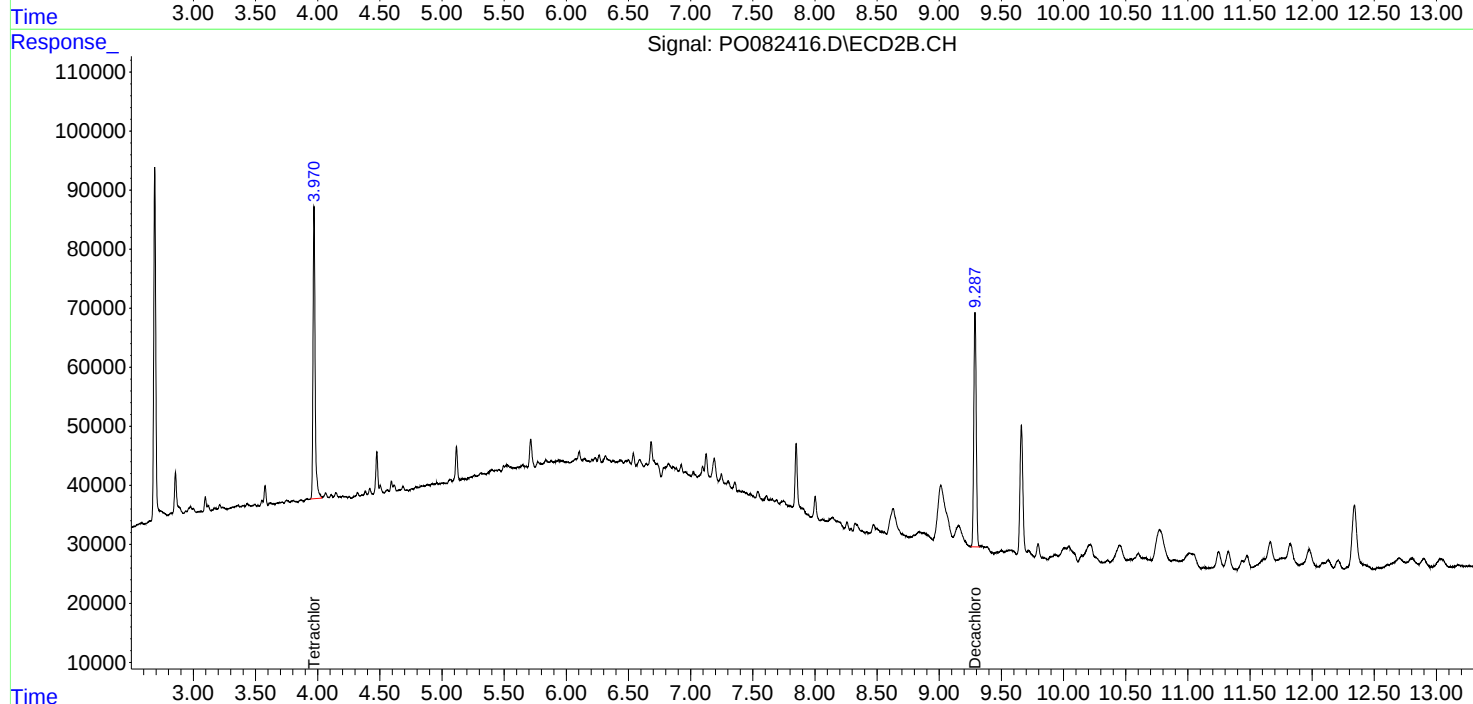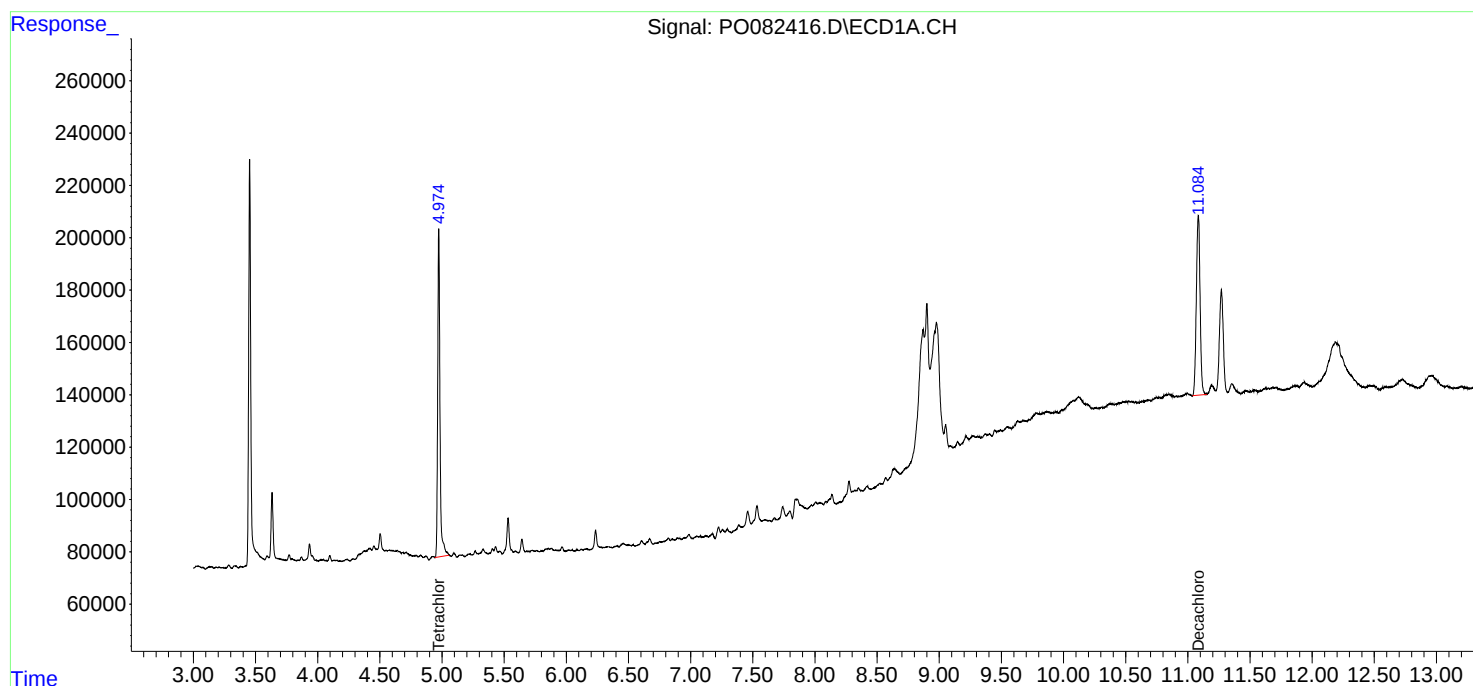


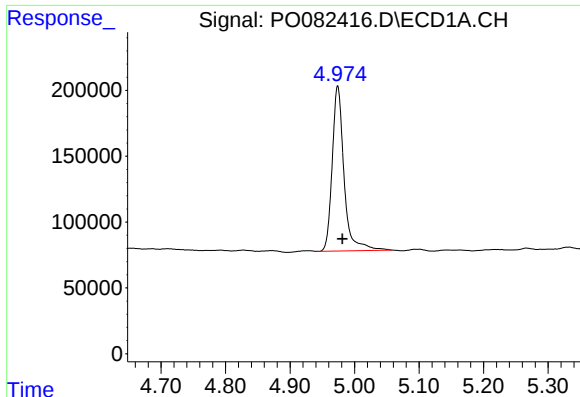

#1 Tetrachloro-m-xylene


R.T.: 4.974 min  
Delta R.T.: -0.007 min  
Response: 1599037  
Conc: 19.79 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
FDR-BH-4-20211029-7.5-8M

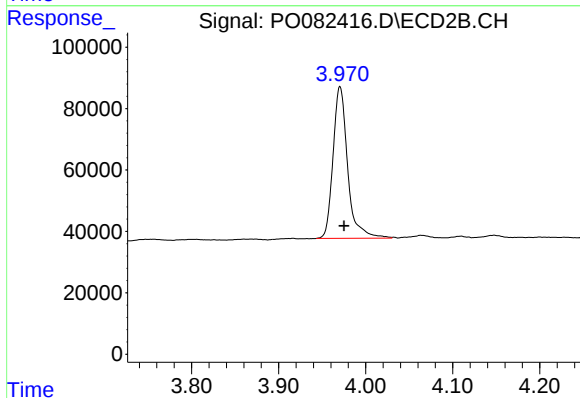


#1 Tetrachloro-m-xylene

R.T.: 3.971 min  
Delta R.T.: -0.005 min  
Response: 576769  
Conc: 19.55 ng/ml

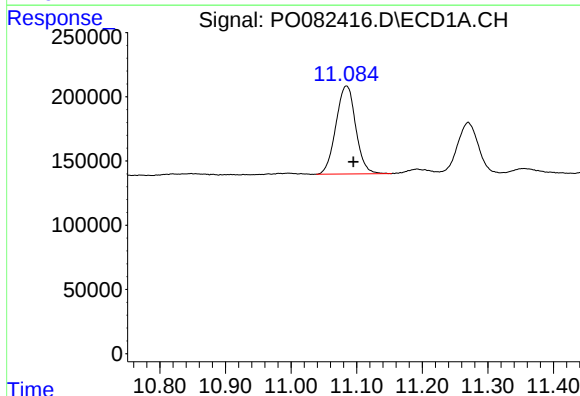

#2 Decachlorobiphenyl

R.T.: 11.084 min  
Delta R.T.: -0.011 min  
Response: 1437697  
Conc: 25.87 ng/ml

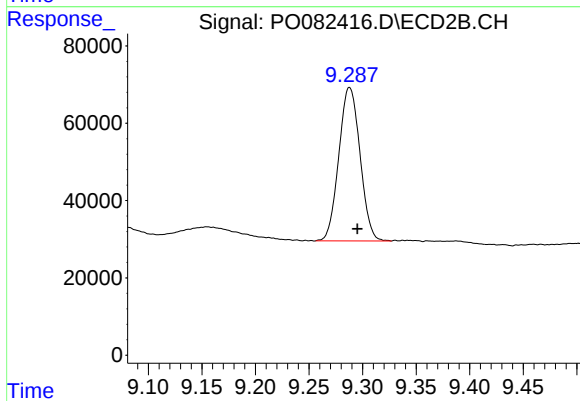

#2 Decachlorobiphenyl

R.T.: 9.288 min  
Delta R.T.: -0.007 min  
Response: 546446  
Conc: 21.45 ng/ml