

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110221\
 Data File : PO082419.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2021 13:13
 Operator : AJ\MA
 Sample : M4427-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FDR-BH-3-20211029-5-5.5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:37:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 29 11:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.974	3.970	1526520	524360	18.892	17.772
2) SA Decachlor...	11.085	9.289	1506167	539622	27.099	21.187

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110221\
Data File : PO082419.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2021 13:13
Operator : AJ\MA
Sample : M4427-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FDR-BH-3-20211029-5-5.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:37:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

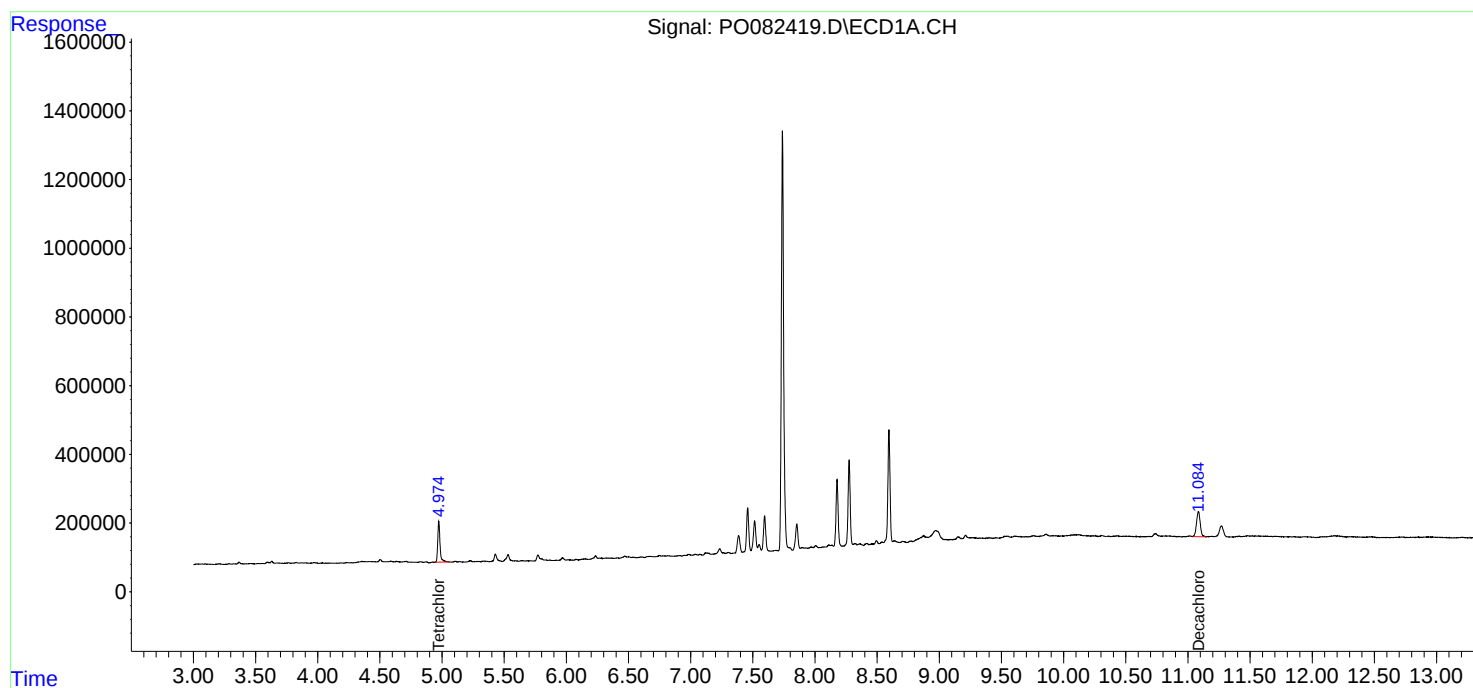


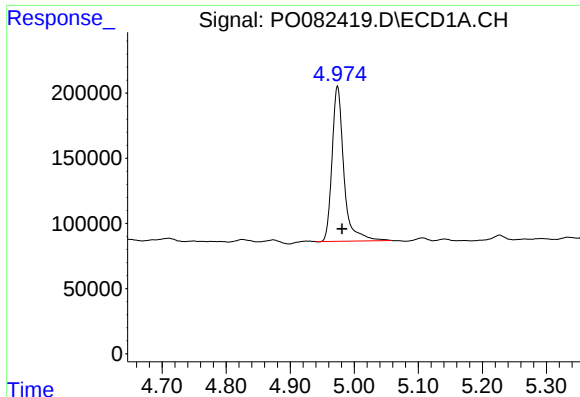

#1 Tetrachloro-m-xylene


R.T.: 4.974 min
Delta R.T.: -0.007 min
Response: 1526520
Conc: 18.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDR-BH-3-20211029-5-5.5

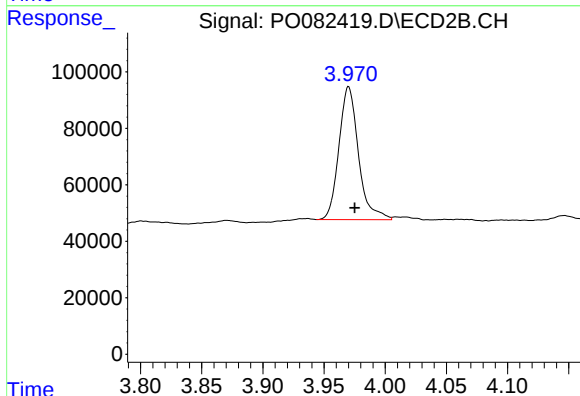


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: -0.005 min
Response: 524360
Conc: 17.77 ng/ml

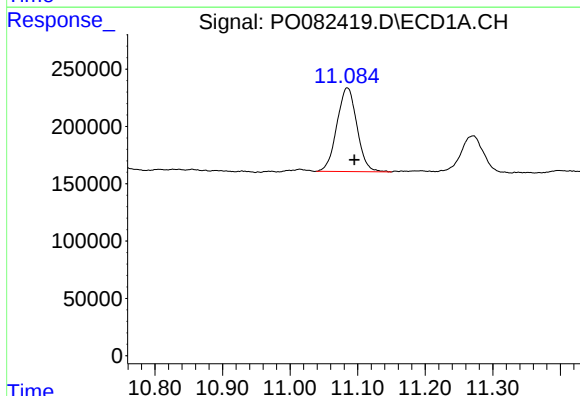

#2 Decachlorobiphenyl

R.T.: 11.085 min
Delta R.T.: -0.010 min
Response: 1506167
Conc: 27.10 ng/ml

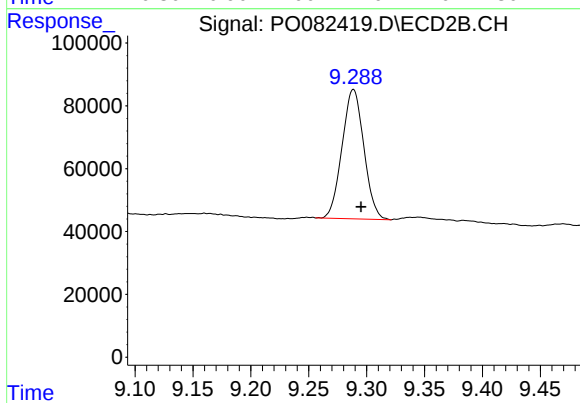

#2 Decachlorobiphenyl

R.T.: 9.289 min
Delta R.T.: -0.006 min
Response: 539622
Conc: 21.19 ng/ml