

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110221\
Data File : PO082422.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2021 14:48
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:39:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.982	3.969	1834789	654619	22.707	22.187
2)	SA Decachlor...	11.094	9.289	1364680	597329	24.554	23.452

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110221\
Data File : PO082422.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2021 14:48
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:39:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

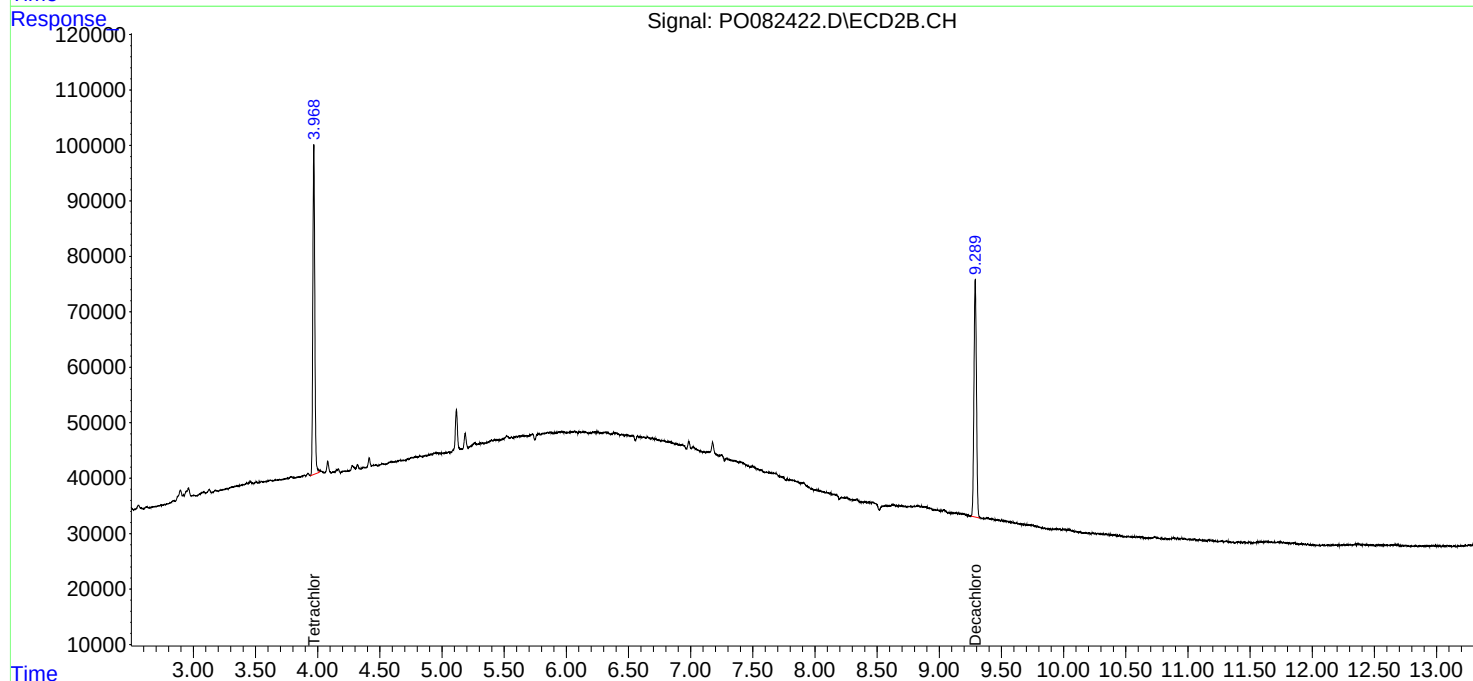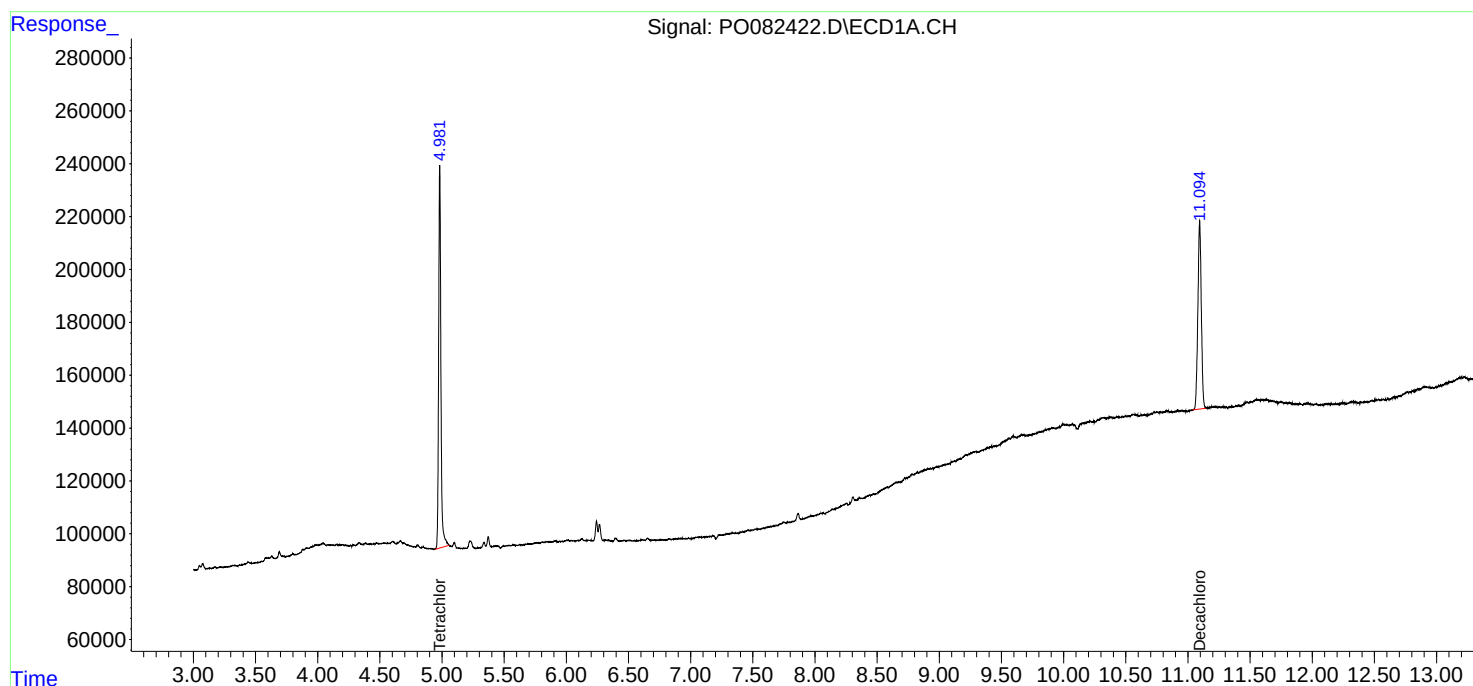


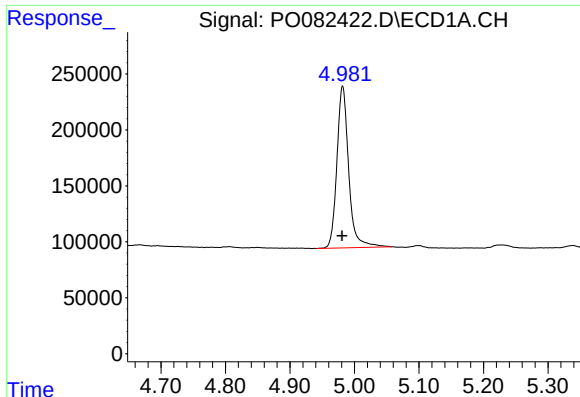

#1 Tetrachloro-m-xylene


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 1834789
Conc: 22.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

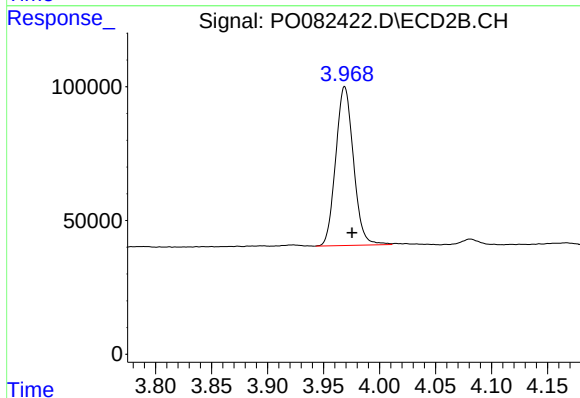


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.006 min
Response: 654619
Conc: 22.19 ng/ml

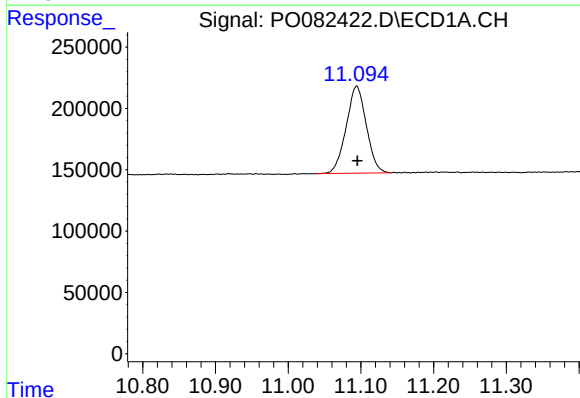

#2 Decachlorobiphenyl

R.T.: 11.094 min
Delta R.T.: 0.000 min
Response: 1364680
Conc: 24.55 ng/ml

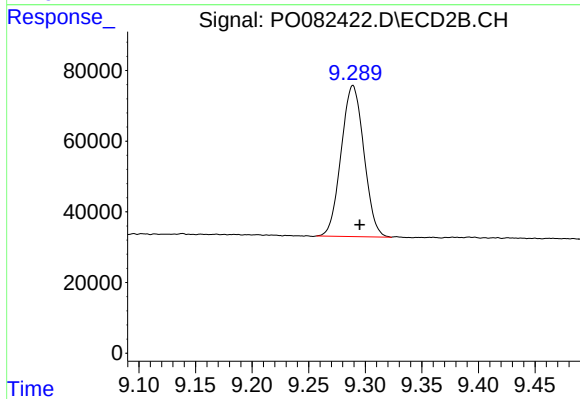

#2 Decachlorobiphenyl

R.T.: 9.289 min
Delta R.T.: -0.006 min
Response: 597329
Conc: 23.45 ng/ml