

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110320\
 Data File : PO073026.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2020 17:01
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 05:00:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.947	4.022	972408	670949	21.090	19.144
2)	SA Decachlor...	10.979	9.302	885608	705824	23.971	21.165
Target Compounds							
20)	L4 AR-1242-5	7.213f	0.000	182435	0	178.098	N.D. #
24)	L5 AR-1248-4	7.213	0.000	182435	0	101.020	N.D. #
26)	L6 AR-1254-1	7.213f	0.000	182435	0	105.269	N.D. #
34)	L7 AR-1260-4	8.836	0.000	159532	0	79.862	N.D. #
38)	L8 AR-1262-3	0.000	8.231	0	394039	N.D.	215.339 #
40)	L8 AR-1262-5	0.000	8.764f	0	118351	N.D.	72.274 #
41)	L9 AR-1268-1	0.000	8.231	0	394039	N.D.	66.082 #
43)	L9 AR-1268-3	0.000	8.526f	0	186258	N.D.	38.210 #
44)	L9 AR-1268-4	0.000	8.764f	0	118351	N.D.	54.203 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110320\
Data File : PO073026.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2020 17:01
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:00:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

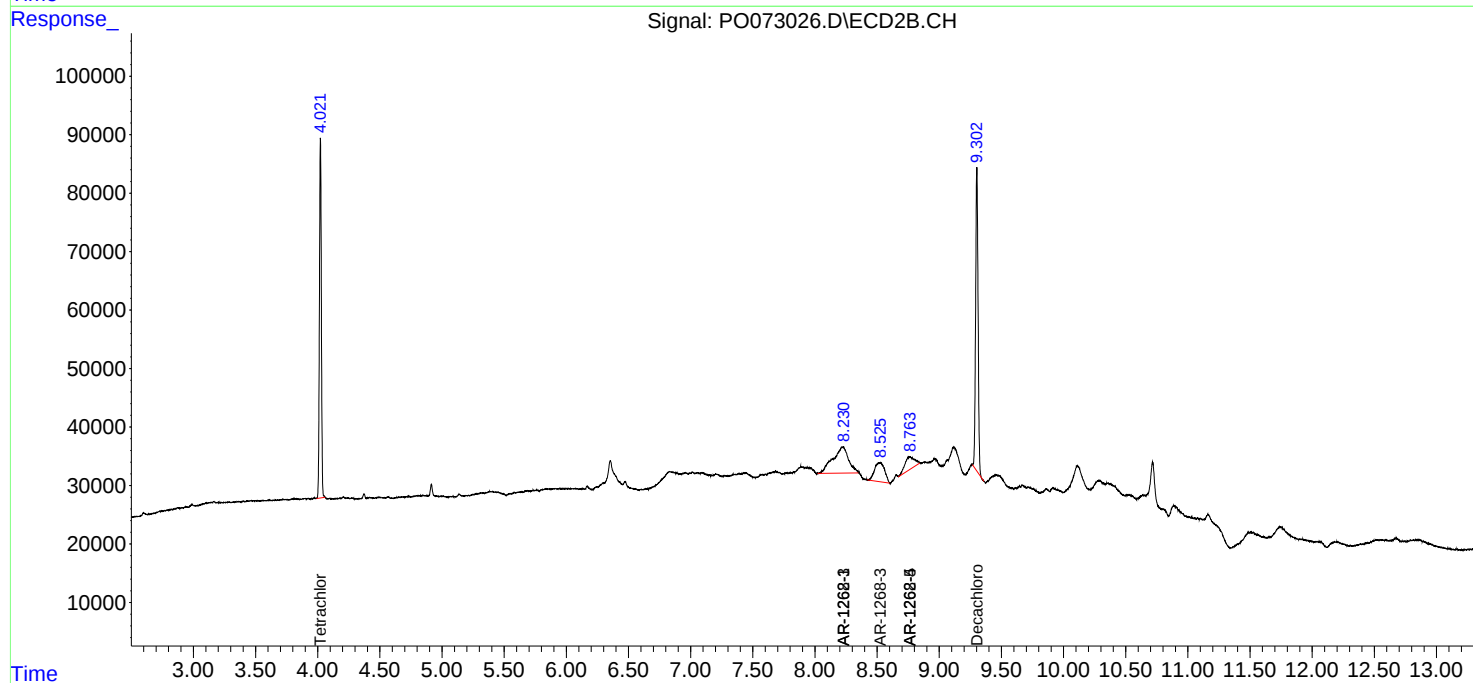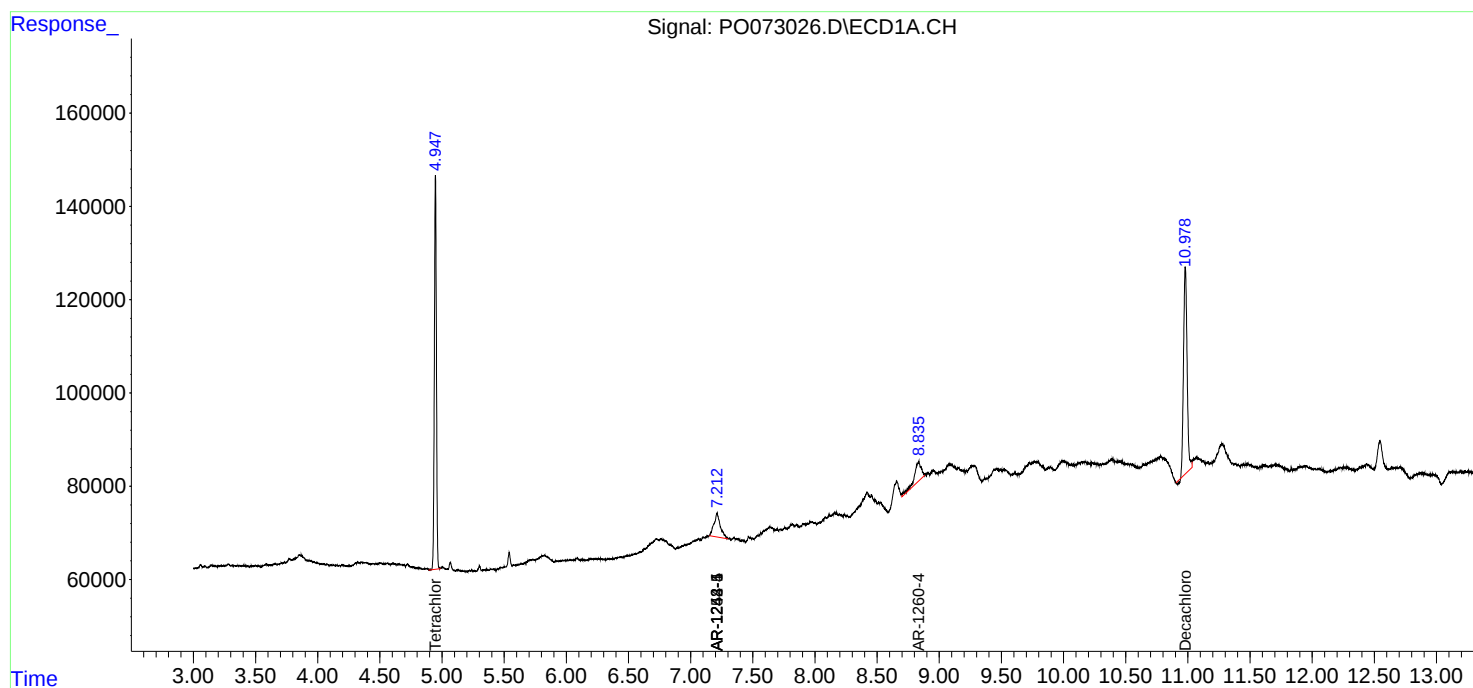

Response_

Signal: PO073026.D\ECD1A.CH

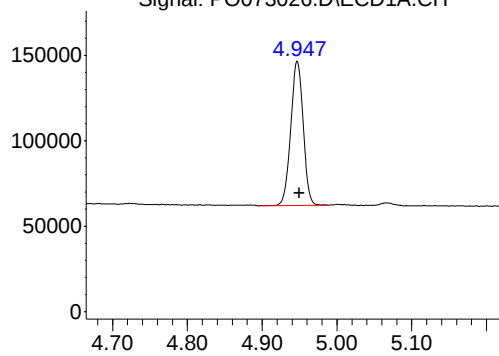

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: -0.003 min
Response: 972408
Conc: 21.09 ng/ml

Instrument :
ECD_O
ClientSampleId :

Time

Response_

Signal: PO073026.D\ECD2B.CH

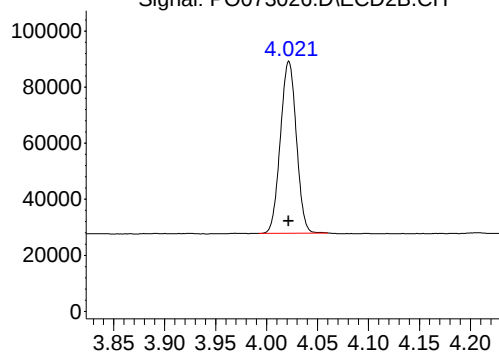

#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 670949
Conc: 19.14 ng/ml

Time