

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110320\
 Data File : PO073029.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2020 17:52
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 05:46:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.948	4.022	1012619	679398	21.963	19.385
2) SA Decachlor...	10.980	9.304	938347	779797	25.398	23.383
Target Compounds						
43) L9 AR-1268-3	9.787	0.000	139837	0	25.102	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110320\
Data File : PO073029.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2020 17:52
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:46:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

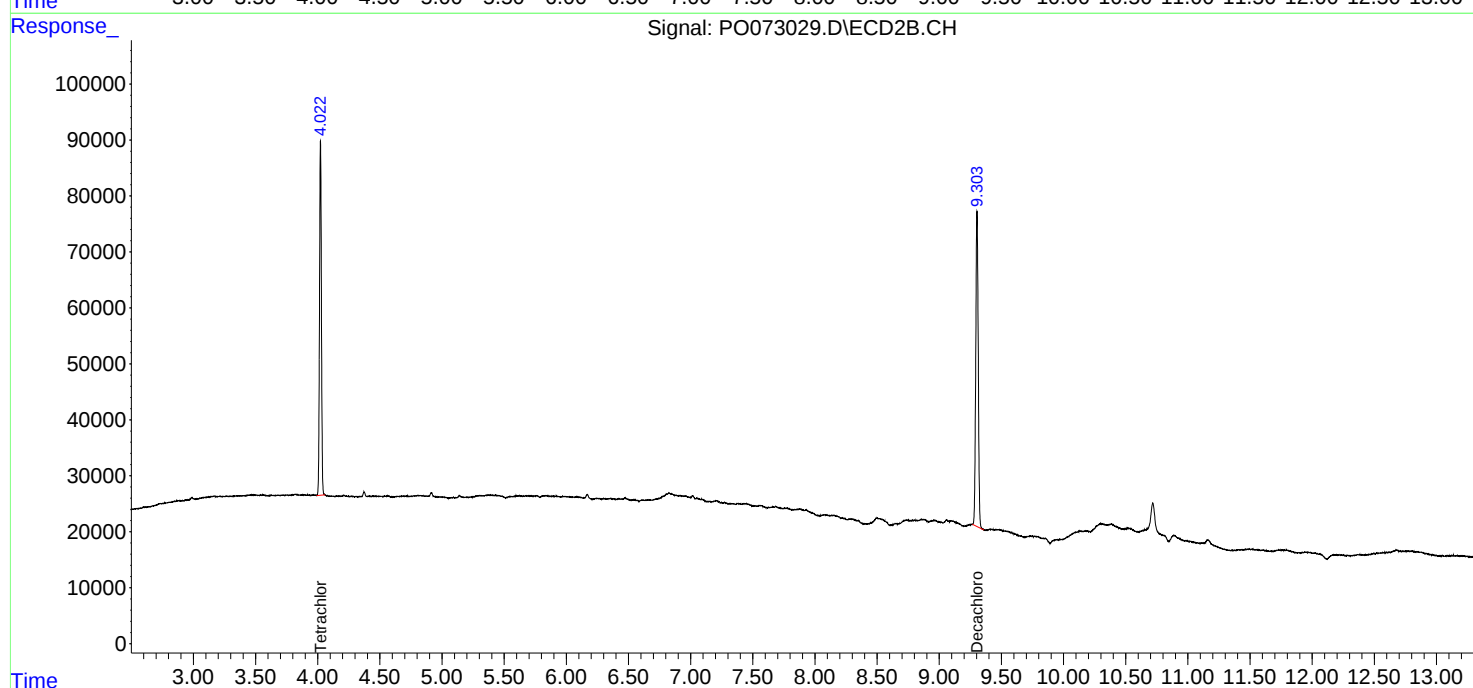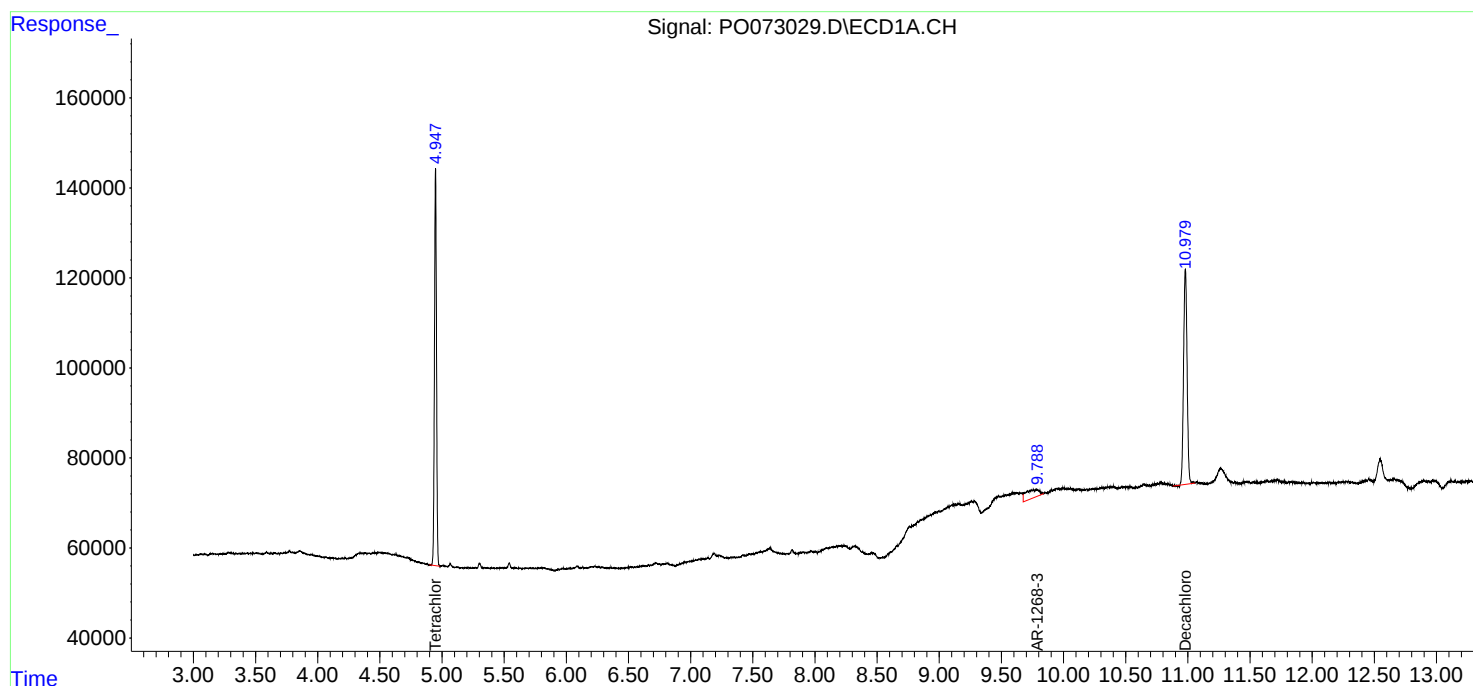


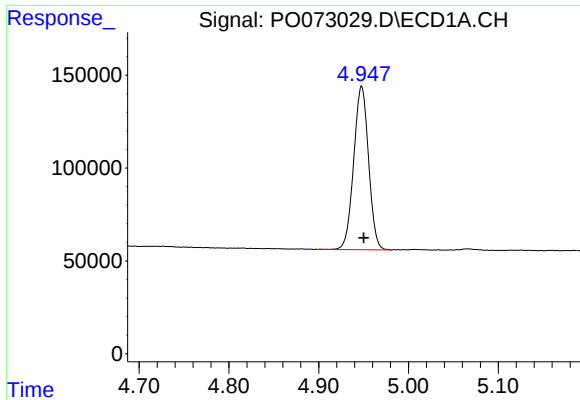

#1 Tetrachloro-m-xylene


R.T.: 4.948 min
Delta R.T.: -0.002 min
Response: 1012619
Conc: 21.96 ng/ml

Instrument :
ECD_O
ClientSampleId :

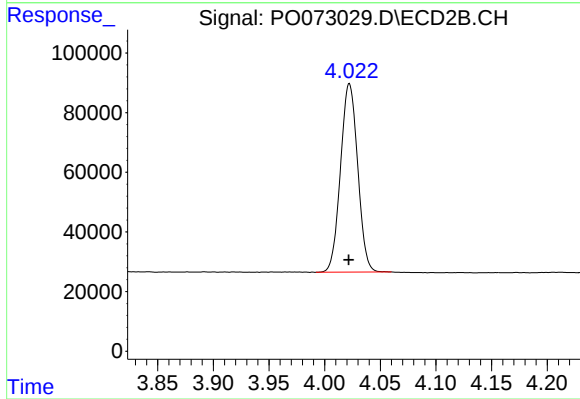


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 679398
Conc: 19.39 ng/ml

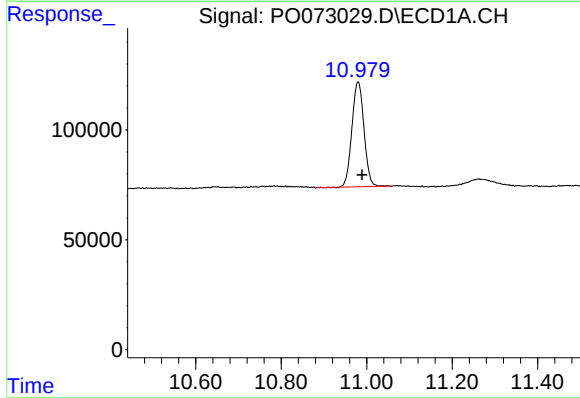


#2 Decachlorobiphenyl

R.T.: 10.980 min
Delta R.T.: -0.010 min
Response: 938347
Conc: 25.40 ng/ml

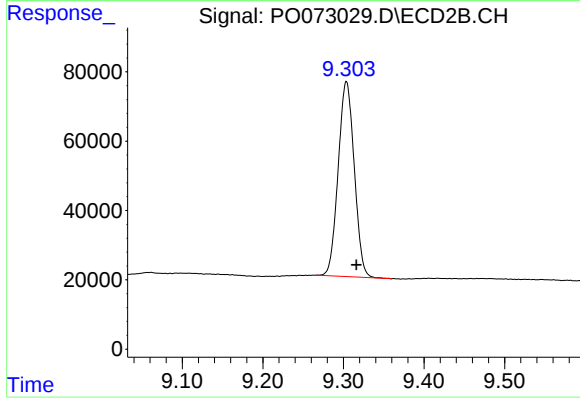

#2 Decachlorobiphenyl


R.T.: 9.304 min
Delta R.T.: -0.012 min
Response: 779797
Conc: 23.38 ng/ml

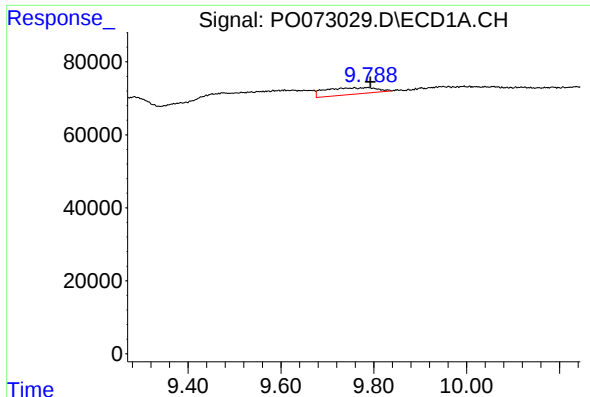

#43 AR-1268-3

R.T.: 9.787 min
Delta R.T.: -0.006 min
Response: 139837
Conc: 25.10 ng/ml

Instrument :
ECD_O
ClientSampleId :

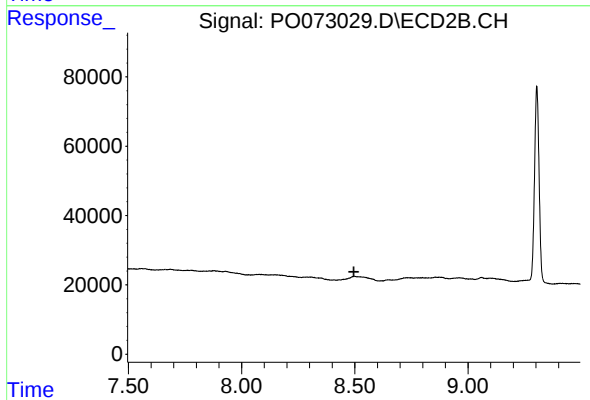

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.496 min
Response: 0
Conc: N.D.