

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO110320\  
 Data File : PO073021.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 03 Nov 2020 15:35  
 Operator : DD\AJ  
 Sample : L4573-01  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 OB-722-EB

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 04 04:56:00 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO102620.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Sat Oct 31 07:06:26 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|---------|--------|--------|
| -----                       |        |       |         |         |        |        |
| System Monitoring Compounds |        |       |         |         |        |        |
| 1) SA Tetrachlo...          | 4.949  | 4.024 | 1649398 | 1070794 | 35.774 | 30.553 |
| 2) SA Decachlor...          | 10.983 | 9.304 | 1073333 | 847313  | 29.052 | 25.408 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO110320\  
Data File : PO073021.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 03 Nov 2020 15:35  
Operator : DD\AJ  
Sample : L4573-01  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
OB-722-EB

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 04 04:56:00 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO102620.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Sat Oct 31 07:06:26 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

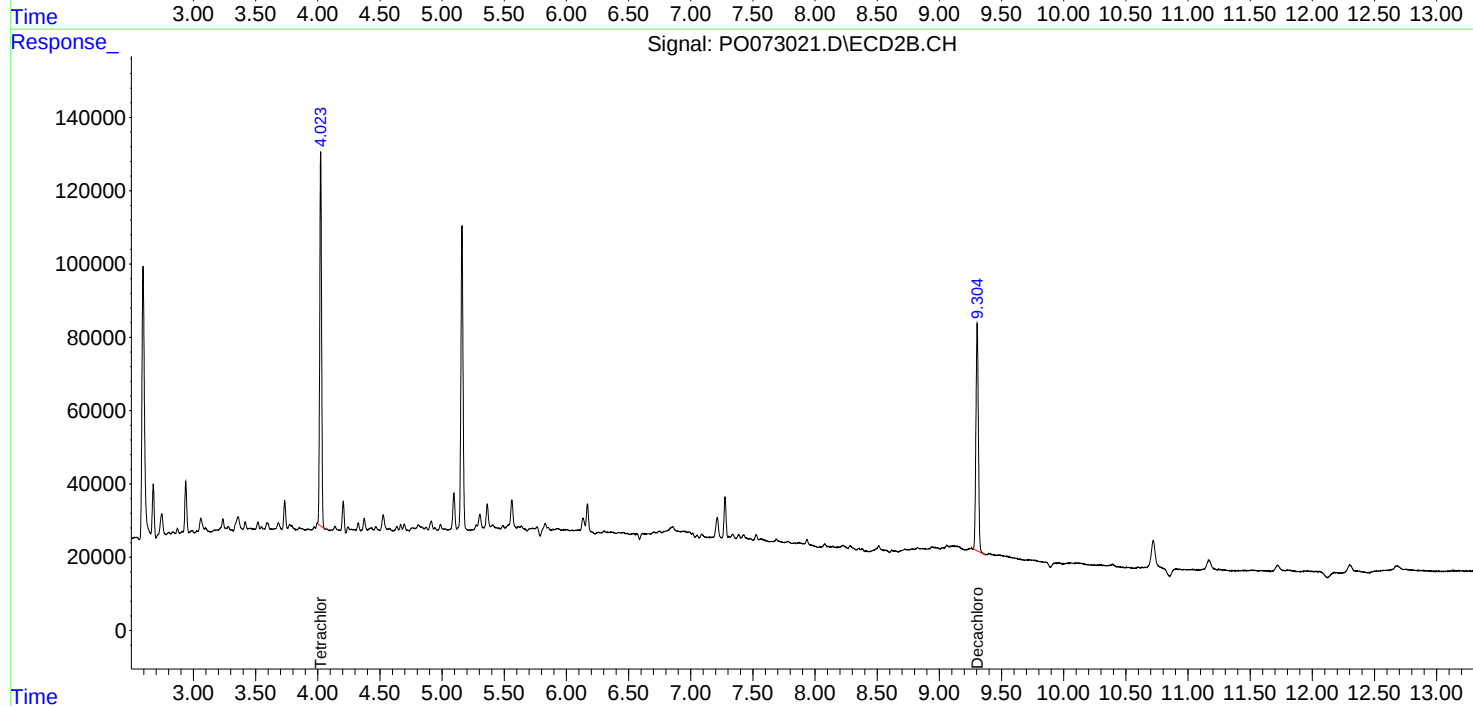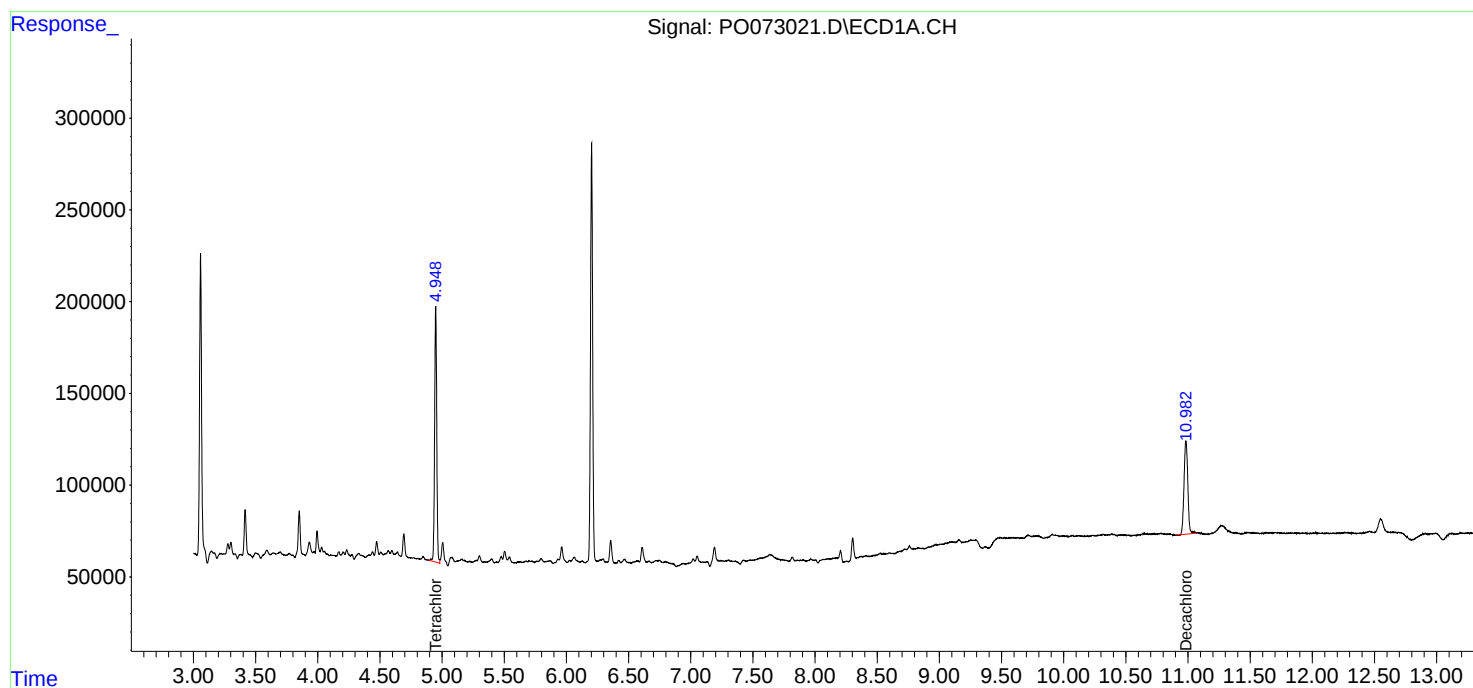


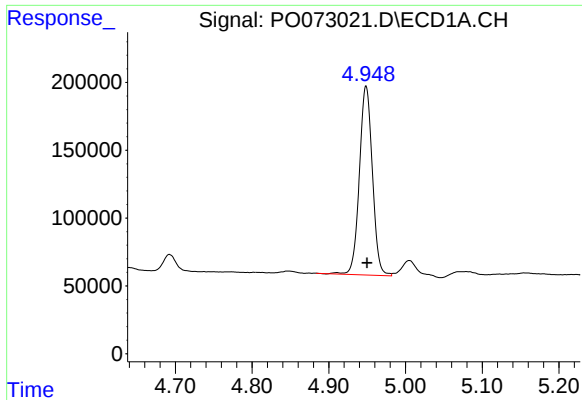

#1 Tetrachloro-m-xylene


R.T.: 4.949 min  
Delta R.T.: -0.001 min  
Response: 1649398  
Conc: 35.77 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
OB-722-EB

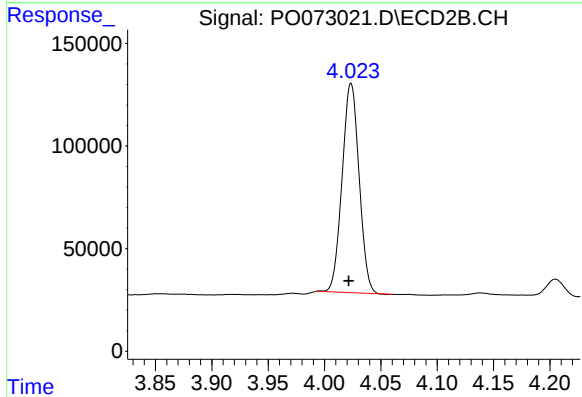


#1 Tetrachloro-m-xylene

R.T.: 4.024 min  
Delta R.T.: 0.002 min  
Response: 1070794  
Conc: 30.55 ng/ml

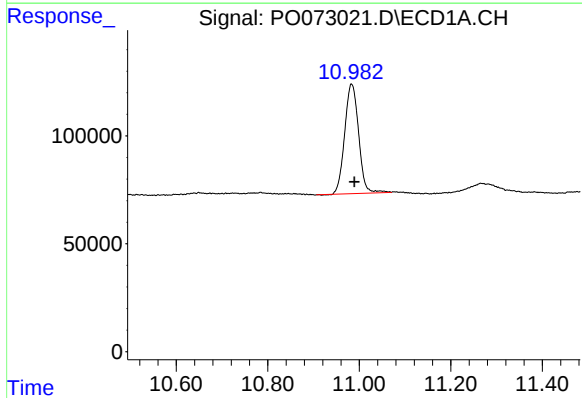

#2 Decachlorobiphenyl

R.T.: 10.983 min  
Delta R.T.: -0.006 min  
Response: 1073333  
Conc: 29.05 ng/ml

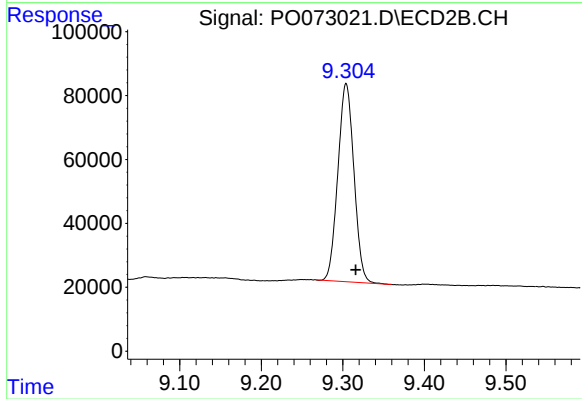

#2 Decachlorobiphenyl

R.T.: 9.304 min  
Delta R.T.: -0.012 min  
Response: 847313  
Conc: 25.41 ng/ml