

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110320\
 Data File : PO073043.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2020 21:51
 Operator : DD\AJ
 Sample : L4600-09
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CRT-19

Manual Integrations
 APPROVED

Ankita
 11/4/2020 4:58:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 05:50:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.947	4.021	1229213	802602	26.660	22.900
2) SA Decachlor...	10.976	9.300f	1064215	867590	28.805	26.016m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110320\
Data File : PO073043.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2020 21:51
Operator : DD\AJ
Sample : L4600-09
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CRT-19


Manual Integrations
APPROVED

Ankita
11/4/2020 4:58:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:50:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

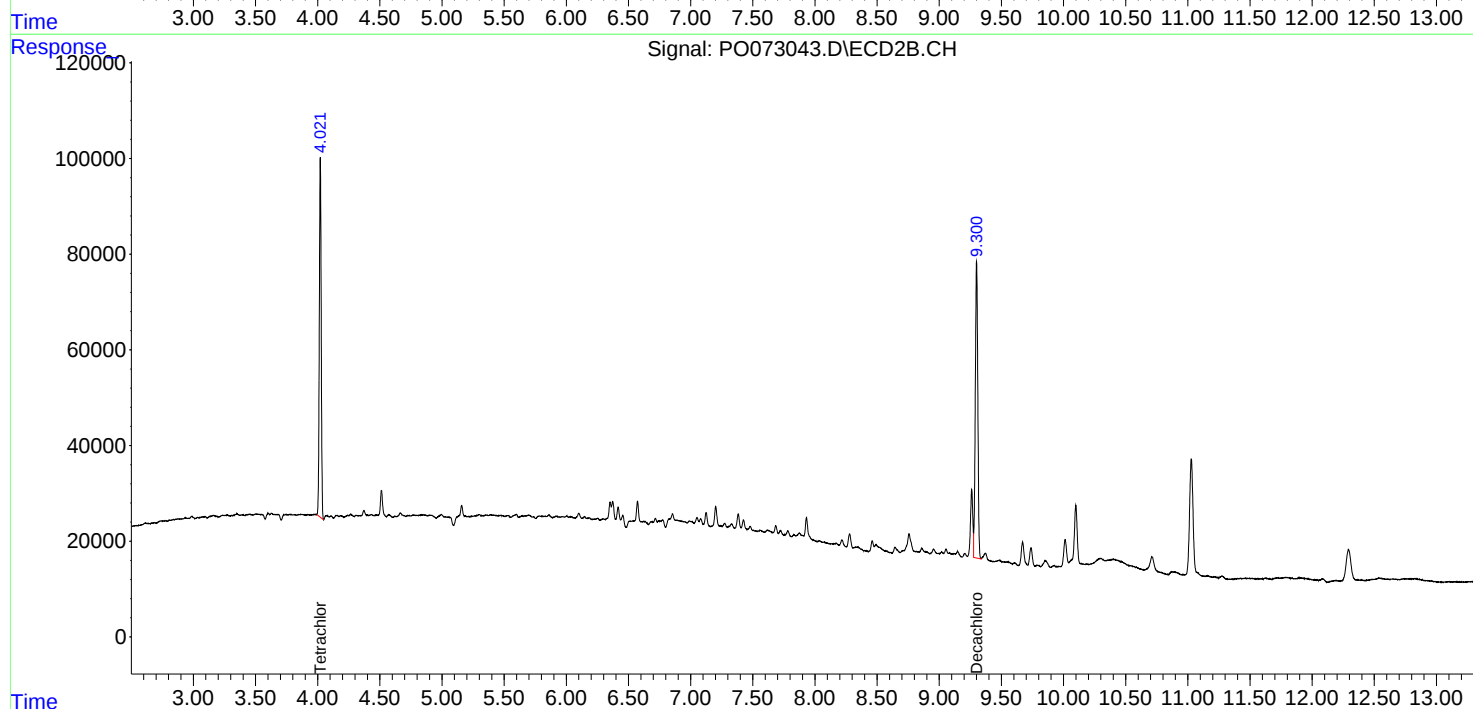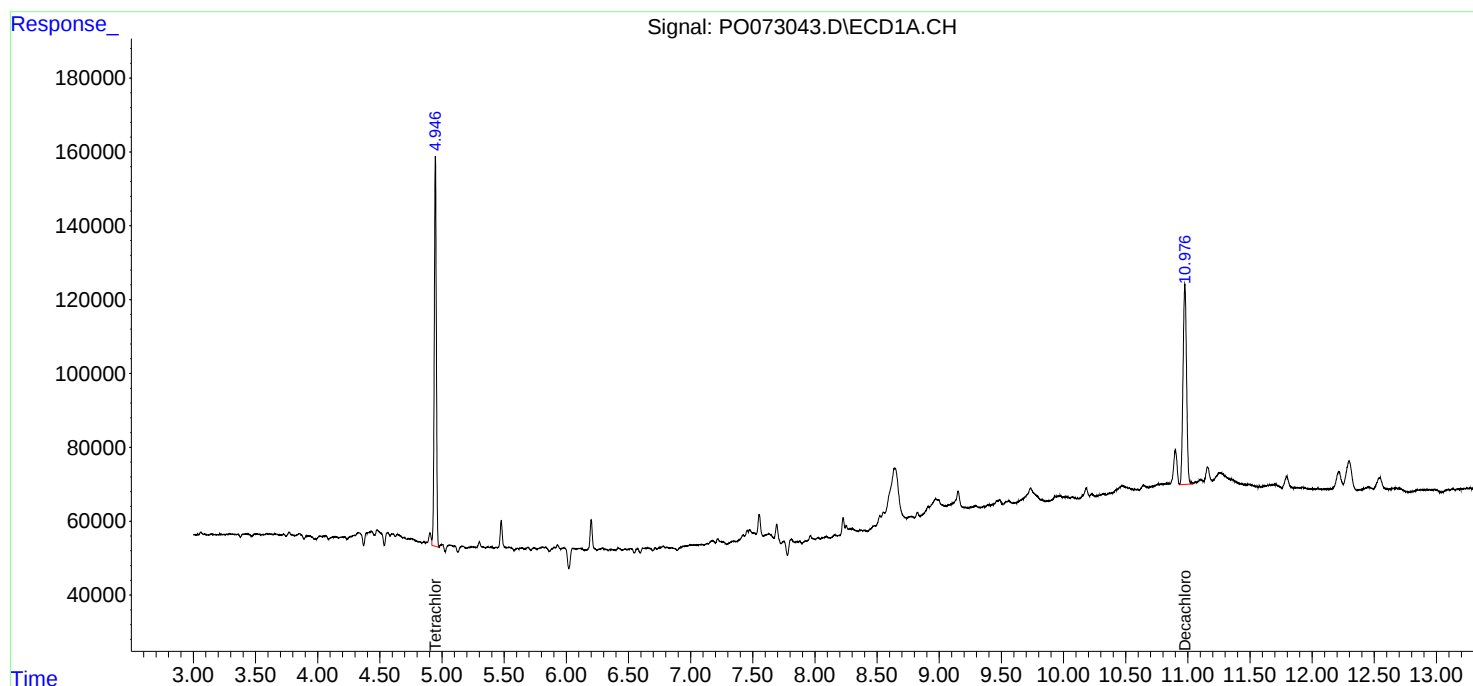

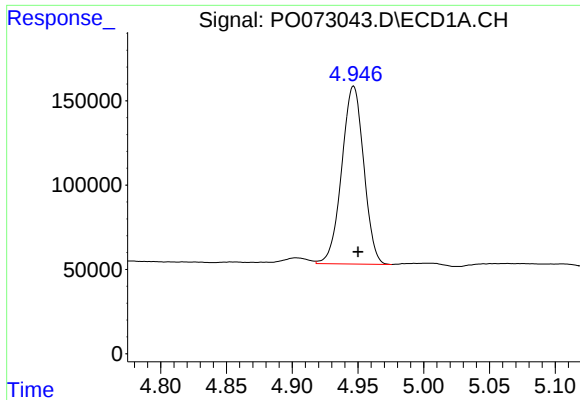


#1 Tetrachloro-m-xylene

R.T.: 4.947 min
Delta R.T.: -0.003 min
Response: 1229213
Conc: 26.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
CRT-19


Manual Integrations
APPROVED

Ankita
11/4/2020 4:58:39 PM

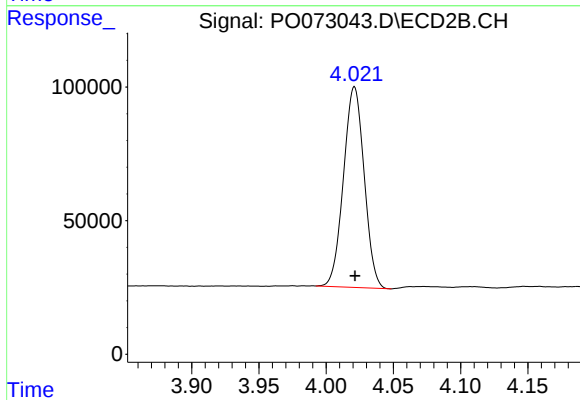


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 802602
Conc: 22.90 ng/ml

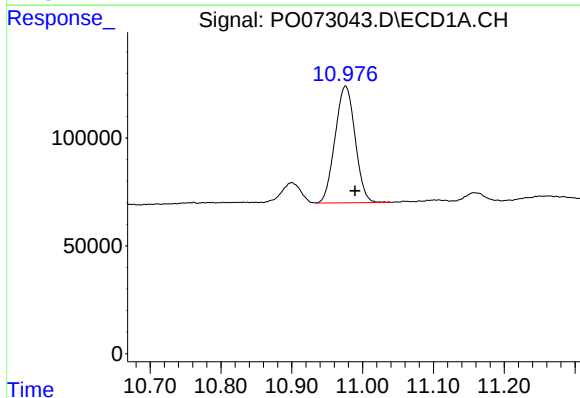

#2 Decachlorobiphenyl

R.T.: 10.976 min
Delta R.T.: -0.013 min
Response: 1064215
Conc: 28.81 ng/ml

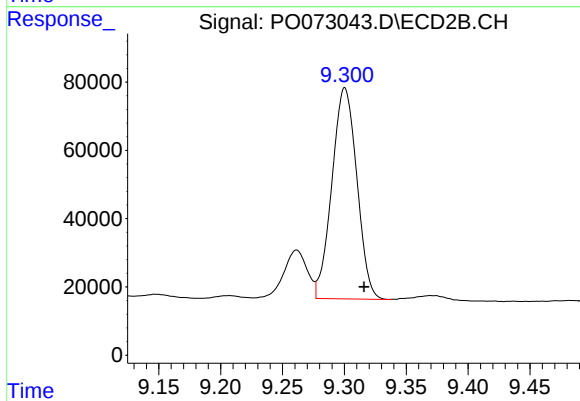

#2 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: -0.016 min
Response: 867590
Conc: 26.02 ng/ml m