

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110325\
 Data File : PO114840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2025 10:38
 Operator : YP/AJ
 Sample : Q3400-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FRAC-TANK-0760450

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/04/2025
 Supervised By :Yogesh Patel 11/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 12:54:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.349	3.652	130.0E6	85603238	23.941	21.389
2) SA Decachlor...	9.929	8.641	29717666	27624507	8.162	8.288m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110325\
Data File : PO114840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2025 10:38
Operator : YP/AJ
Sample : Q3400-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FRAC-TANK-0760450


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/04/2025
Supervised By :Yogesh Patel 11/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 12:54:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

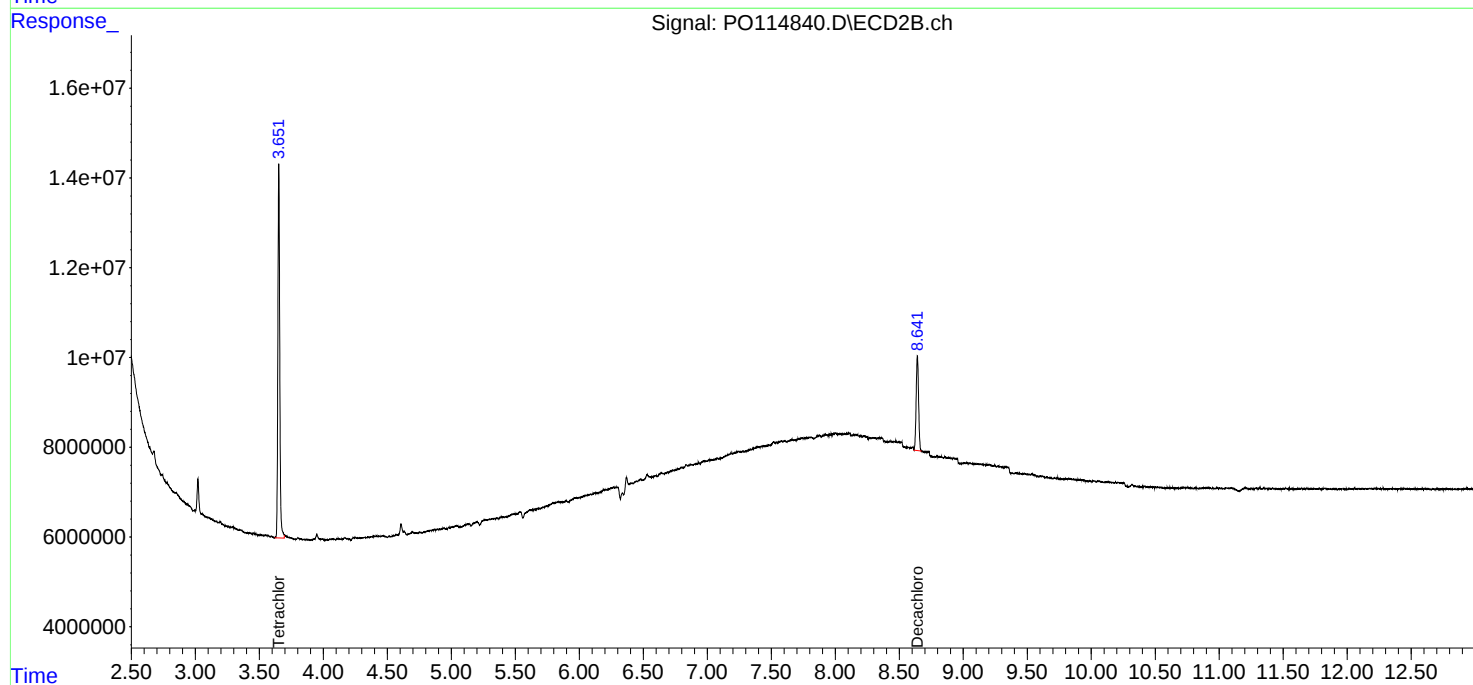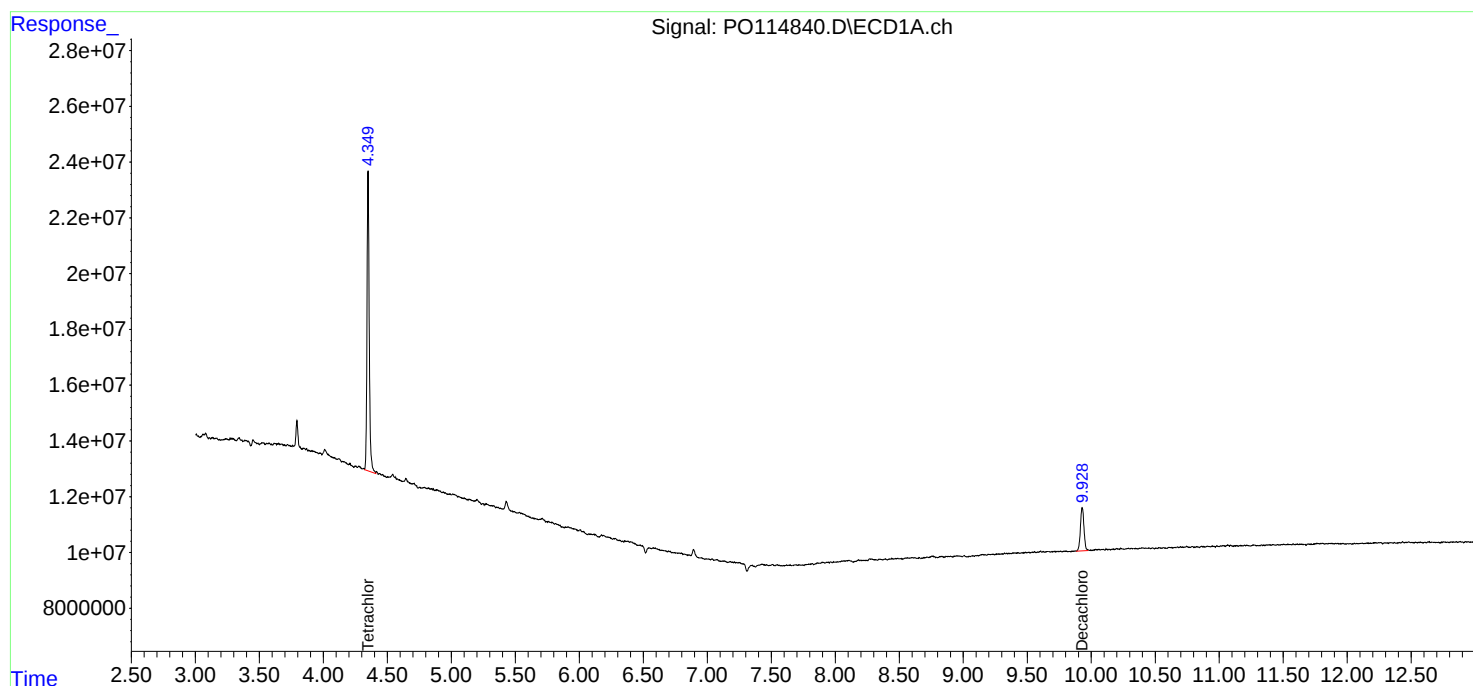

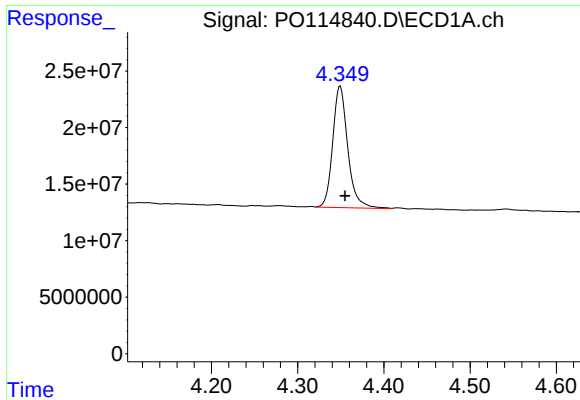


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: -0.006 min
Response: 129977616
Conc: 23.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
FRAC-TANK-0760450


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/04/2025
Supervised By :Yogesh Patel 11/04/2025

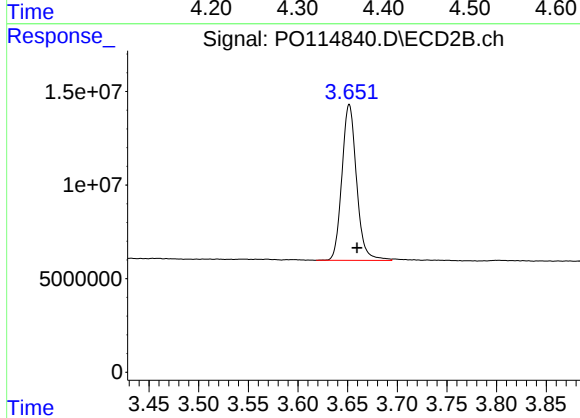


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.008 min
Response: 85603238
Conc: 21.39 ng/ml

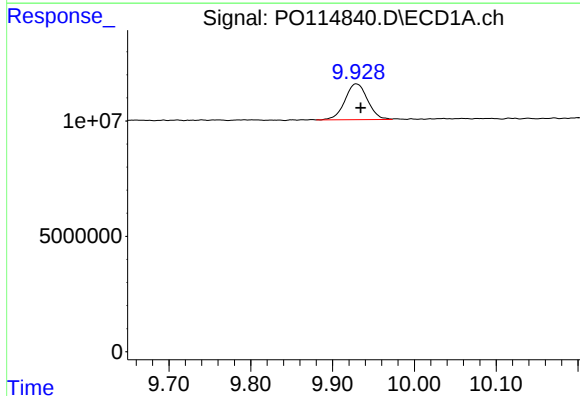

#2 Decachlorobiphenyl

R.T.: 9.929 min
Delta R.T.: -0.005 min
Response: 29717666
Conc: 8.16 ng/ml

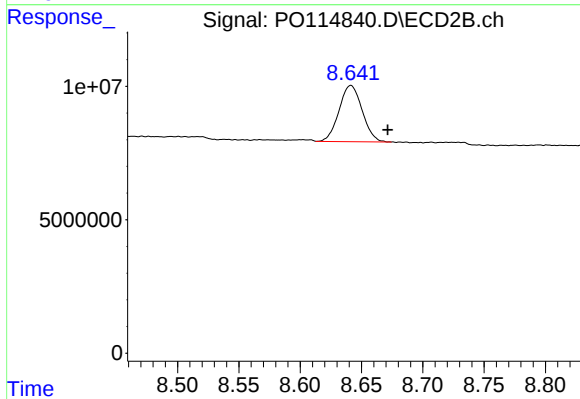

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: -0.030 min
Response: 27624507
Conc: 8.29 ng/ml m