

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110325\
 Data File : PO114841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2025 10:57
 Operator : YP/AJ
 Sample : Q3505-04RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 10-10-25-WATERRE

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/04/2025
 Supervised By :Yogesh Patel 11/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 12:55:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.652	16108296	9417974	2.967m	2.353
2) SA Decachlor...	9.930	8.641	11509178	9776602	3.161	2.933m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110325\
Data File : PO114841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2025 10:57
Operator : YP/AJ
Sample : Q3505-04RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
10-10-25-WATERRE


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/04/2025
Supervised By :Yogesh Patel 11/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 12:55:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

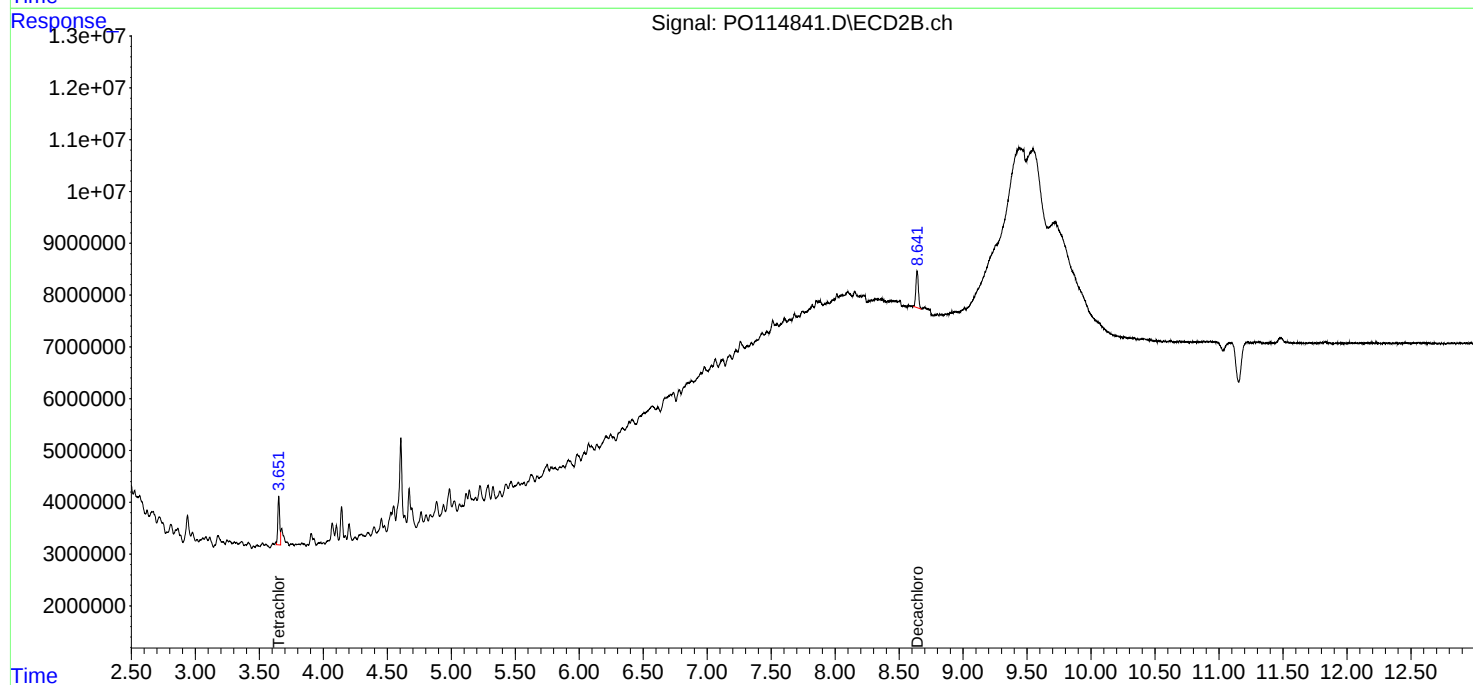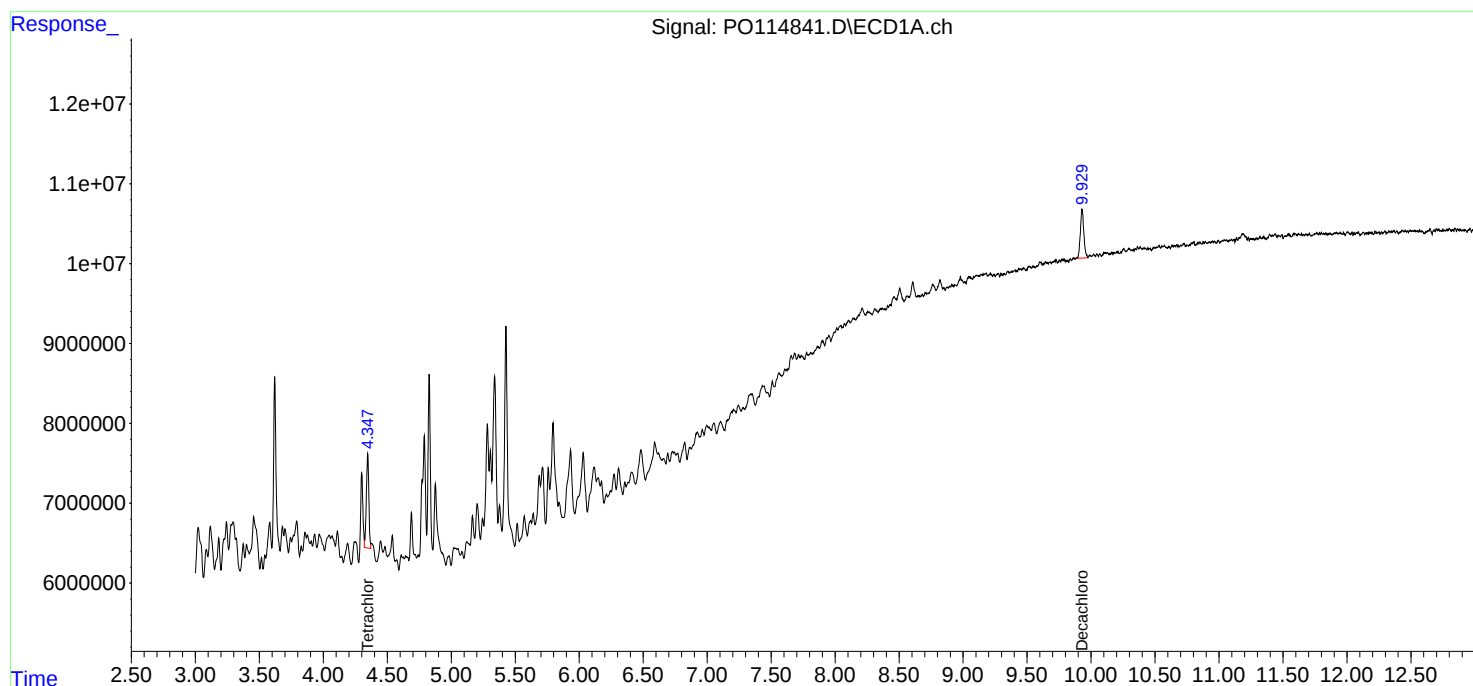

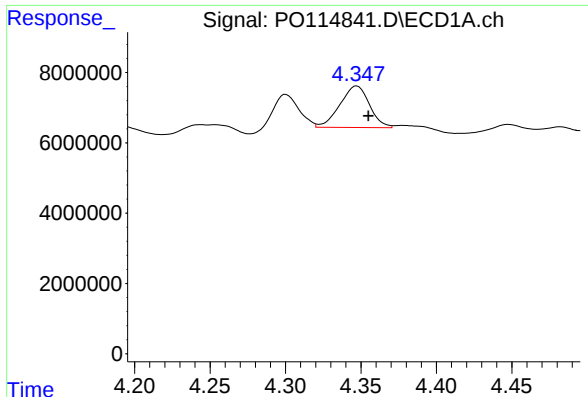


#1 Tetrachloro-m-xylene

R.T.: 4.347 min
Delta R.T.: -0.008 min
Response: 16108296
Conc: 2.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
10-10-25-WATERRE


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/04/2025
Supervised By :Yogesh Patel 11/04/2025

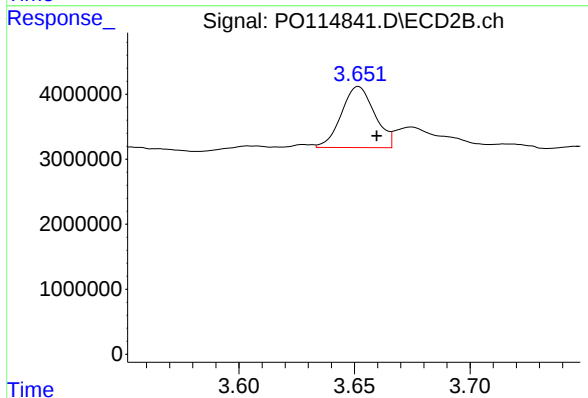


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: -0.008 min
Response: 9417974
Conc: 2.35 ng/ml

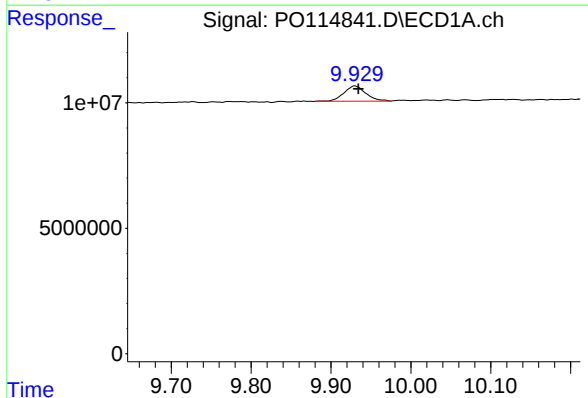

#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: -0.005 min
Response: 11509178
Conc: 3.16 ng/ml

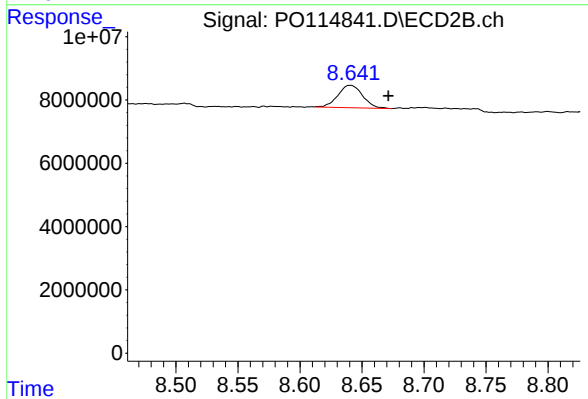

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: -0.030 min
Response: 9776602
Conc: 2.93 ng/ml m