

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110325\
 Data File : PO114843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2025 11:33
 Operator : YP/AJ
 Sample : Q3503-07 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 320

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/04/2025
 Supervised By :Yogesh Patel 11/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 12:58:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.349	3.651	3833052	5335486	0.706	1.333m#
2) SA Decachlor...	9.931	8.640	2222898	2112033	0.610m	0.634m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110325\
Data File : PO114843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2025 11:33
Operator : YP/AJ
Sample : Q3503-07 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
320


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/04/2025
Supervised By :Yogesh Patel 11/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 12:58:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

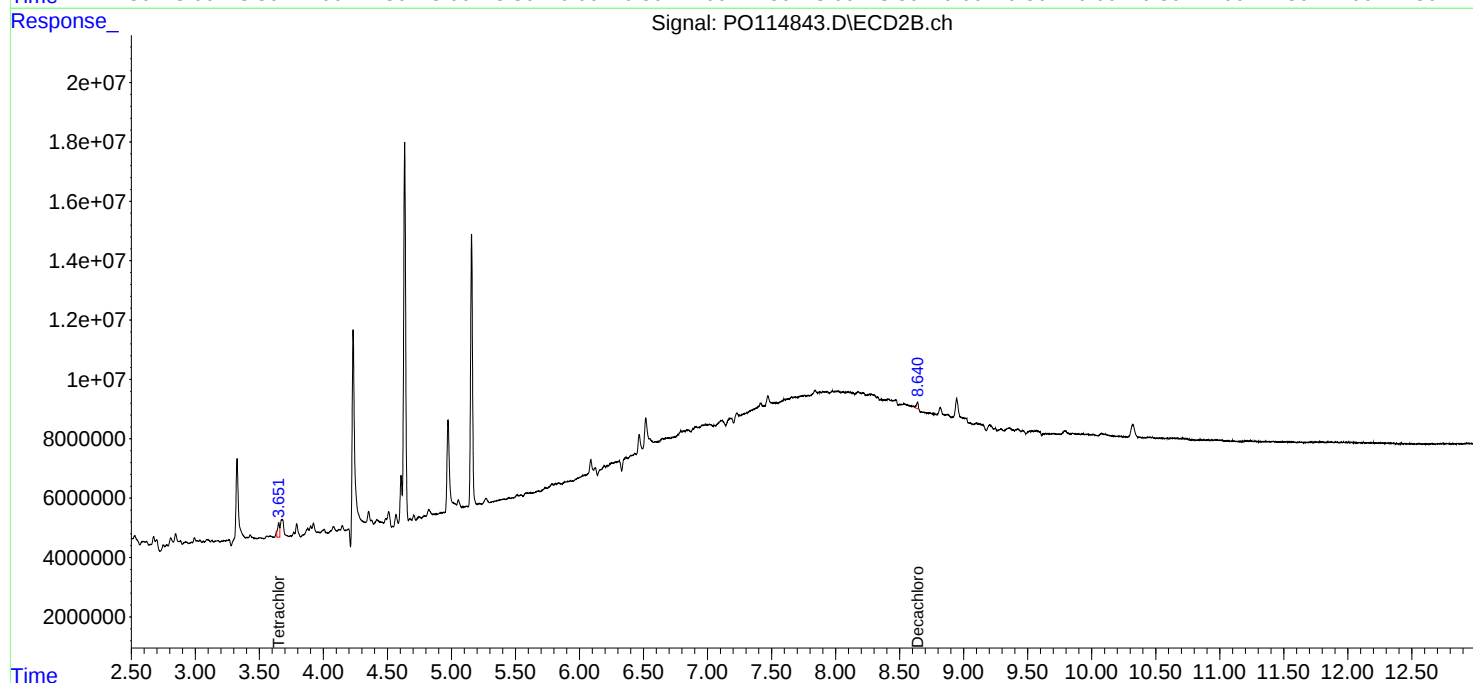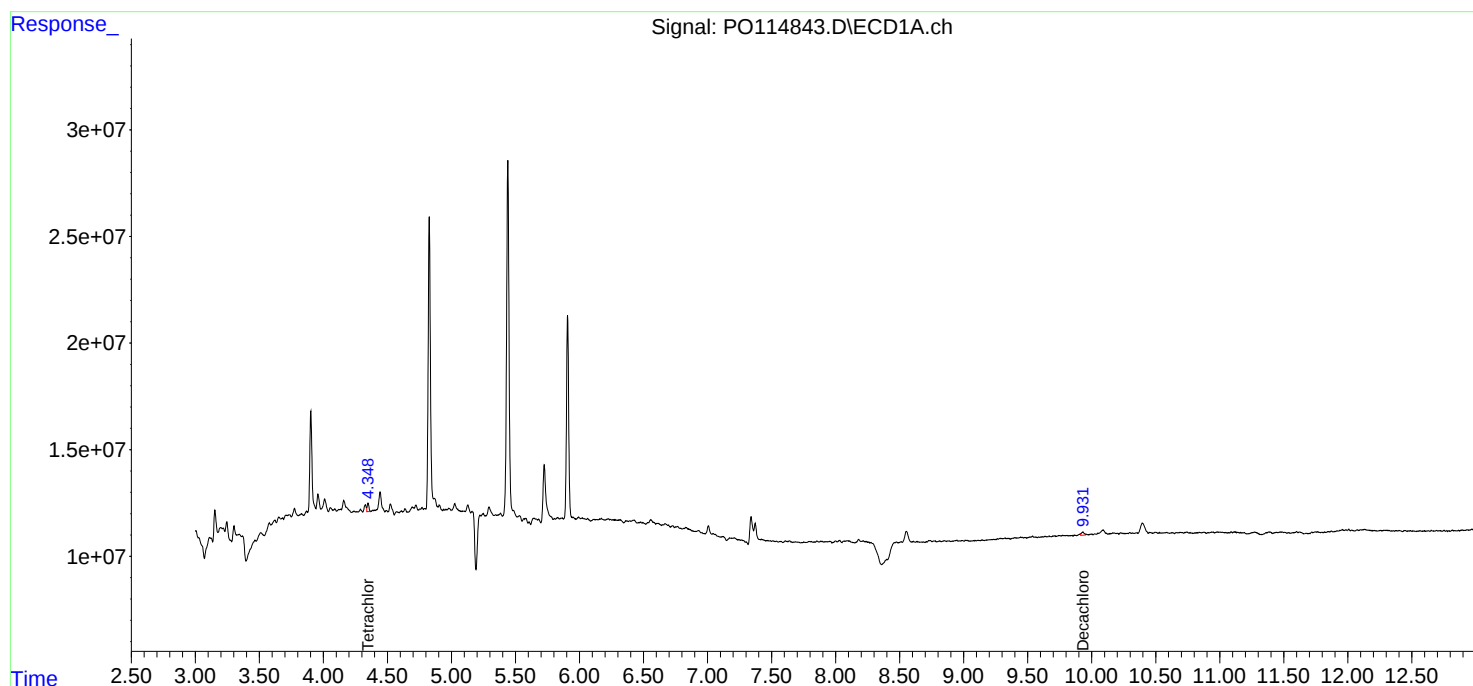

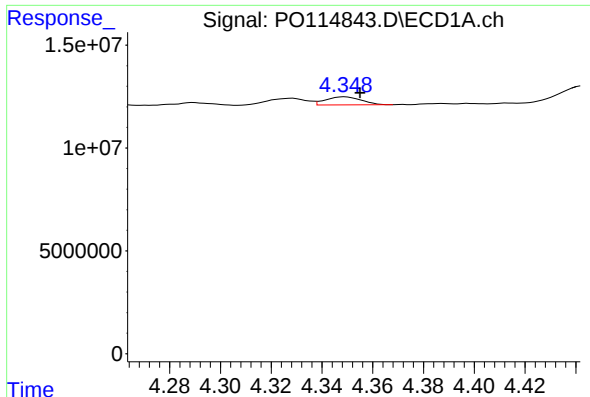


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: -0.006 min
Response: 3833052
Conc: 0.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
320


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/04/2025
Supervised By :Yogesh Patel 11/04/2025

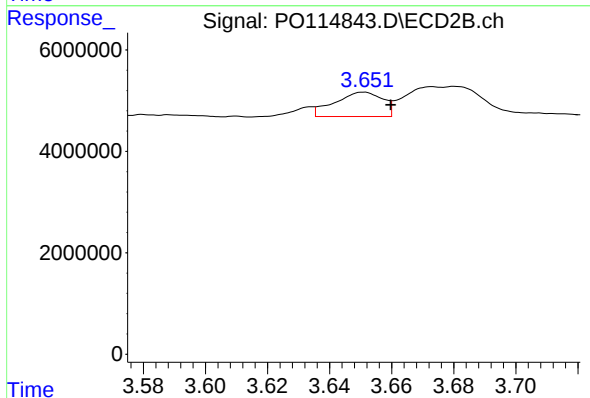


#1 Tetrachloro-m-xylene

R.T.: 3.651 min
Delta R.T.: -0.008 min
Response: 5335486
Conc: 1.33 ng/ml m

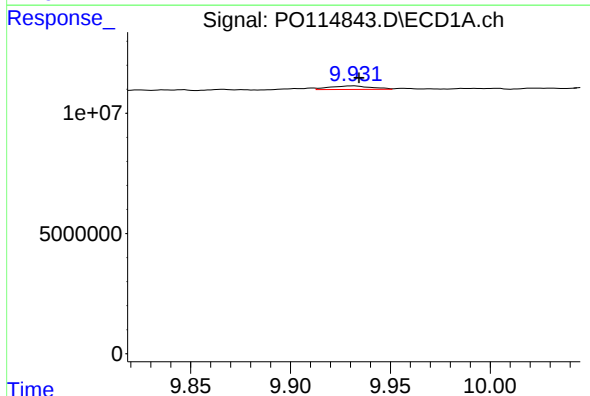

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.003 min
Response: 2222898
Conc: 0.61 ng/ml m

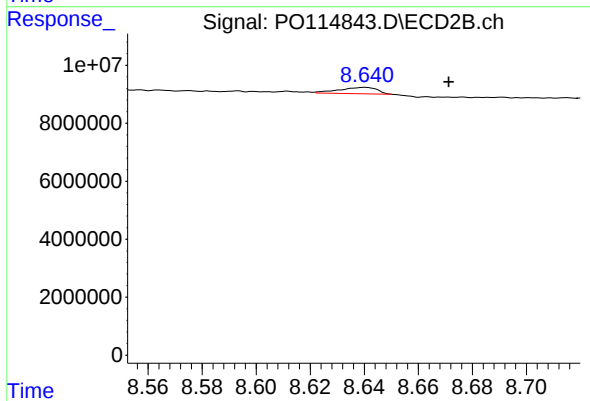

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: -0.031 min
Response: 2112033
Conc: 0.63 ng/ml m