

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110325\
 Data File : PO114854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2025 16:03
 Operator : YP/AJ
 Sample : PB170380BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB170380BL

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/04/2025
 Supervised By :Yogesh Patel 11/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:24:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.367	3.651	144.7E6	94746089	26.644	23.673
2) SA Decachlor...	9.949	8.643	87762864	76335159	24.103	22.902m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110325\
Data File : PO114854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2025 16:03
Operator : YP/AJ
Sample : PB170380BL
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB170380BL


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/04/2025
Supervised By :Yogesh Patel 11/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:24:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

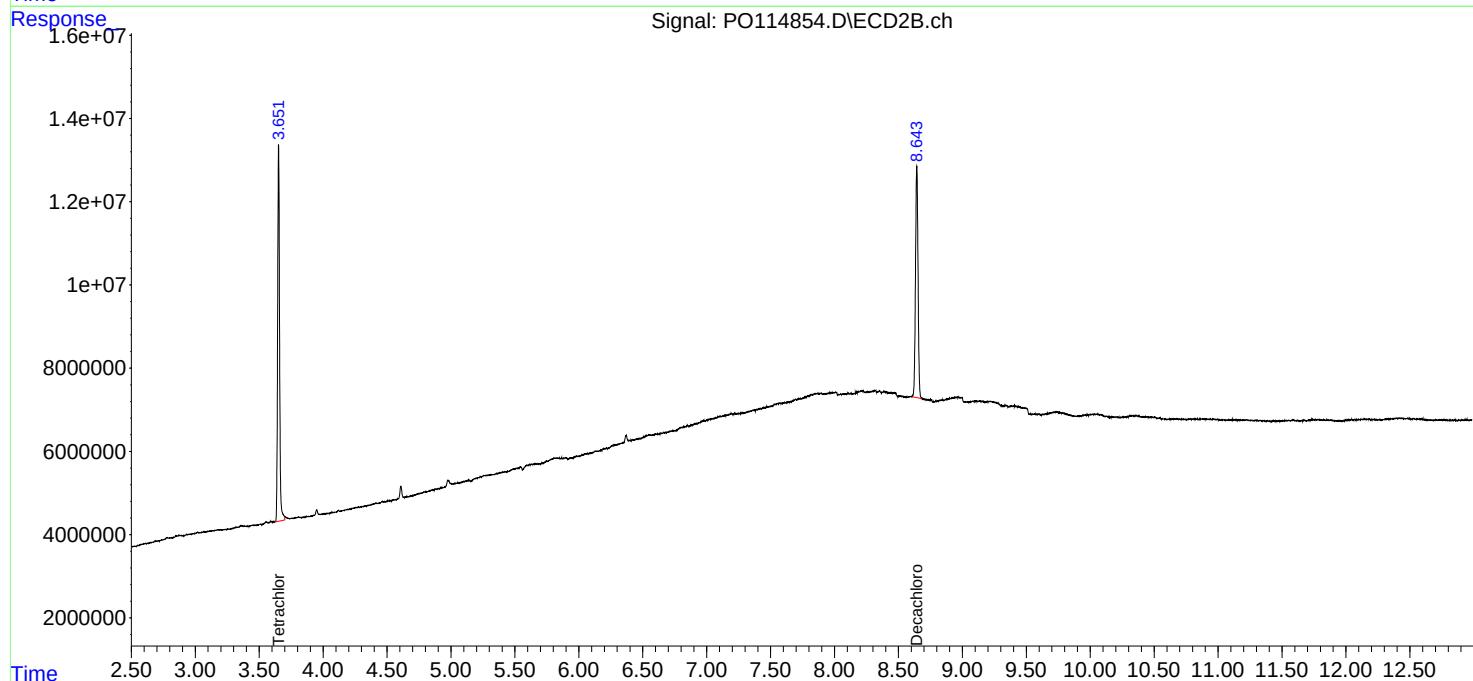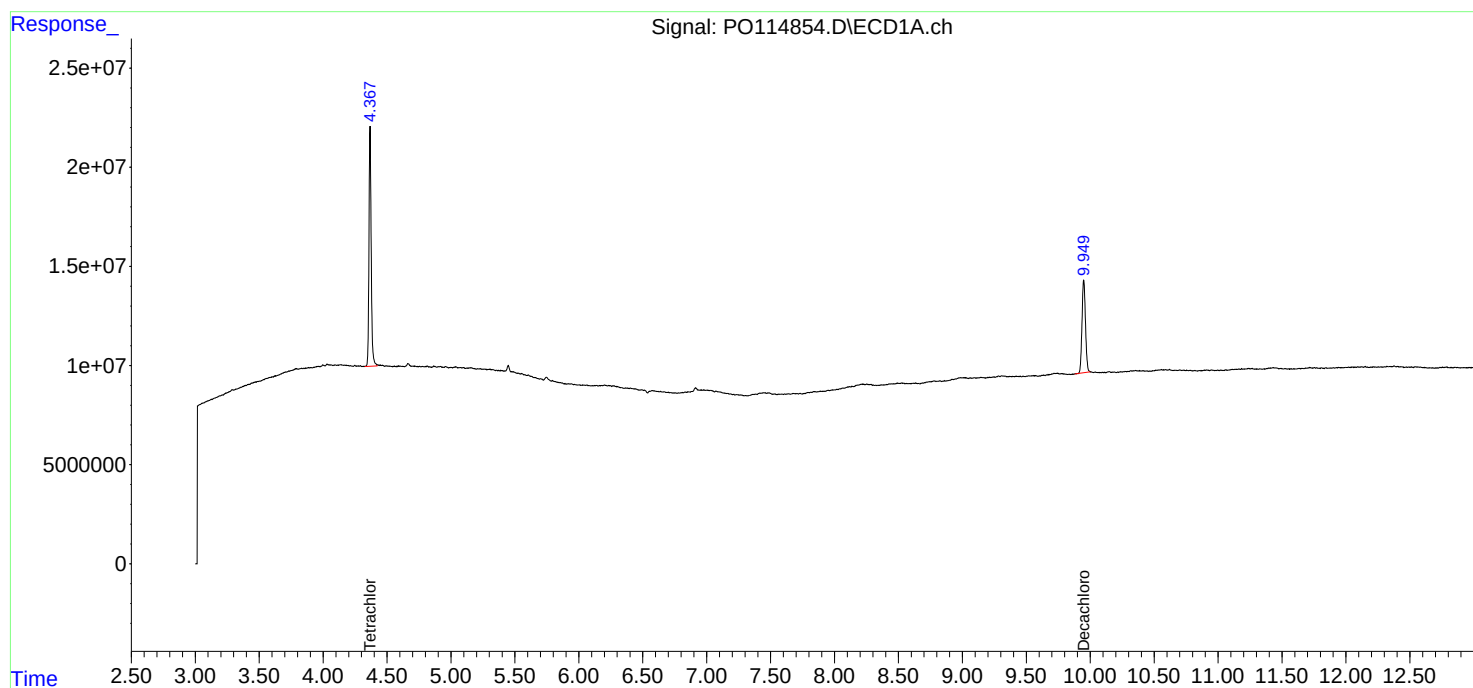

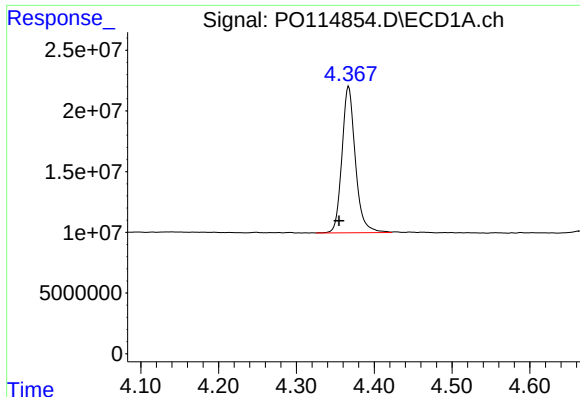


#1 Tetrachloro-m-xylene

R.T.: 4.367 min
Delta R.T.: 0.012 min
Response: 144650757
Conc: 26.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB170380BL


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/04/2025
Supervised By :Yogesh Patel 11/04/2025

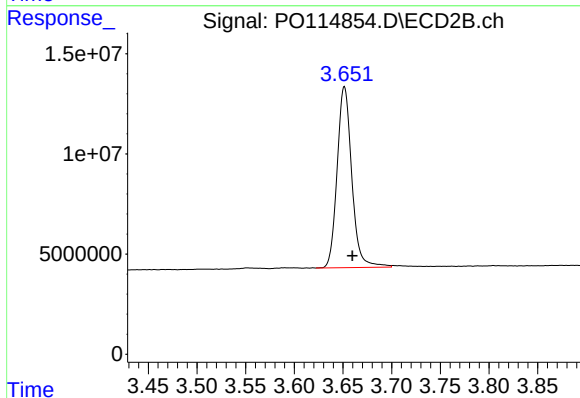


#1 Tetrachloro-m-xylene

R.T.: 3.651 min
Delta R.T.: -0.008 min
Response: 94746089
Conc: 23.67 ng/ml

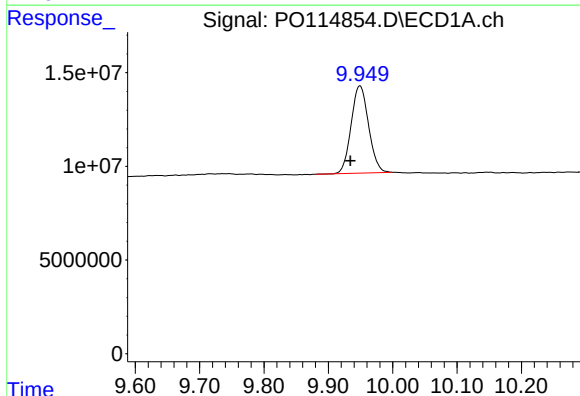

#2 Decachlorobiphenyl

R.T.: 9.949 min
Delta R.T.: 0.015 min
Response: 87762864
Conc: 24.10 ng/ml

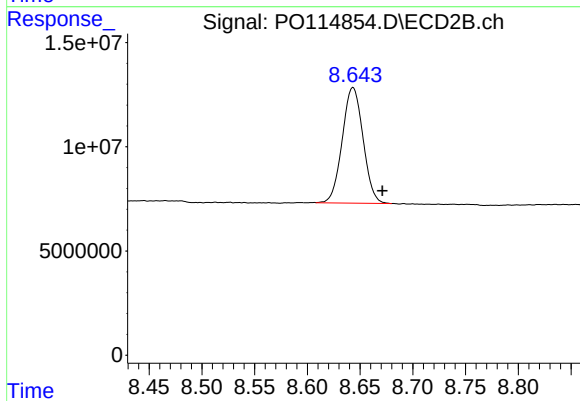

#2 Decachlorobiphenyl

R.T.: 8.643 min
Delta R.T.: -0.028 min
Response: 76335159
Conc: 22.90 ng/ml m