

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110421\
 Data File : PO082494.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2021 20:31
 Operator : AJ\MA
 Sample : M4438-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FDR-20211101-WC-LS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 11:31:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.969	3.966	1331218	482377	15.209	15.587
2) SA Decachlor...	11.073	9.279	817170	340164	12.940	11.814

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110421\
Data File : PO082494.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2021 20:31
Operator : AJ\MA
Sample : M4438-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FDR-20211101-WC-LS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 11:31:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

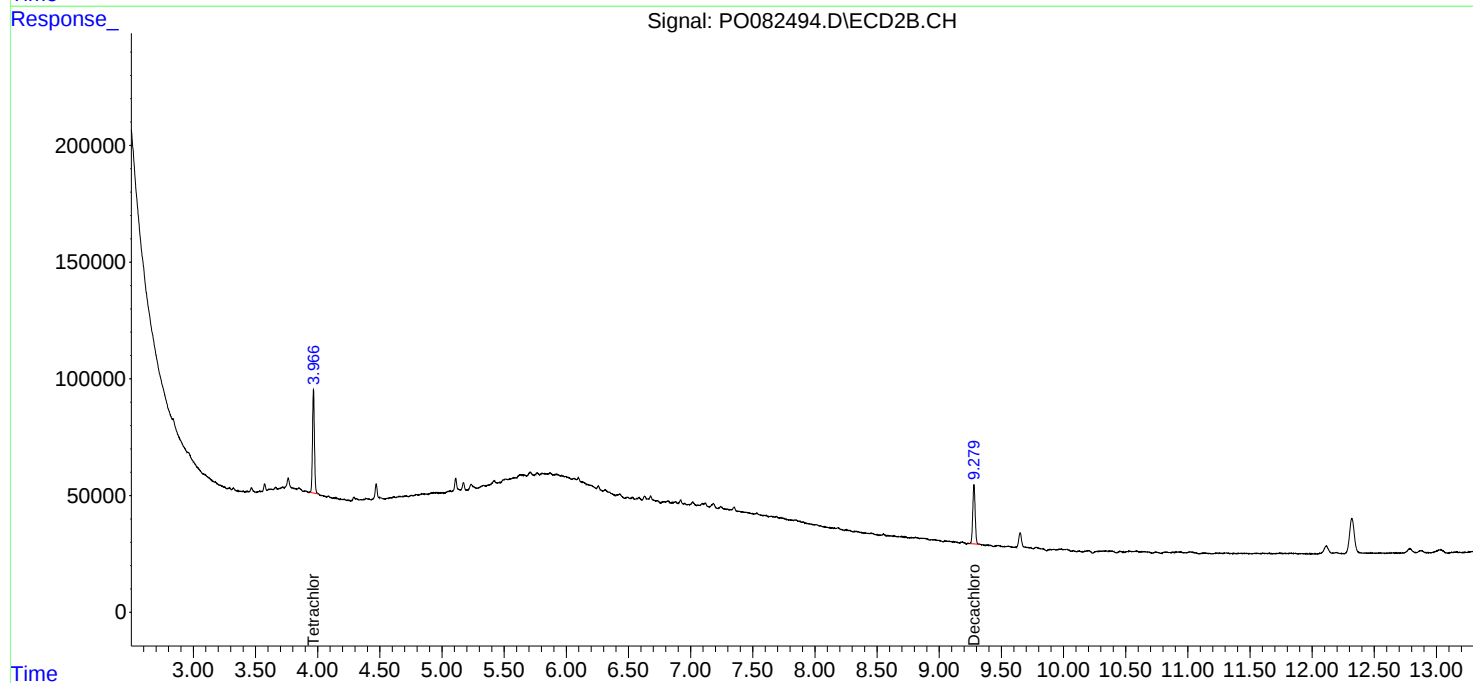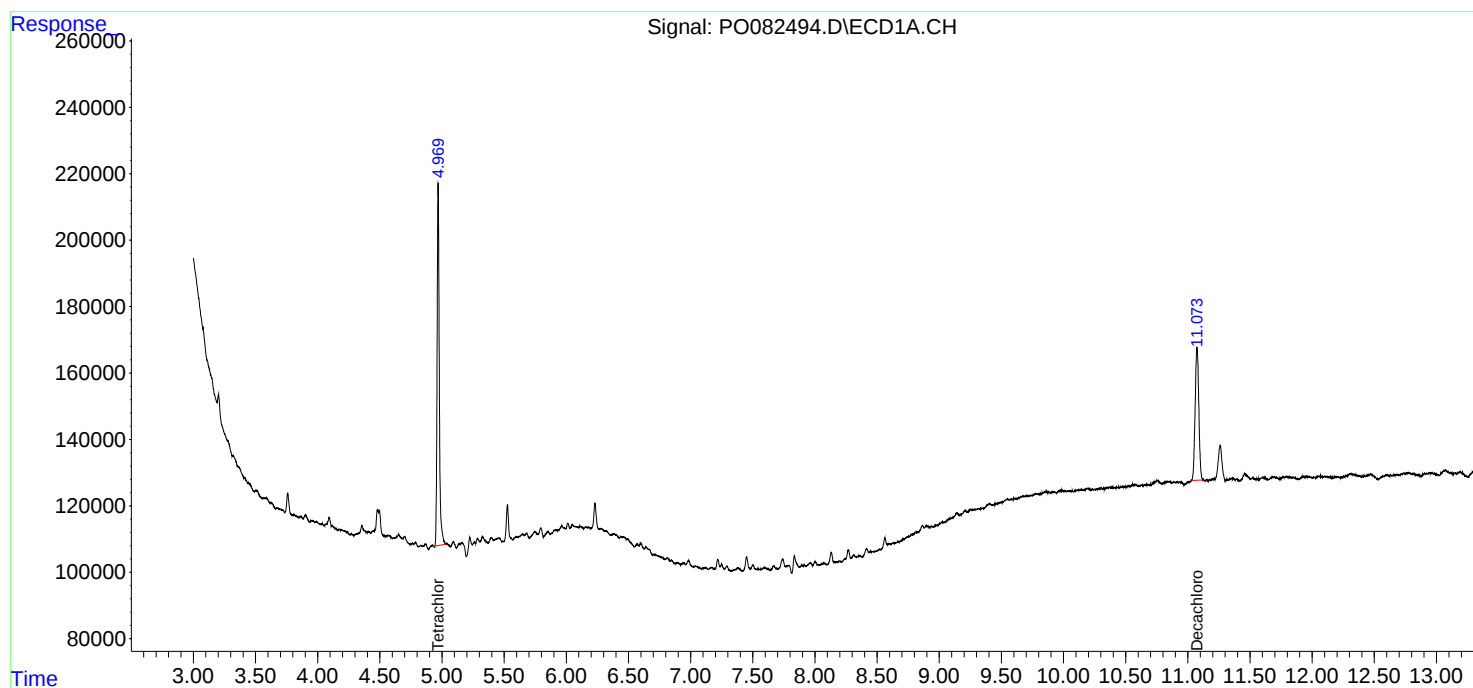


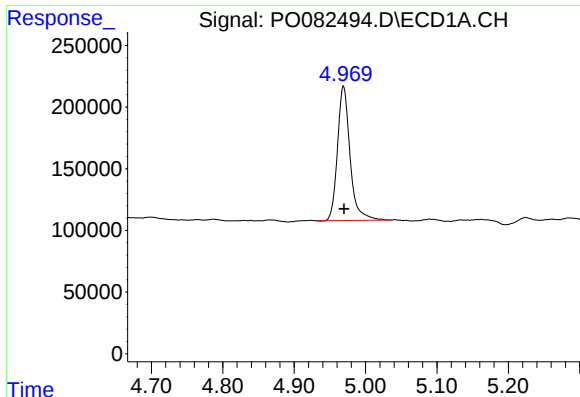

#1 Tetrachloro-m-xylene


R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 1331218
Conc: 15.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDR-20211101-WC-LS

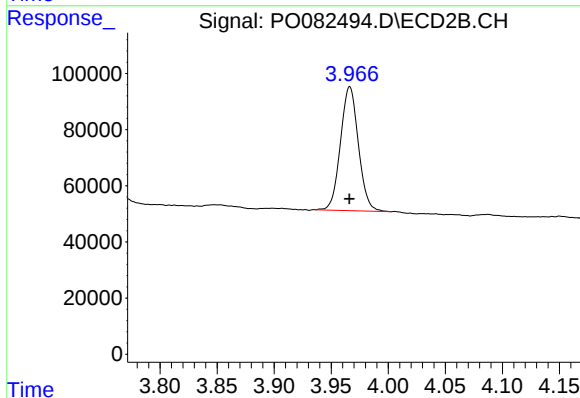


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 482377
Conc: 15.59 ng/ml

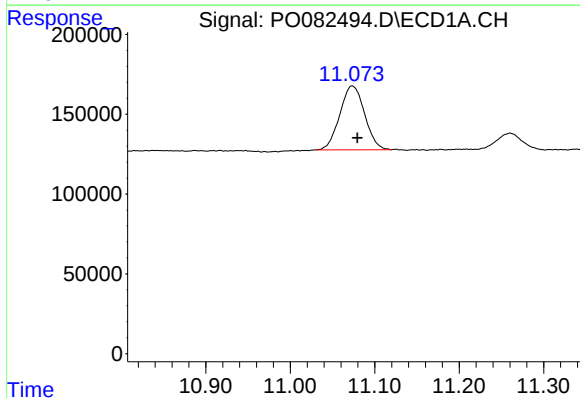

#2 Decachlorobiphenyl

R.T.: 11.073 min
Delta R.T.: -0.007 min
Response: 817170
Conc: 12.94 ng/ml

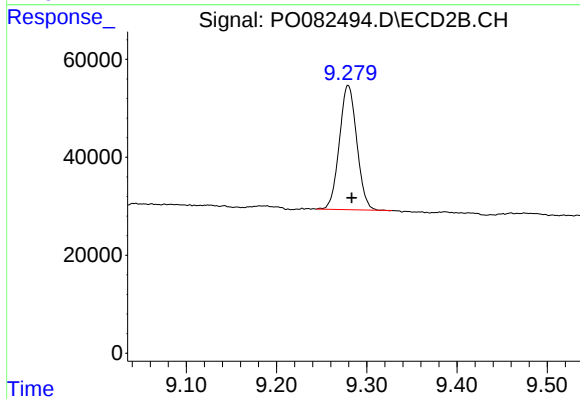

#2 Decachlorobiphenyl

R.T.: 9.279 min
Delta R.T.: -0.004 min
Response: 340164
Conc: 11.81 ng/ml