

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110421\
Data File : PO082496.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2021 21:06
Operator : AJ\MA
Sample : PB140443BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140443BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 11:31:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.968	3.964	1634180	597384	18.670	19.304
2) SA Decachlor...	11.073	9.280	1300568	597942	20.594	20.767

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110421\
Data File : PO082496.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2021 21:06
Operator : AJ\MA
Sample : PB140443BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140443BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 11:31:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

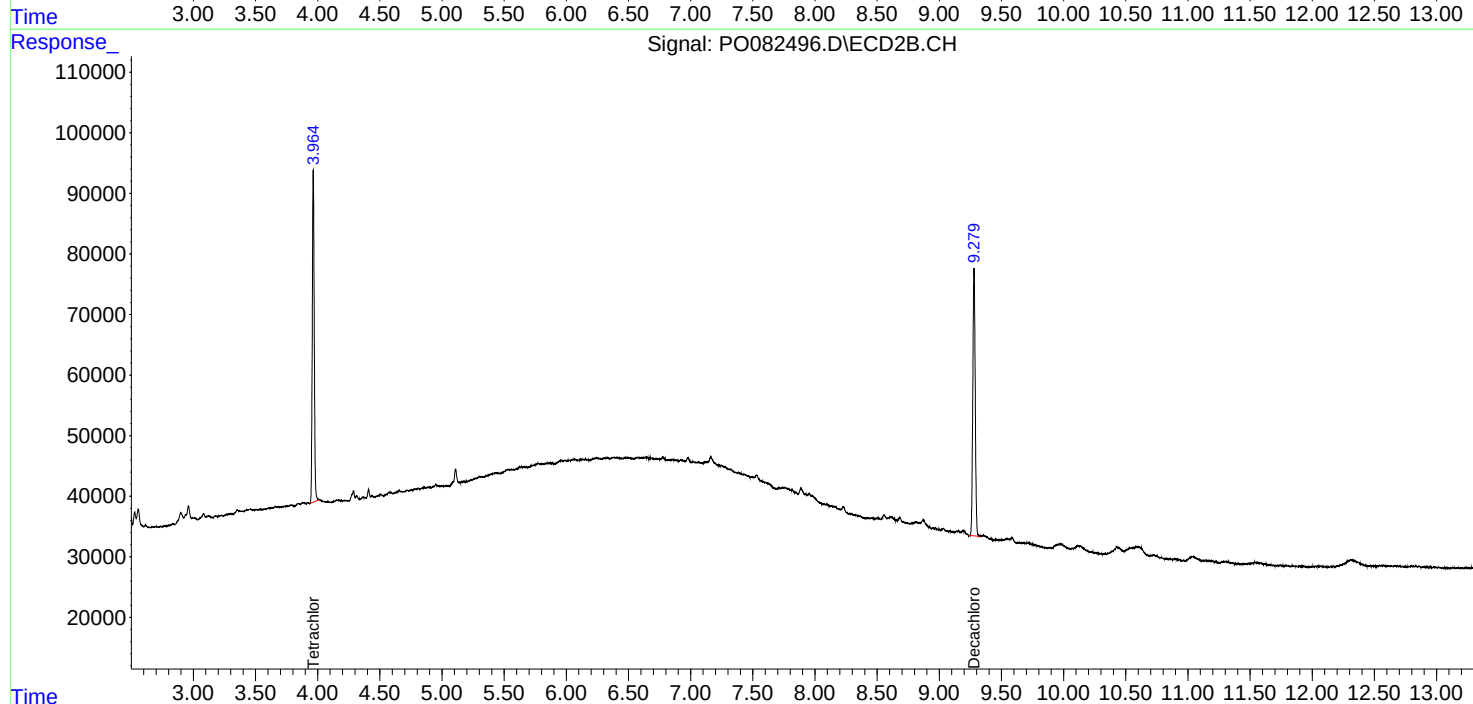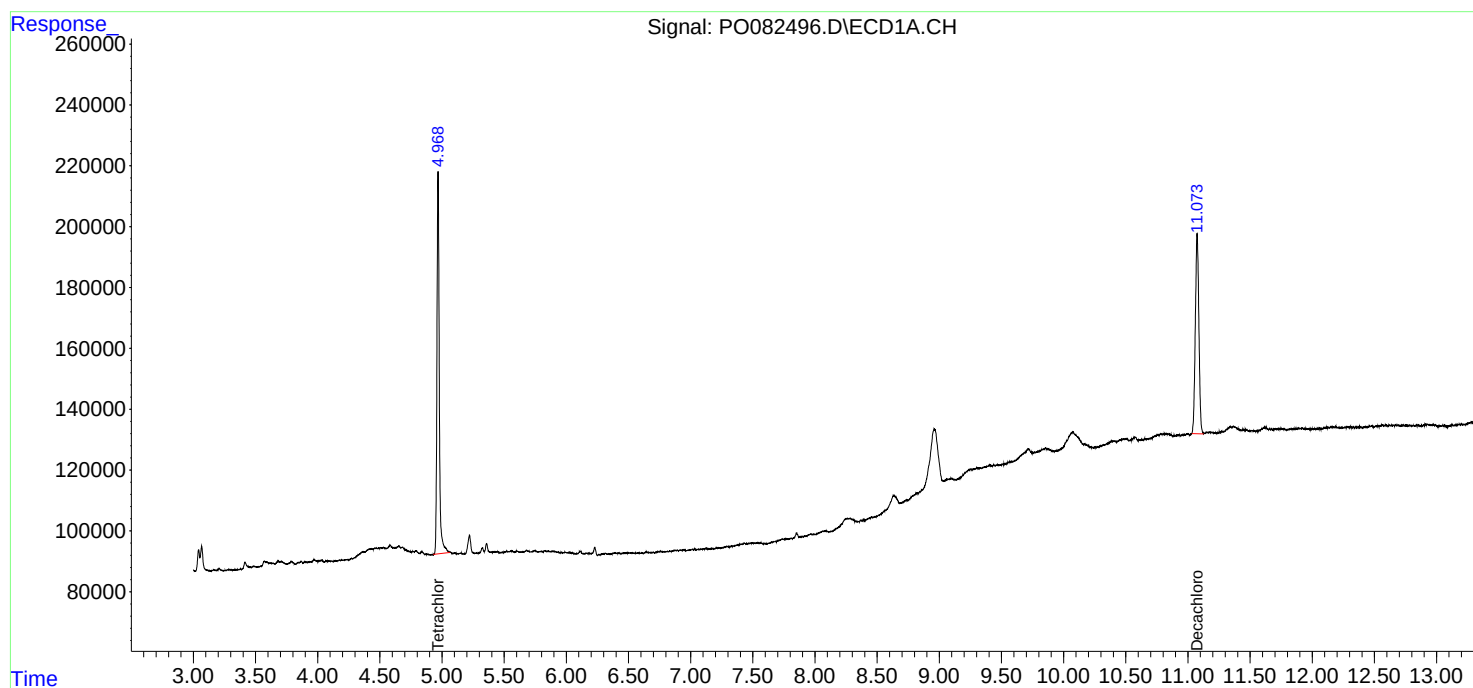


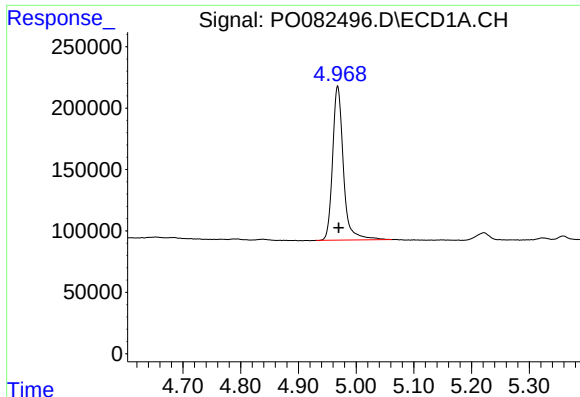

#1 Tetrachloro-m-xylene


R.T.: 4.968 min
Delta R.T.: -0.002 min
Response: 1634180
Conc: 18.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB140443BL

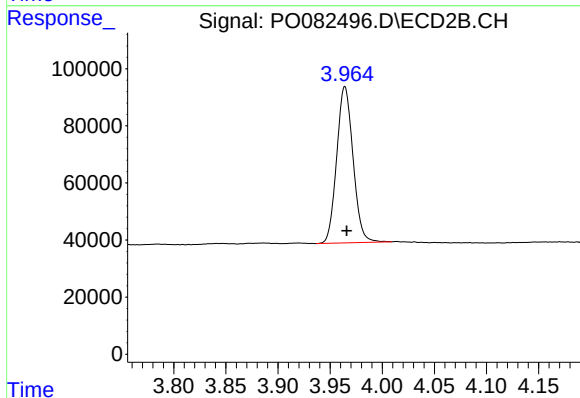


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: -0.002 min
Response: 597384
Conc: 19.30 ng/ml

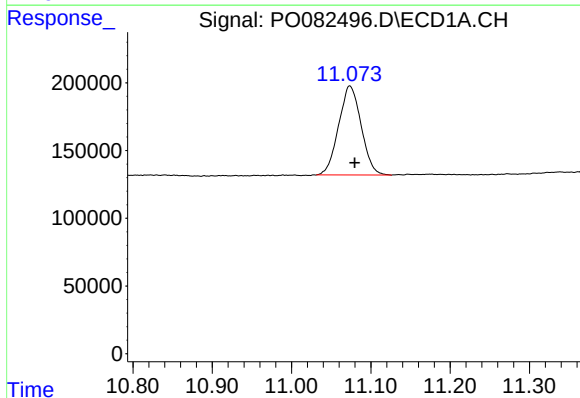

#2 Decachlorobiphenyl

R.T.: 11.073 min
Delta R.T.: -0.006 min
Response: 1300568
Conc: 20.59 ng/ml

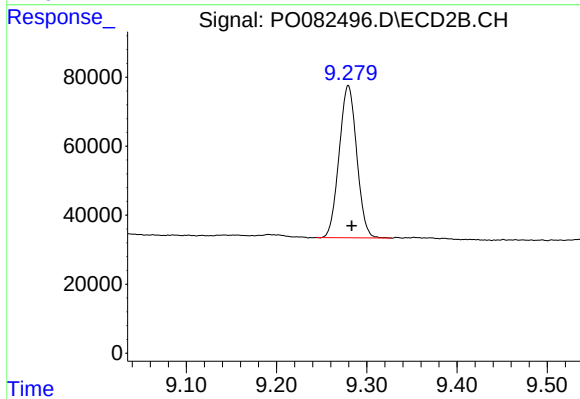

#2 Decachlorobiphenyl

R.T.: 9.280 min
Delta R.T.: -0.004 min
Response: 597942
Conc: 20.77 ng/ml