

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110421\
 Data File : PO082498.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2021 21:40
 Operator : AJ\MA
 Sample : PB140450BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB140450BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 11:31:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.968	3.964	1594193	583949	18.213	18.869
2) SA Decachlor...	11.072	9.279	1258694	598542	19.931	20.788

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110421\
Data File : PO082498.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2021 21:40
Operator : AJ\MA
Sample : PB140450BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140450BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 11:31:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

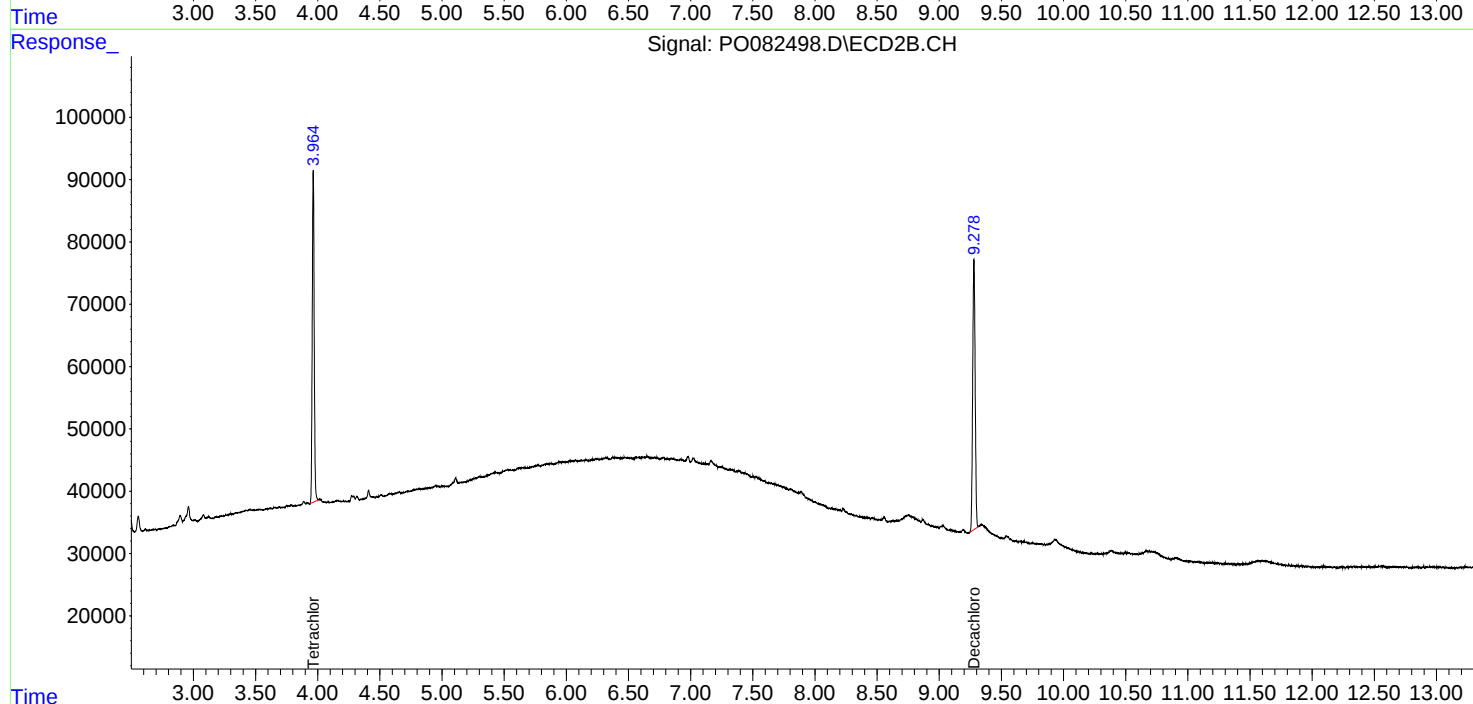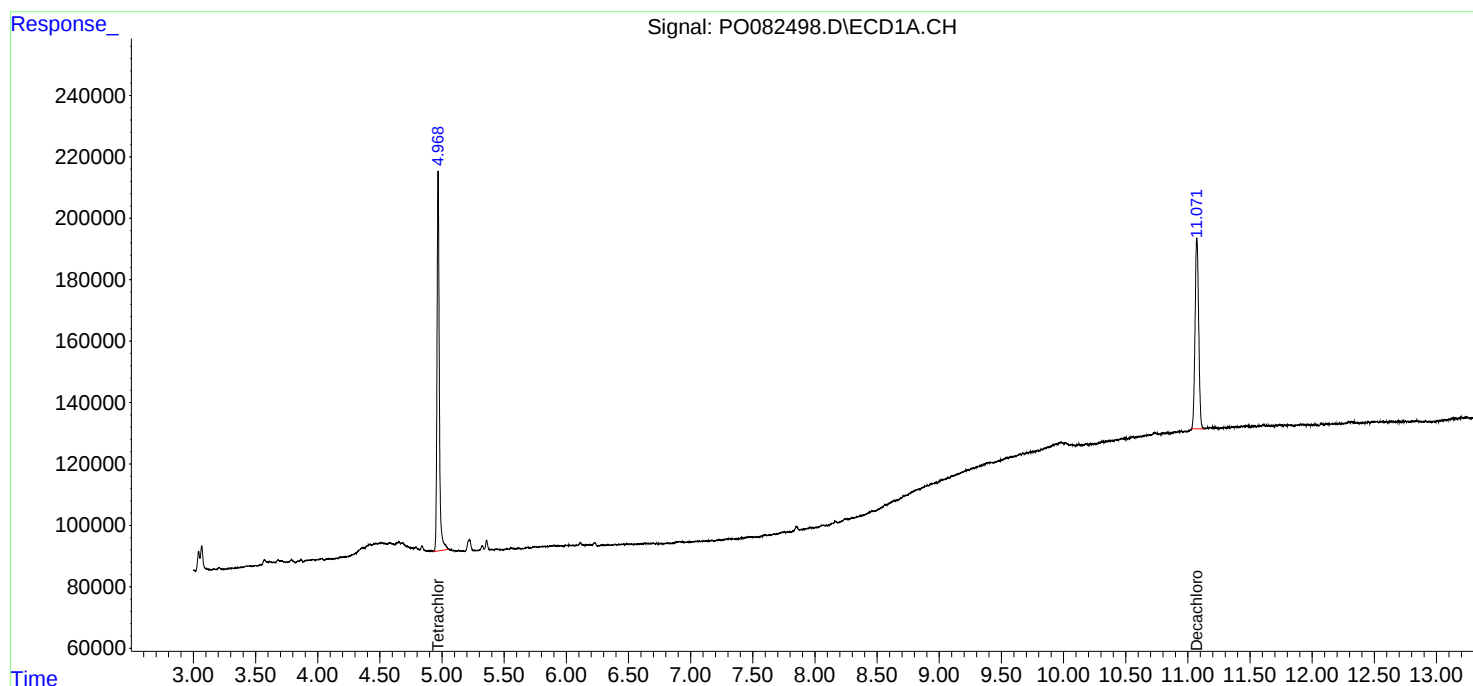


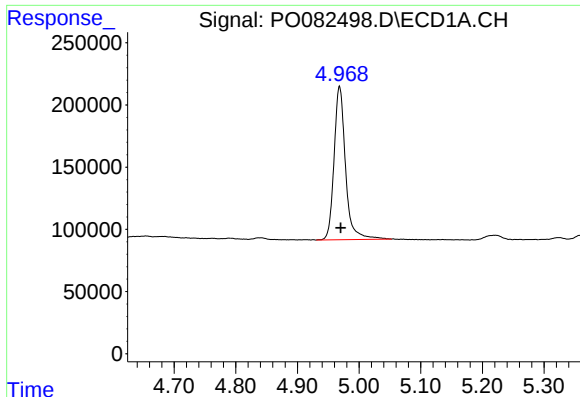

#1 Tetrachloro-m-xylene


R.T.: 4.968 min
Delta R.T.: -0.002 min
Response: 1594193
Conc: 18.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB140450BL

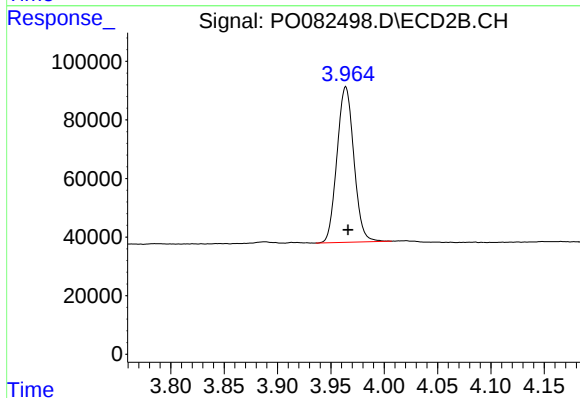


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: -0.002 min
Response: 583949
Conc: 18.87 ng/ml

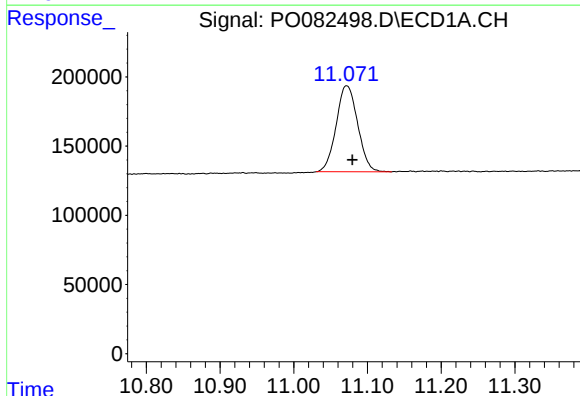

#2 Decachlorobiphenyl

R.T.: 11.072 min
Delta R.T.: -0.008 min
Response: 1258694
Conc: 19.93 ng/ml

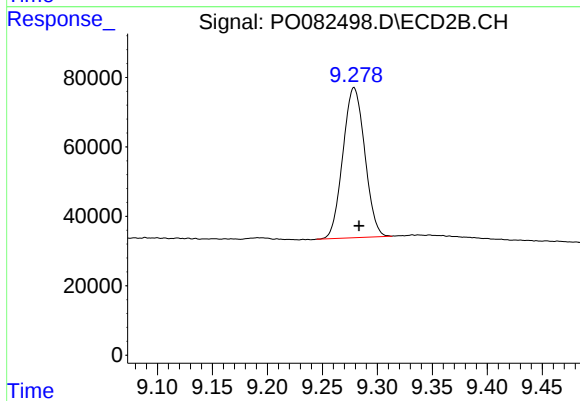

#2 Decachlorobiphenyl

R.T.: 9.279 min
Delta R.T.: -0.005 min
Response: 598542
Conc: 20.79 ng/ml