

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110425\
 Data File : PO114904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2025 22:48
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 02:17:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 02:14:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.339	3.652	182514	34187	0.026	0.008 #
2)	SA Decachlor...	9.934	8.638	164771	1475806	0.037	0.378 #
Target Compounds							
3)	L1 AR-1016-1	5.468	4.728	1700245	490647	6.911	2.579 #
4)	L1 AR-1016-2	5.513	4.739	686414	95995	1.729	0.354 #
5)	L1 AR-1016-3	5.569	4.918	582925	151117	2.614	1.021 #
6)	L1 AR-1016-4	5.662	4.964	338026	97657	1.790	0.832 #
7)	L1 AR-1016-5	5.946	5.175	498406	347942	2.797	2.278
8)	L2 AR-1221-1	4.541	3.861	472909	14706	5.622	0.238 #
9)	L2 AR-1221-2	4.642	3.955	129741	481657	2.156	10.554 #
10)	L2 AR-1221-3	4.706	4.021	287005	133569	1.484	0.952 #
11)	L3 AR-1232-1	4.706	4.021	287005	133569	1.913	1.198 #
12)	L3 AR-1232-2	5.212	4.739	1153721	95995	15.899	0.856 #
13)	L3 AR-1232-3	5.513	4.918	686414	151117	4.326	2.533 #
14)	L3 AR-1232-4	5.662	5.004	338026	135841	4.581	2.669 #
15)	L3 AR-1232-5	5.754	5.175	250886	347942	4.864	6.149 #
16)	L4 AR-1242-1	5.468	4.728	1700245	490647	9.129	3.356 #
17)	L4 AR-1242-2	5.513	4.739	686414	95995	2.297	0.463 #
18)	L4 AR-1242-3	5.569	4.918	582925	151117	3.402	1.350 #
19)	L4 AR-1242-4	5.662	5.004	338026	135841	2.361	1.268 #
20)	L4 AR-1242-5	6.398	5.526	166983	101966	1.185	0.713 #
21)	L5 AR-1248-1	5.468	4.728	1700245	490647	12.158	4.489 #
22)	L5 AR-1248-2	5.754	4.964	250886	97657	1.290	0.656 #
23)	L5 AR-1248-3	5.946	5.004	498406	135841	2.364	0.874 #
24)	L5 AR-1248-4	6.353	5.175	186420	347942	0.738	1.899 #
25)	L5 AR-1248-5	6.398	5.567	166983	126125	0.708	0.684
26)	L6 AR-1254-1	6.340	5.526	440575	101966	1.688	0.340 #
27)	L6 AR-1254-2	6.542	5.671	5628319	26694	15.384	0.099 #
28)	L6 AR-1254-3	6.915	6.064	13634801	976839	35.428	2.313 #
29)	L6 AR-1254-4	7.189	6.322	658871	24481	1.975	0.532 #
30)	L6 AR-1254-5	7.621	6.719	2550.9E6	2583.5E6	8450.956	6498.921
31)	L7 AR-1260-1	7.074	6.200	1689589	693263	5.528	2.341 #
32)	L7 AR-1260-2	7.308	6.397	2664.1E6	1361002	6729.682	3.165 #
33)	L7 AR-1260-3	7.713	6.556	3283204	774049	9.895	2.204 #
34)	L7 AR-1260-4	7.933	7.014	195325	523809	0.640	1.729 #
35)	L7 AR-1260-5	8.199	7.255	790948	229963	1.109	0.280 #
36)	L8 AR-1262-1	7.713	6.798f	3283204	1290033	7.241	2.610 #
37)	L8 AR-1262-2	8.237	7.255	781324	229963	1.105	0.289 #
38)	L8 AR-1262-3	8.535	7.548	49418	7697694	0.109	23.395 #
39)	L8 AR-1262-4	8.633	7.621	286752	367412	0.853	0.683
40)	L8 AR-1262-5	9.229	8.094	170513	179791	0.705	0.755
41)	L9 AR-1268-1	8.509	7.548	156111	7697694	0.179	7.886 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110425\
Data File : PO114904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2025 22:48
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 02:17:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 02:14:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.597	7.621	261920	367412	0.351	0.462 #
43)	L9 AR-1268-3	8.823	7.818	127308	152315	0.193	0.225
44)	L9 AR-1268-4	9.215	8.094	179057	179791	0.638	0.653
45)	L9 AR-1268-5	9.618	8.389	435428	531494	0.225	0.298 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110425\
Data File : PO114904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2025 22:48
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 02:17:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 02:14:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

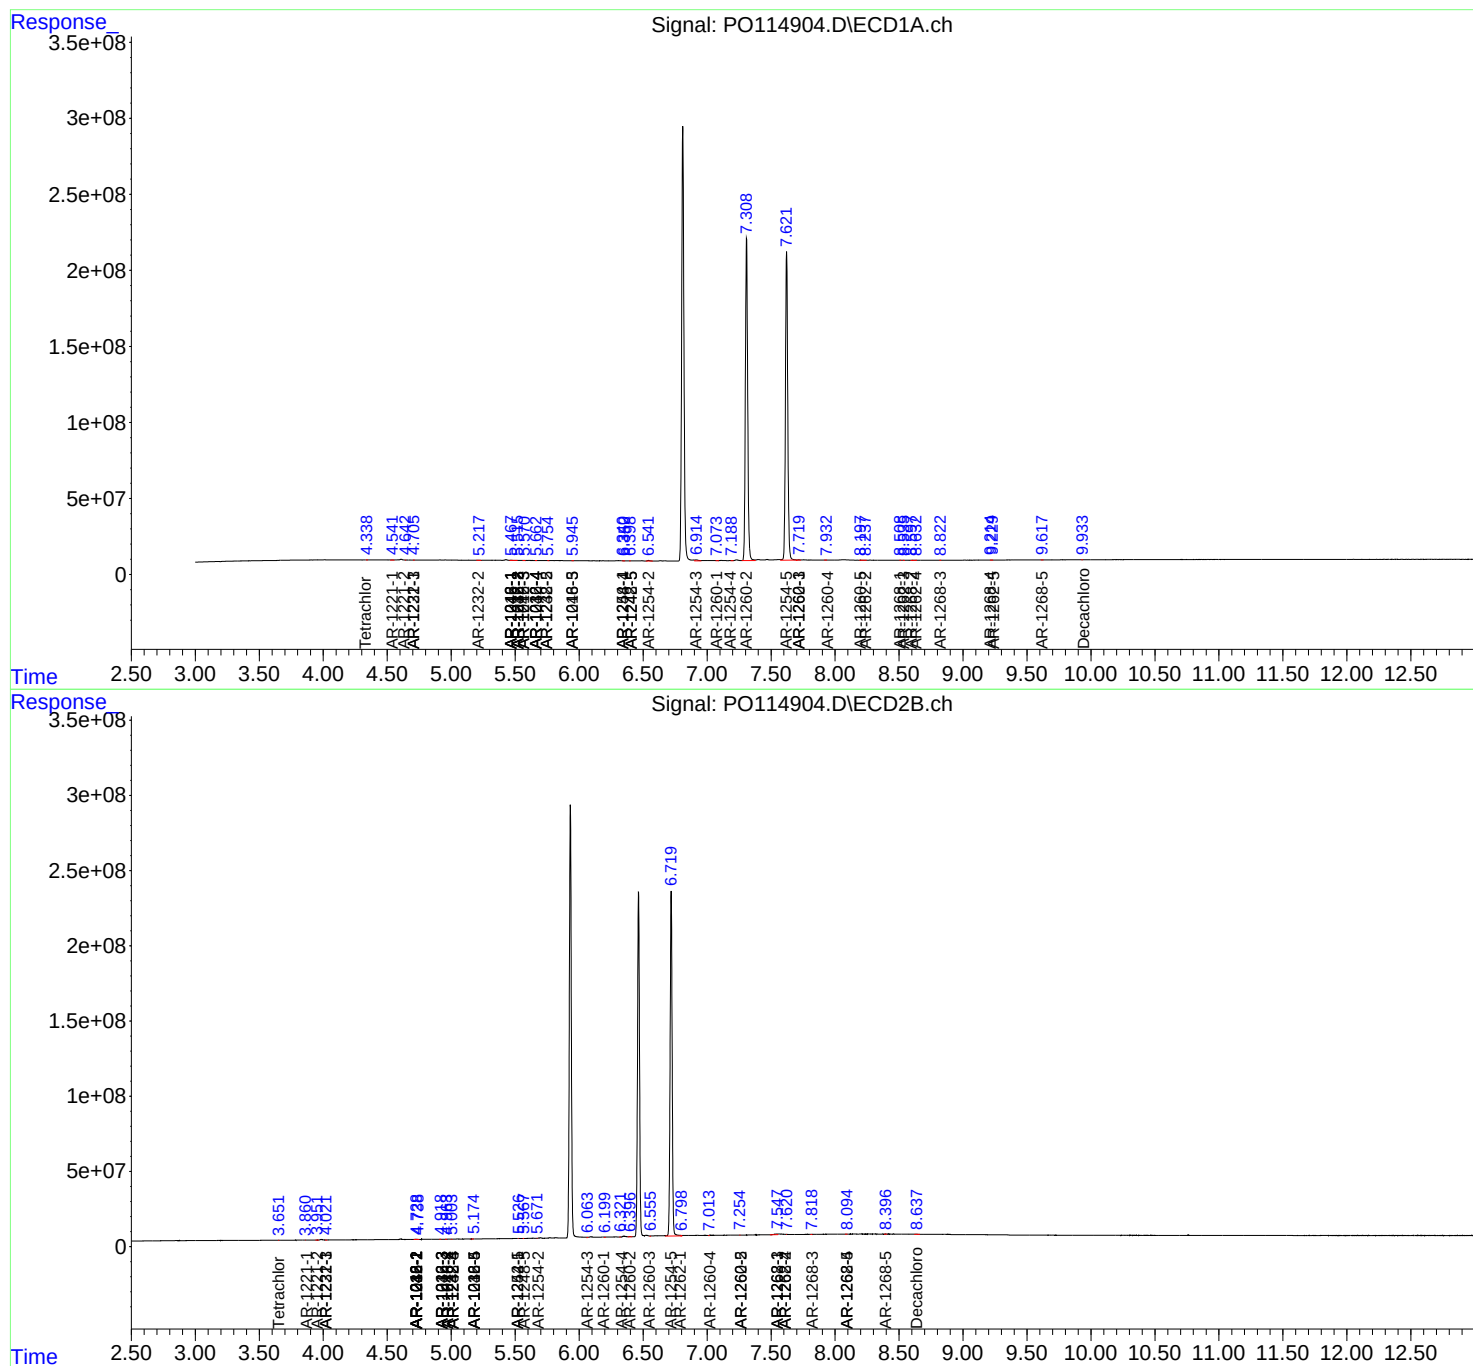


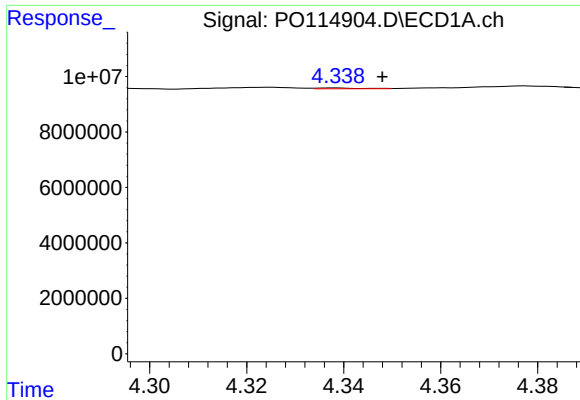

#1 Tetrachloro-m-xylene


R.T.: 4.339 min
Delta R.T.: -0.009 min
Response: 182514
Conc: 0.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

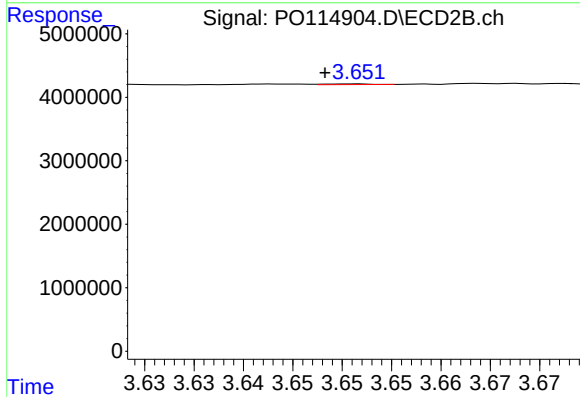


#1 Tetrachloro-m-xylene

R.T.: 3.652 min
Delta R.T.: 0.003 min
Response: 34187
Conc: 0.01 ng/ml

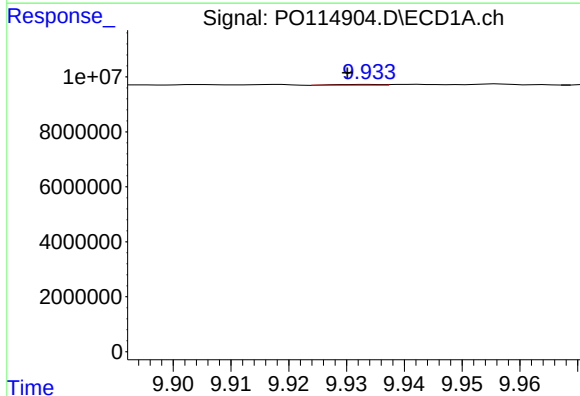


#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: 0.004 min
Response: 164771
Conc: 0.04 ng/ml

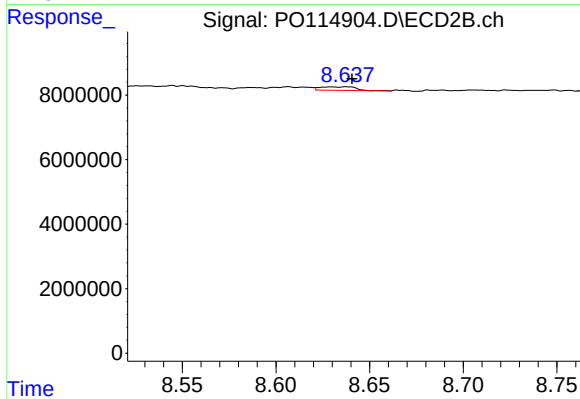

#2 Decachlorobiphenyl


R.T.: 8.638 min
Delta R.T.: -0.003 min
Response: 1475806
Conc: 0.38 ng/ml

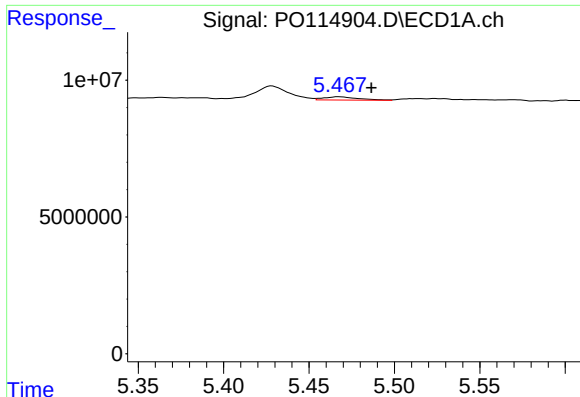

#3 AR-1016-1


R.T.: 5.468 min
Delta R.T.: -0.019 min
Response: 1700245
Conc: 6.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

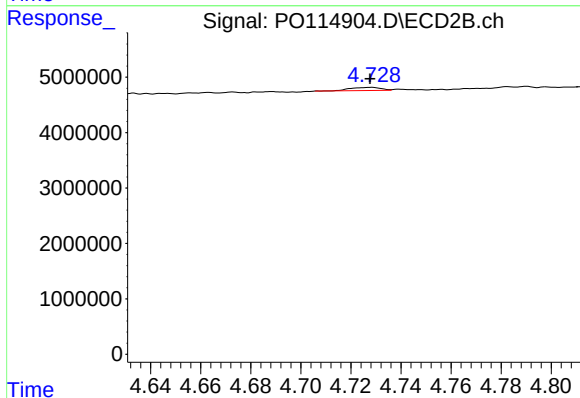


#3 AR-1016-1

R.T.: 4.728 min
Delta R.T.: 0.000 min
Response: 490647
Conc: 2.58 ng/ml

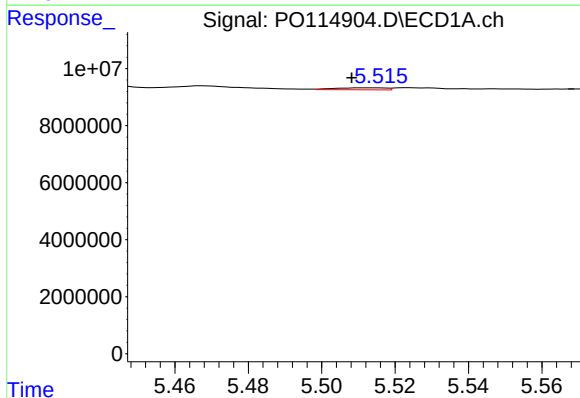


#4 AR-1016-2

R.T.: 5.513 min
Delta R.T.: 0.005 min
Response: 686414
Conc: 1.73 ng/ml

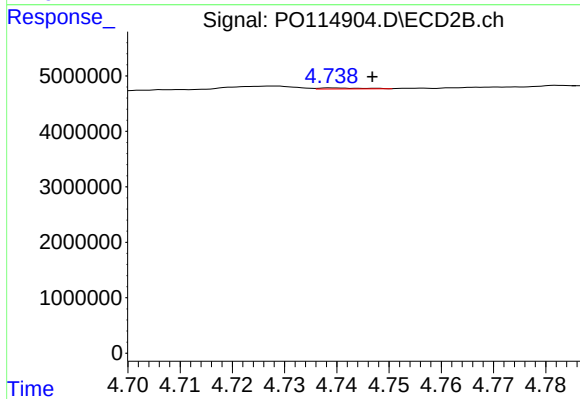

#4 AR-1016-2


R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 95995
Conc: 0.35 ng/ml

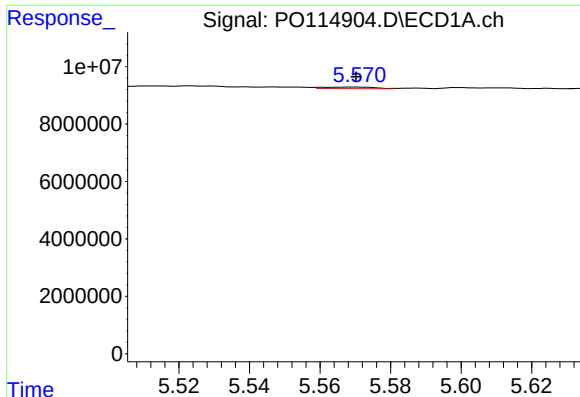

#5 AR-1016-3


R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 582925
Conc: 2.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

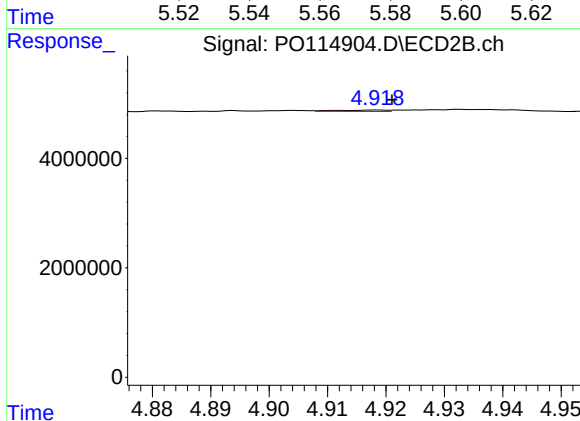


#5 AR-1016-3

R.T.: 4.918 min
Delta R.T.: -0.003 min
Response: 151117
Conc: 1.02 ng/ml

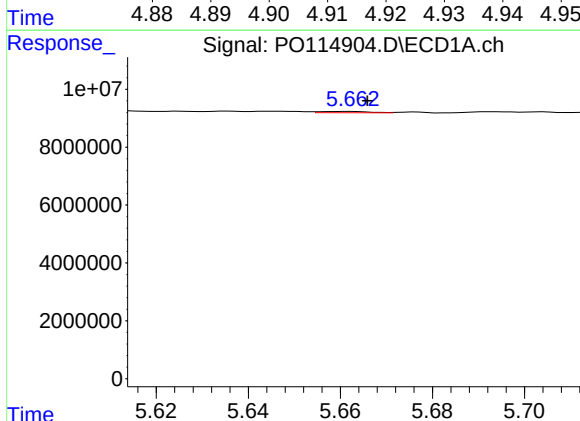


#6 AR-1016-4

R.T.: 5.662 min
Delta R.T.: -0.004 min
Response: 338026
Conc: 1.79 ng/ml

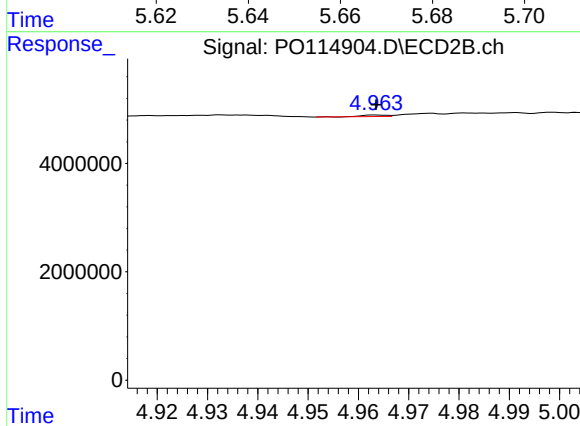

#6 AR-1016-4


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 97657
Conc: 0.83 ng/ml

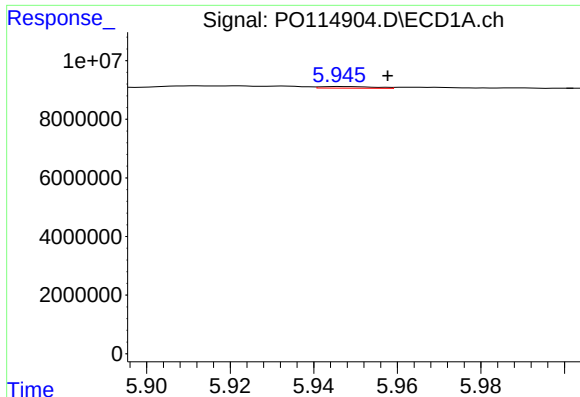

#7 AR-1016-5


R.T.: 5.946 min
Delta R.T.: -0.011 min
Response: 498406
Conc: 2.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

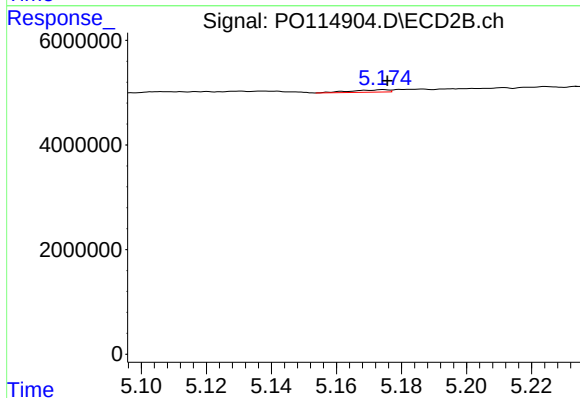


#7 AR-1016-5

R.T.: 5.175 min
Delta R.T.: -0.001 min
Response: 347942
Conc: 2.28 ng/ml

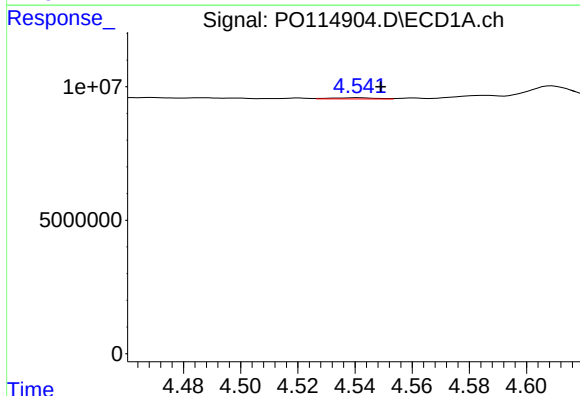


#8 AR-1221-1

R.T.: 4.541 min
Delta R.T.: -0.008 min
Response: 472909
Conc: 5.62 ng/ml

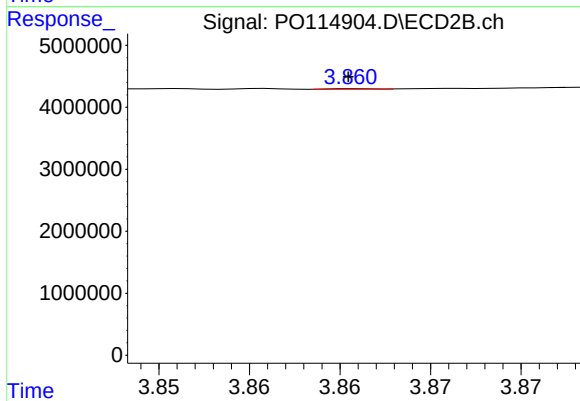

#8 AR-1221-1


R.T.: 3.861 min
Delta R.T.: 0.000 min
Response: 14706
Conc: 0.24 ng/ml

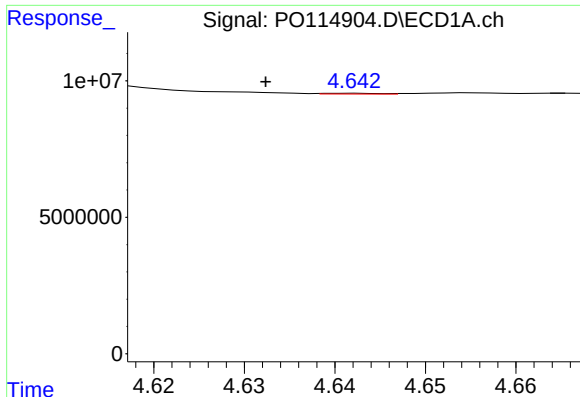

#9 AR-1221-2


R.T.: 4.642 min
Delta R.T.: 0.010 min
Response: 129741
Conc: 2.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

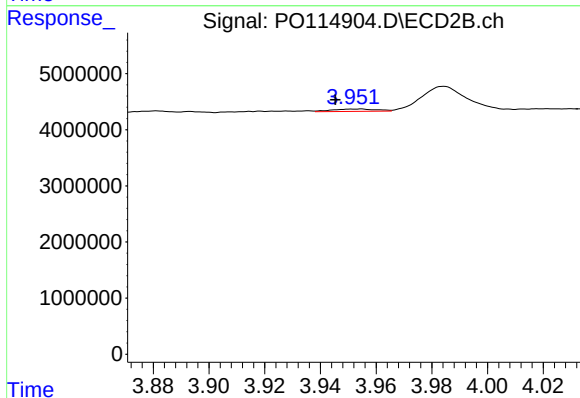


#9 AR-1221-2

R.T.: 3.955 min
Delta R.T.: 0.009 min
Response: 481657
Conc: 10.55 ng/ml

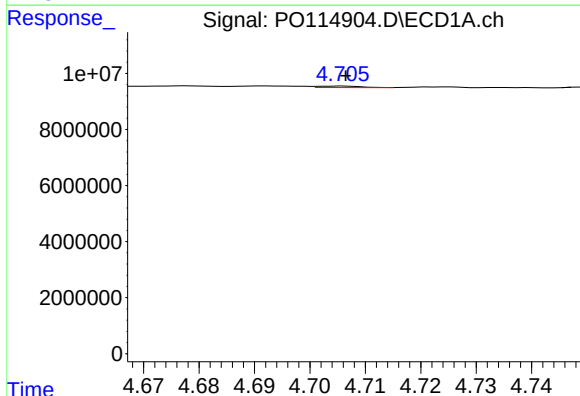


#10 AR-1221-3

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 287005
Conc: 1.48 ng/ml

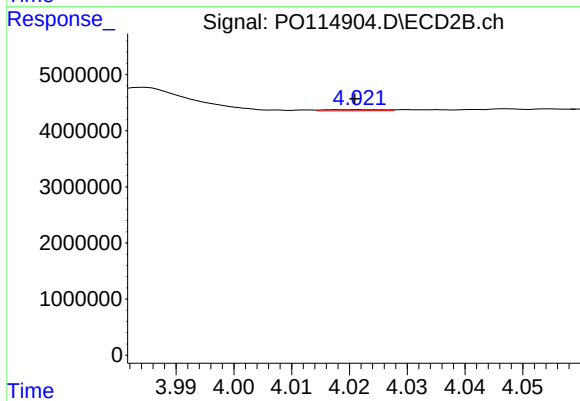

#10 AR-1221-3


R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 133569
Conc: 0.95 ng/ml

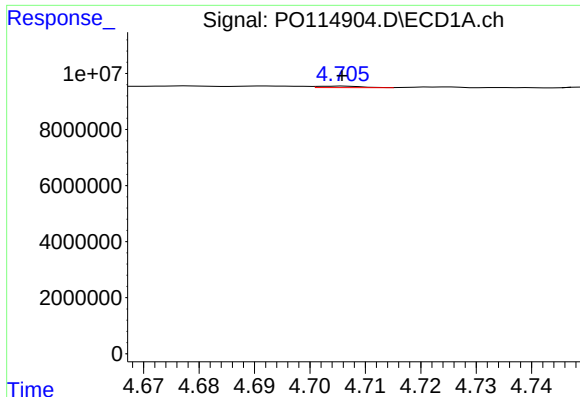

#11 AR-1232-1


R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 287005
Conc: 1.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

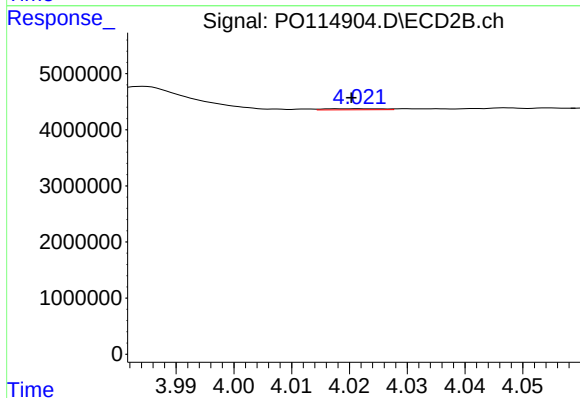


#11 AR-1232-1

R.T.: 4.021 min
Delta R.T.: 0.001 min
Response: 133569
Conc: 1.20 ng/ml

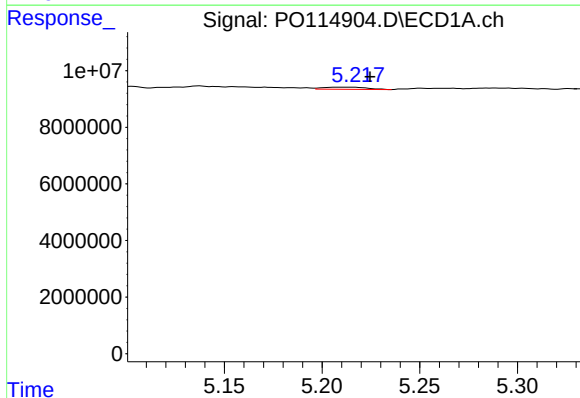


#12 AR-1232-2

R.T.: 5.212 min
Delta R.T.: -0.012 min
Response: 1153721
Conc: 15.90 ng/ml

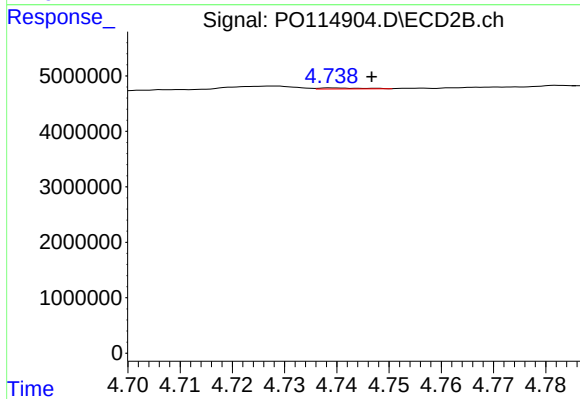

#12 AR-1232-2


R.T.: 4.739 min
Delta R.T.: -0.007 min
Response: 95995
Conc: 0.86 ng/ml

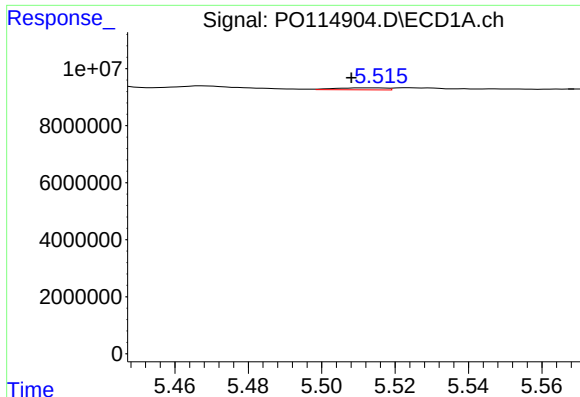

#13 AR-1232-3


R.T.: 5.513 min
Delta R.T.: 0.005 min
Response: 686414
Conc: 4.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

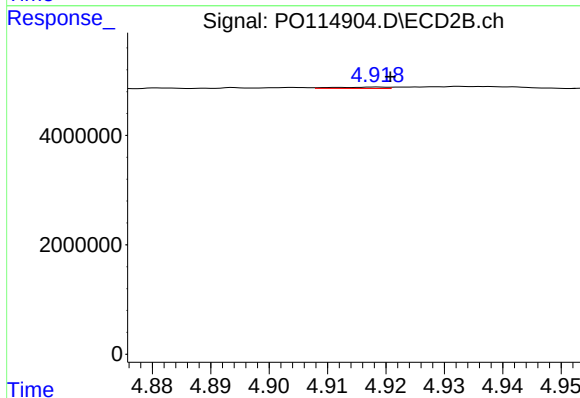


#13 AR-1232-3

R.T.: 4.918 min
Delta R.T.: -0.002 min
Response: 151117
Conc: 2.53 ng/ml

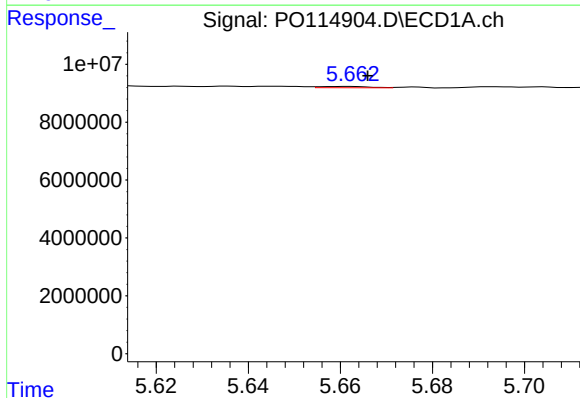


#14 AR-1232-4

R.T.: 5.662 min
Delta R.T.: -0.004 min
Response: 338026
Conc: 4.58 ng/ml

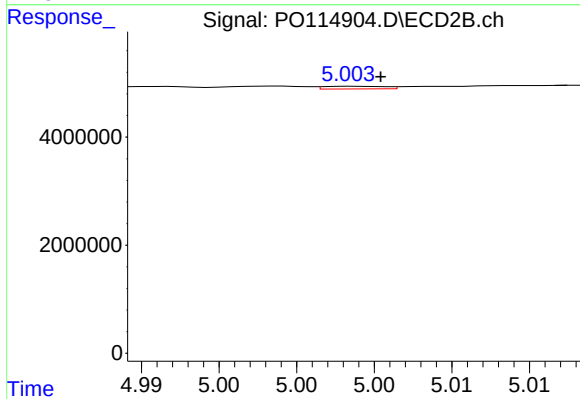

#14 AR-1232-4


R.T.: 5.004 min
Delta R.T.: -0.002 min
Response: 135841
Conc: 2.67 ng/ml

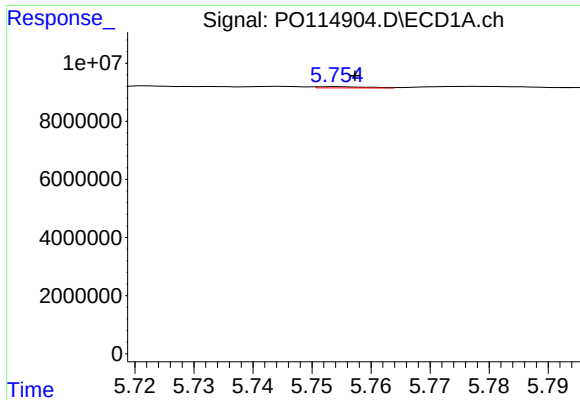

#15 AR-1232-5


R.T.: 5.754 min
Delta R.T.: -0.003 min
Response: 250886
Conc: 4.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

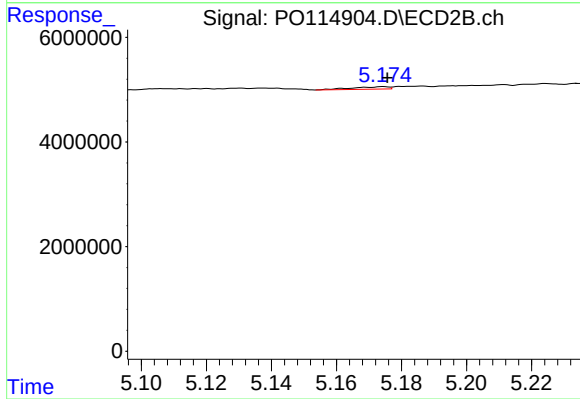


#15 AR-1232-5

R.T.: 5.175 min
Delta R.T.: -0.001 min
Response: 347942
Conc: 6.15 ng/ml

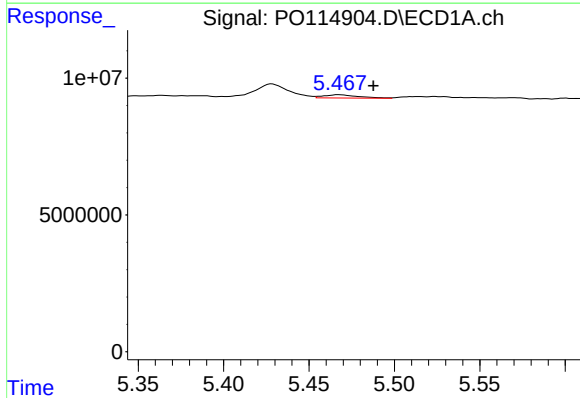


#16 AR-1242-1

R.T.: 5.468 min
Delta R.T.: -0.020 min
Response: 1700245
Conc: 9.13 ng/ml

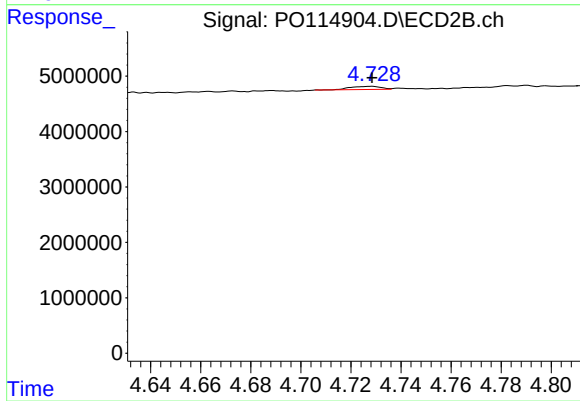

#16 AR-1242-1


R.T.: 4.728 min
Delta R.T.: 0.000 min
Response: 490647
Conc: 3.36 ng/ml

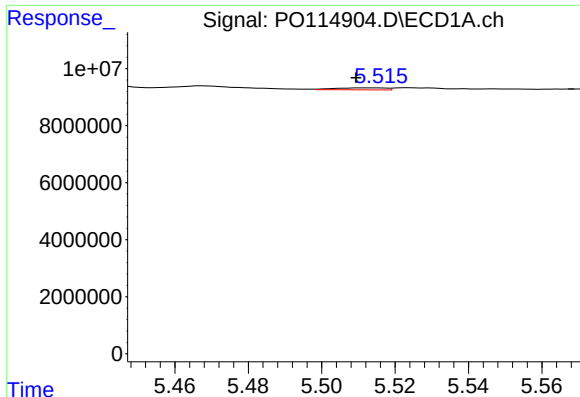

#17 AR-1242-2


R.T.: 5.513 min
Delta R.T.: 0.004 min
Response: 686414
Conc: 2.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

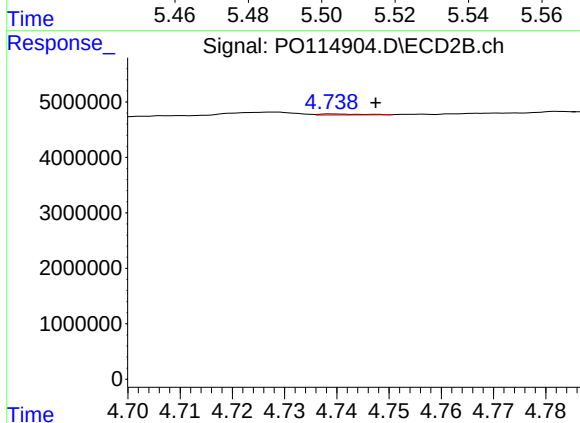


#17 AR-1242-2

R.T.: 4.739 min
Delta R.T.: -0.008 min
Response: 95995
Conc: 0.46 ng/ml

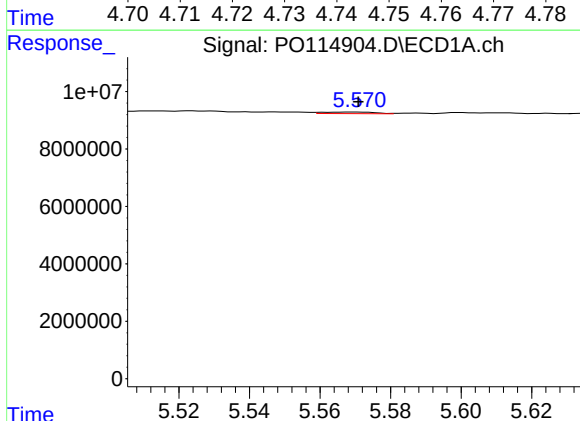


#18 AR-1242-3

R.T.: 5.569 min
Delta R.T.: -0.001 min
Response: 582925
Conc: 3.40 ng/ml

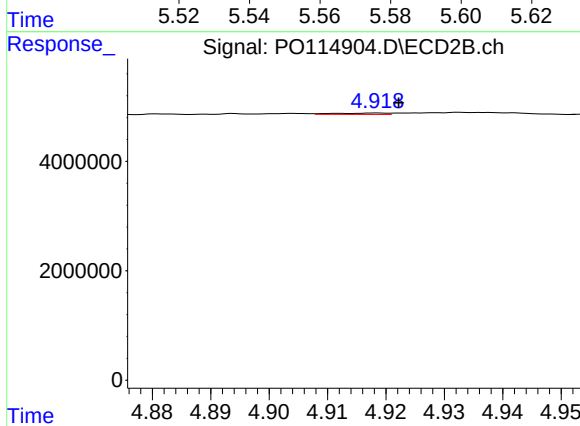

#18 AR-1242-3


R.T.: 4.918 min
Delta R.T.: -0.004 min
Response: 151117
Conc: 1.35 ng/ml

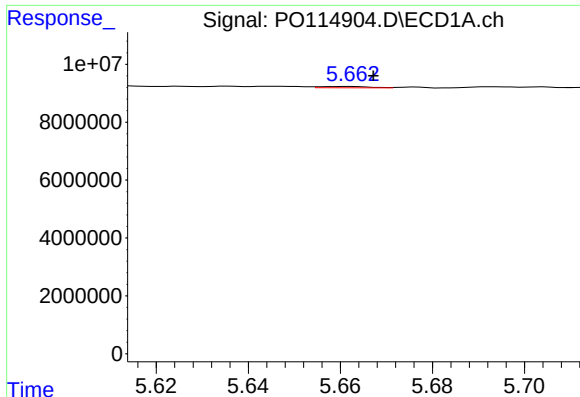

#19 AR-1242-4


R.T.: 5.662 min
Delta R.T.: -0.005 min
Response: 338026
Conc: 2.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

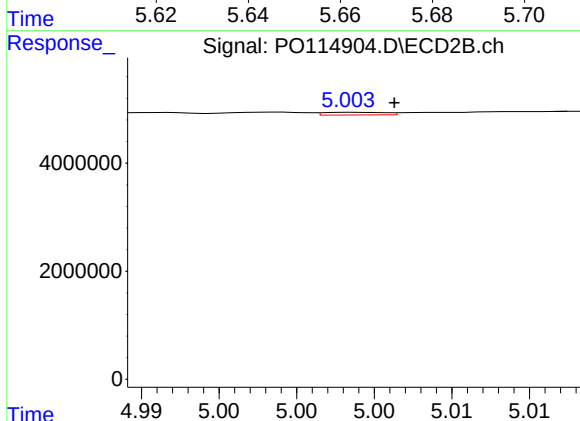


#19 AR-1242-4

R.T.: 5.004 min
Delta R.T.: -0.003 min
Response: 135841
Conc: 1.27 ng/ml

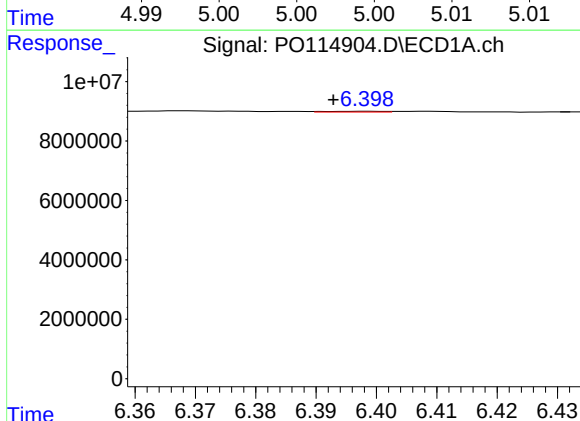


#20 AR-1242-5

R.T.: 6.398 min
Delta R.T.: 0.005 min
Response: 166983
Conc: 1.18 ng/ml

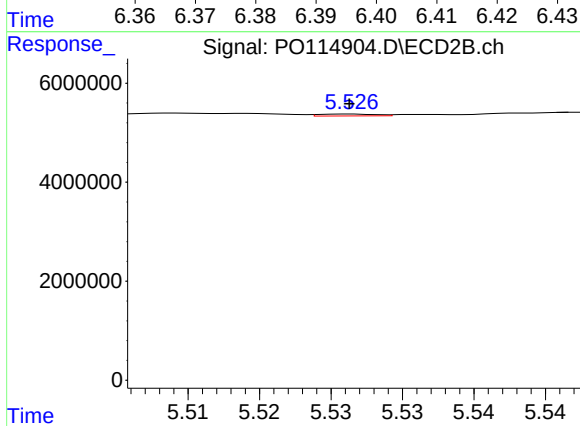

#20 AR-1242-5


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 101966
Conc: 0.71 ng/ml

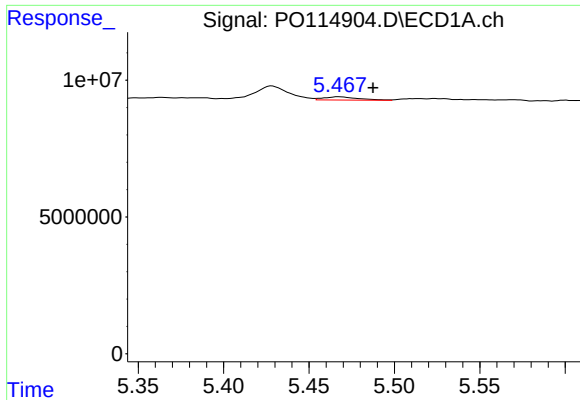

#21 AR-1248-1


R.T.: 5.468 min
Delta R.T.: -0.020 min
Response: 1700245
Conc: 12.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

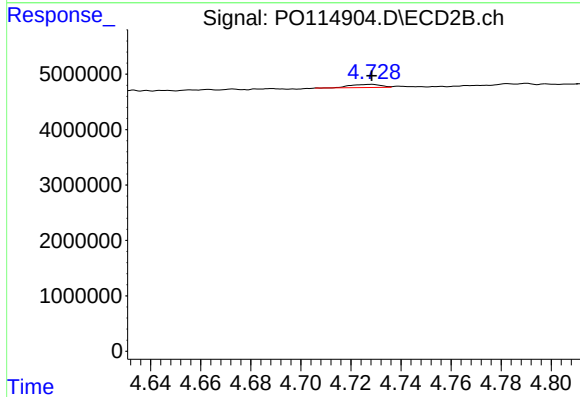


#21 AR-1248-1

R.T.: 4.728 min
Delta R.T.: 0.000 min
Response: 490647
Conc: 4.49 ng/ml

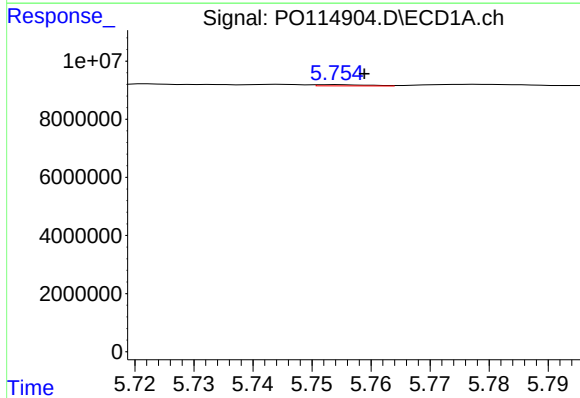


#22 AR-1248-2

R.T.: 5.754 min
Delta R.T.: -0.005 min
Response: 250886
Conc: 1.29 ng/ml

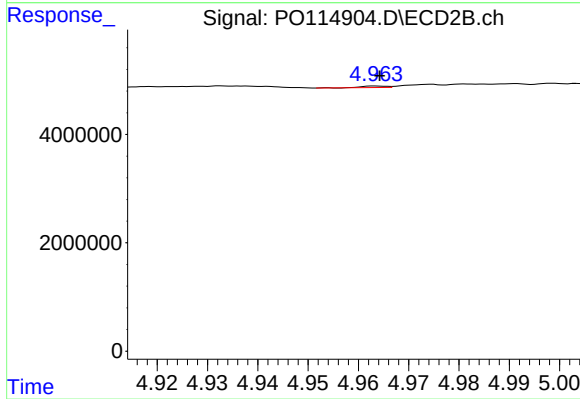

#22 AR-1248-2


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 97657
Conc: 0.66 ng/ml

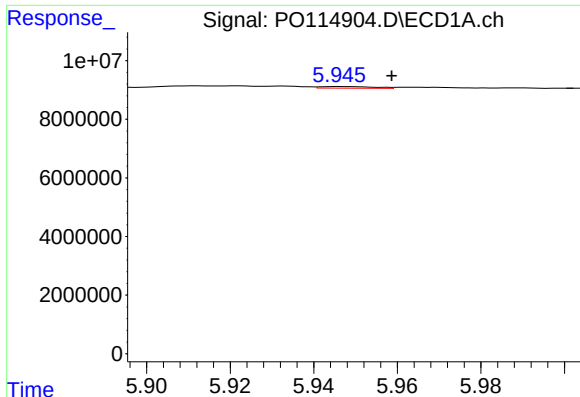

#23 AR-1248-3


R.T.: 5.946 min
Delta R.T.: -0.012 min
Response: 498406
Conc: 2.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

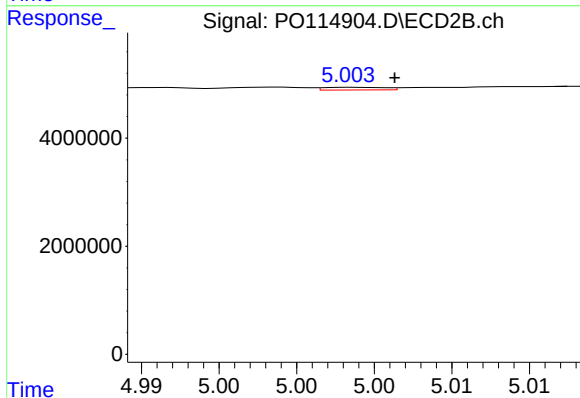


#23 AR-1248-3

R.T.: 5.004 min
Delta R.T.: -0.003 min
Response: 135841
Conc: 0.87 ng/ml

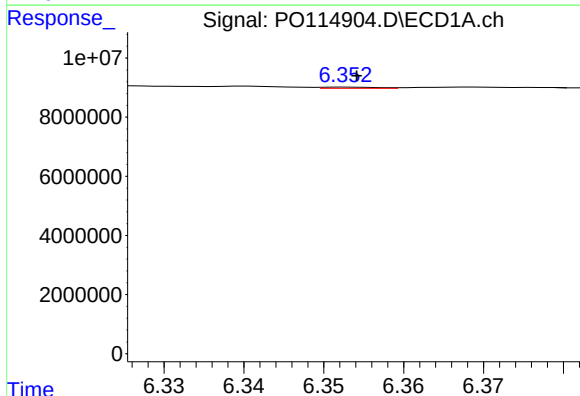


#24 AR-1248-4

R.T.: 6.353 min
Delta R.T.: -0.001 min
Response: 186420
Conc: 0.74 ng/ml

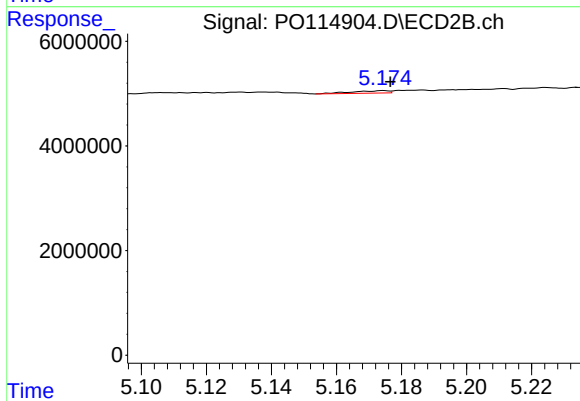

#24 AR-1248-4


R.T.: 5.175 min
Delta R.T.: -0.002 min
Response: 347942
Conc: 1.90 ng/ml

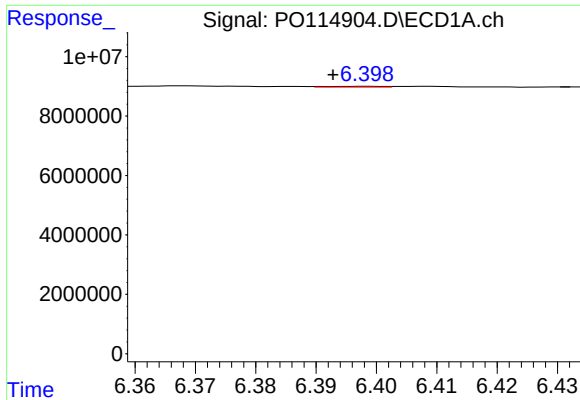

#25 AR-1248-5


R.T.: 6.398 min
Delta R.T.: 0.005 min
Response: 166983
Conc: 0.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

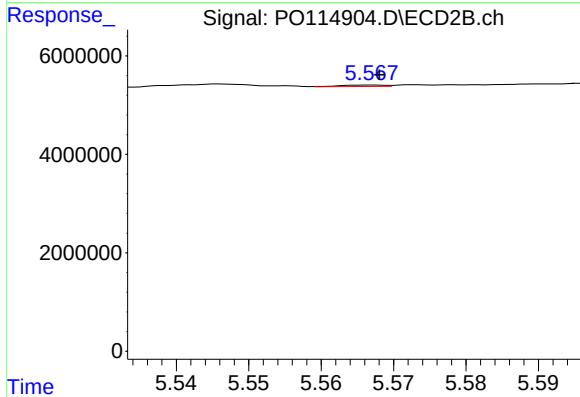


#25 AR-1248-5

R.T.: 5.567 min
Delta R.T.: 0.000 min
Response: 126125
Conc: 0.68 ng/ml

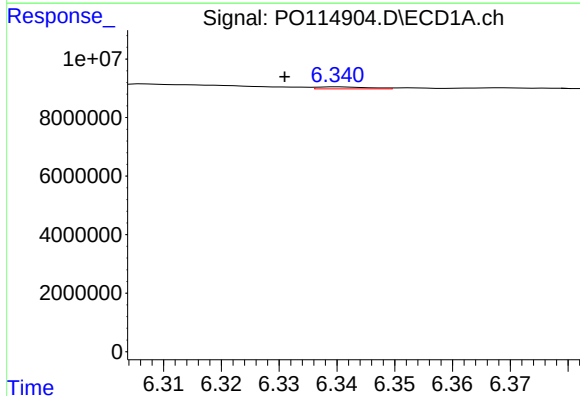


#26 AR-1254-1

R.T.: 6.340 min
Delta R.T.: 0.009 min
Response: 440575
Conc: 1.69 ng/ml

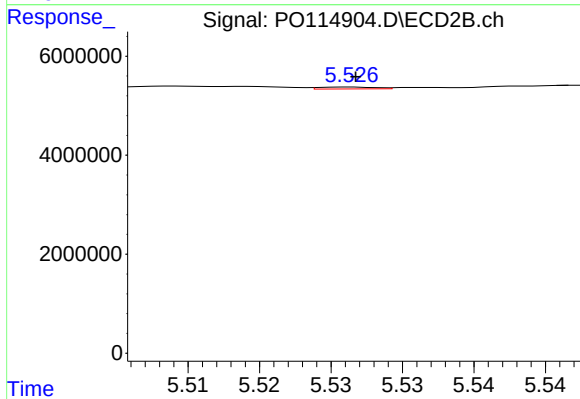

#26 AR-1254-1


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 101966
Conc: 0.34 ng/ml

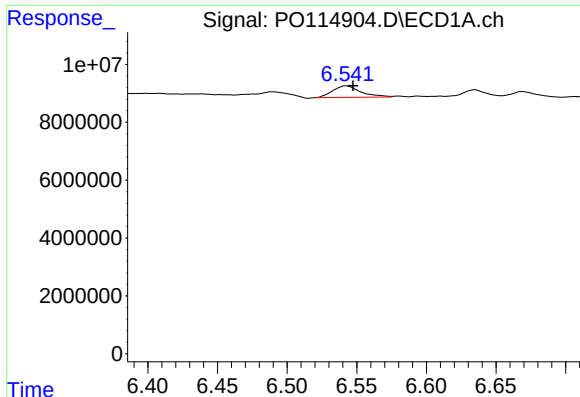

#27 AR-1254-2


R.T.: 6.542 min
Delta R.T.: -0.005 min
Response: 5628319
Conc: 15.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

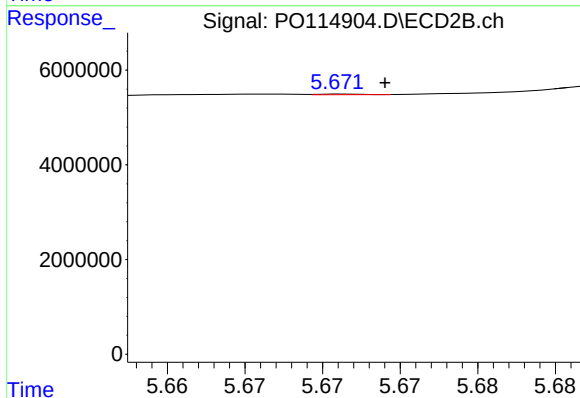


#27 AR-1254-2

R.T.: 5.671 min
Delta R.T.: -0.003 min
Response: 26694
Conc: 0.10 ng/ml

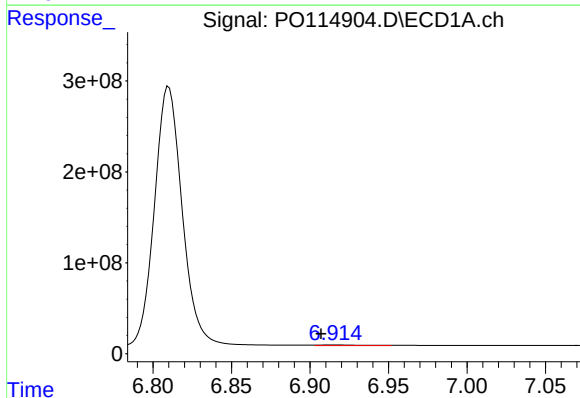


#28 AR-1254-3

R.T.: 6.915 min
Delta R.T.: 0.009 min
Response: 13634801
Conc: 35.43 ng/ml

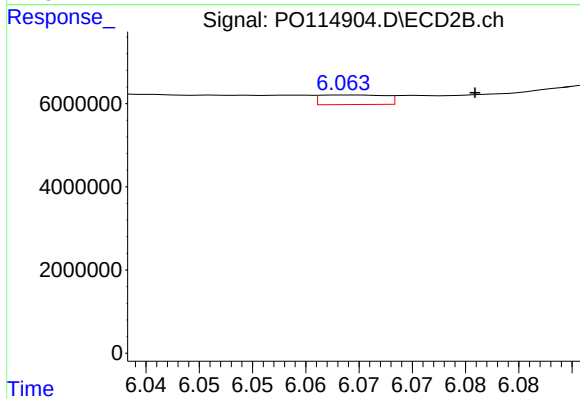

#28 AR-1254-3


R.T.: 6.064 min
Delta R.T.: -0.012 min
Response: 976839
Conc: 2.31 ng/ml

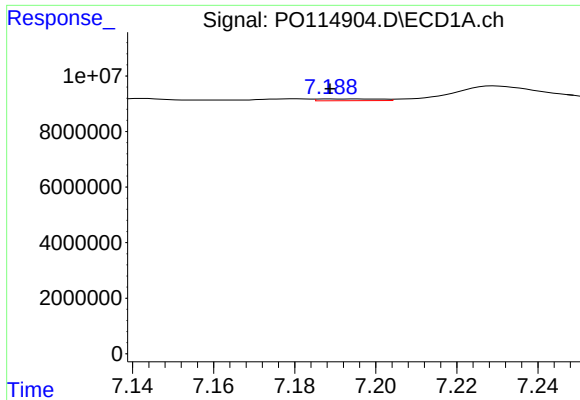

#29 AR-1254-4


R.T.: 7.189 min
Delta R.T.: 0.000 min
Response: 658871
Conc: 1.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

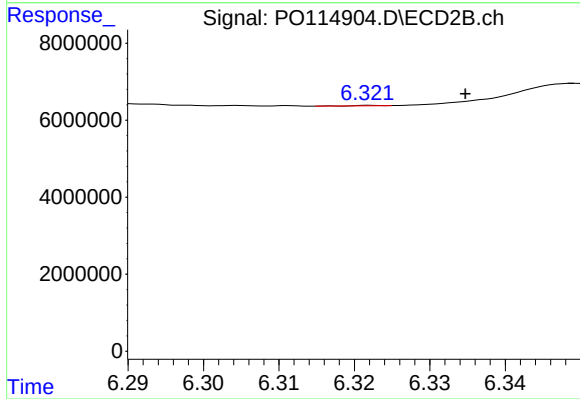


#29 AR-1254-4

R.T.: 6.322 min
Delta R.T.: -0.013 min
Response: 24481
Conc: 0.53 ng/ml

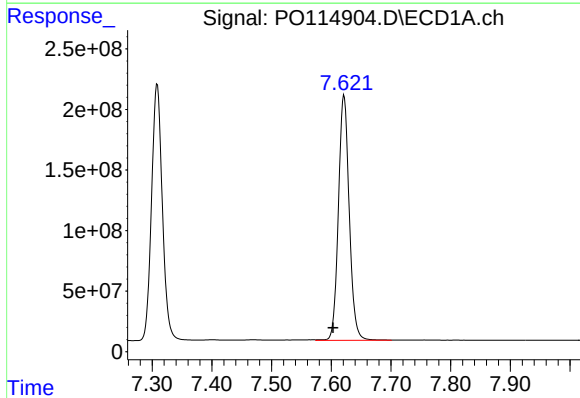


#30 AR-1254-5

R.T.: 7.621 min
Delta R.T.: 0.018 min
Response: 2550949745
Conc: 8450.96 ng/ml

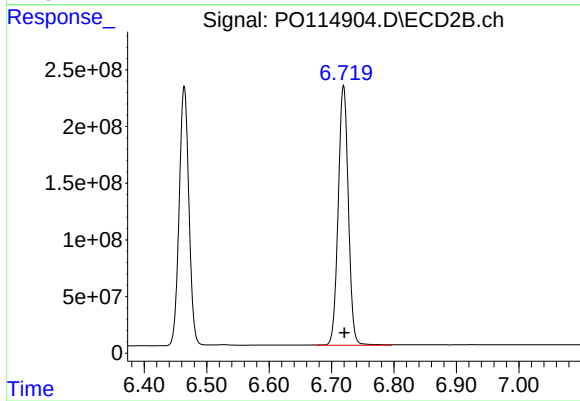

#30 AR-1254-5


R.T.: 6.719 min
Delta R.T.: -0.001 min
Response: 2583490260
Conc: 6498.92 ng/ml

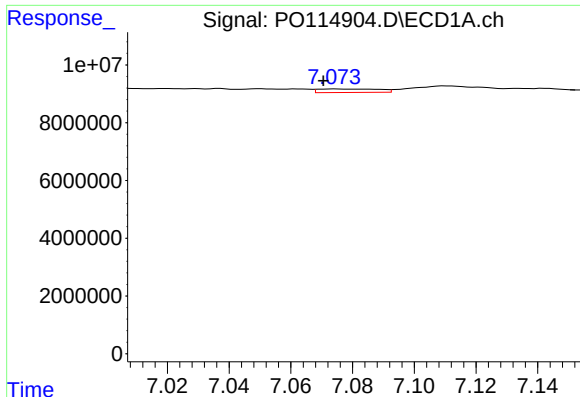

#31 AR-1260-1


R.T.: 7.074 min
Delta R.T.: 0.004 min
Response: 1689589
Conc: 5.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

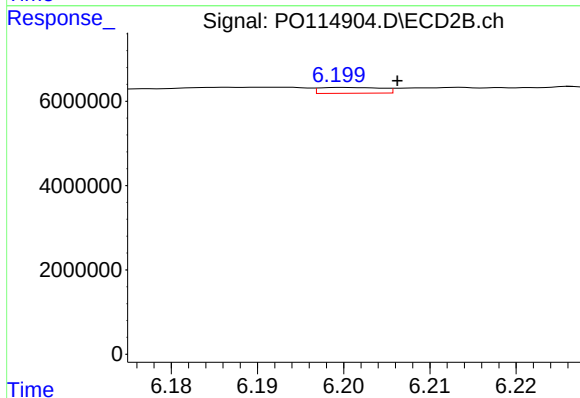


#31 AR-1260-1

R.T.: 6.200 min
Delta R.T.: -0.006 min
Response: 693263
Conc: 2.34 ng/ml

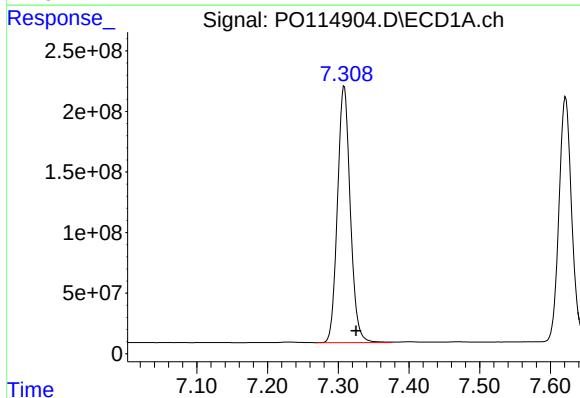


#32 AR-1260-2

R.T.: 7.308 min
Delta R.T.: -0.017 min
Response: 2664127743
Conc: 6729.68 ng/ml

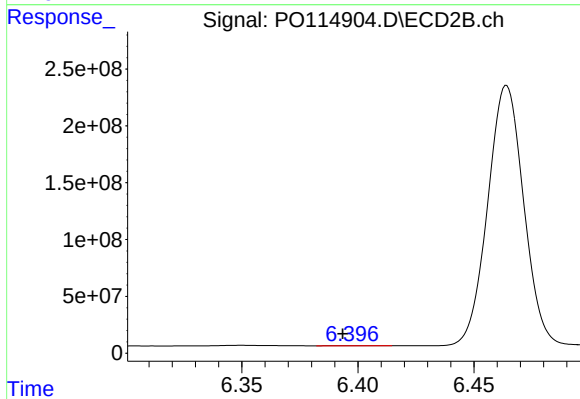

#32 AR-1260-2


R.T.: 6.397 min
Delta R.T.: 0.003 min
Response: 1361002
Conc: 3.16 ng/ml

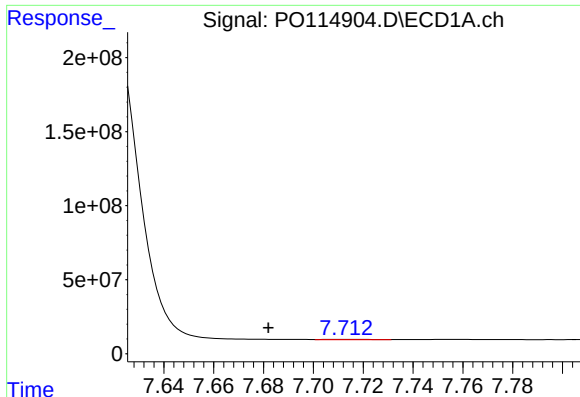

#33 AR-1260-3


R.T.: 7.713 min
Delta R.T.: 0.031 min
Response: 3283204
Conc: 9.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

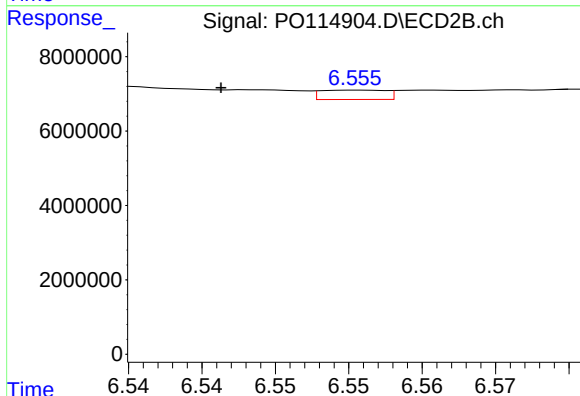


#33 AR-1260-3

R.T.: 6.556 min
Delta R.T.: 0.010 min
Response: 774049
Conc: 2.20 ng/ml

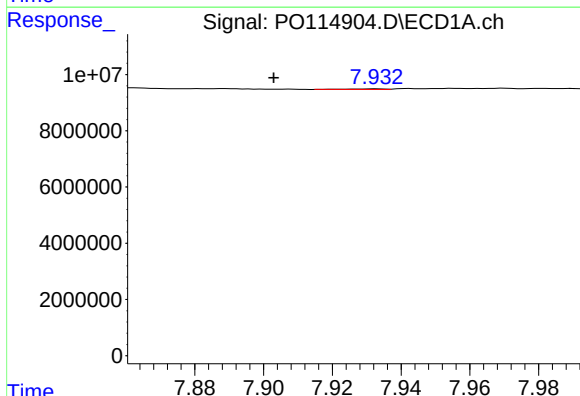


#34 AR-1260-4

R.T.: 7.933 min
Delta R.T.: 0.030 min
Response: 195325
Conc: 0.64 ng/ml

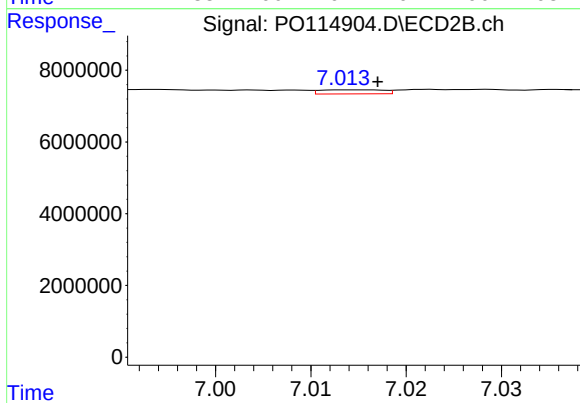

#34 AR-1260-4


R.T.: 7.014 min
Delta R.T.: -0.003 min
Response: 523809
Conc: 1.73 ng/ml

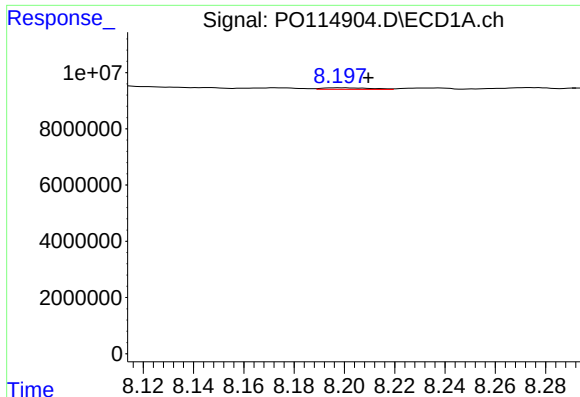

#35 AR-1260-5


R.T.: 8.199 min
Delta R.T.: -0.011 min
Response: 790948
Conc: 1.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

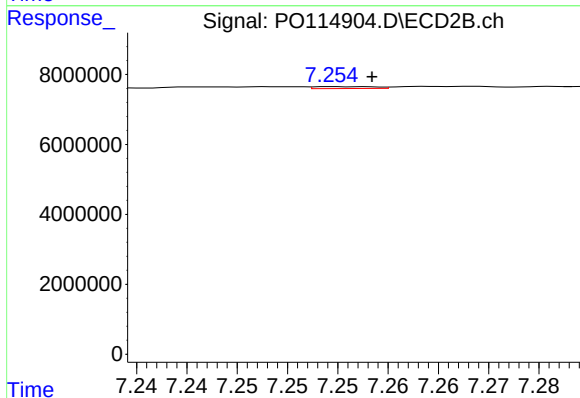


#35 AR-1260-5

R.T.: 7.255 min
Delta R.T.: -0.004 min
Response: 229963
Conc: 0.28 ng/ml

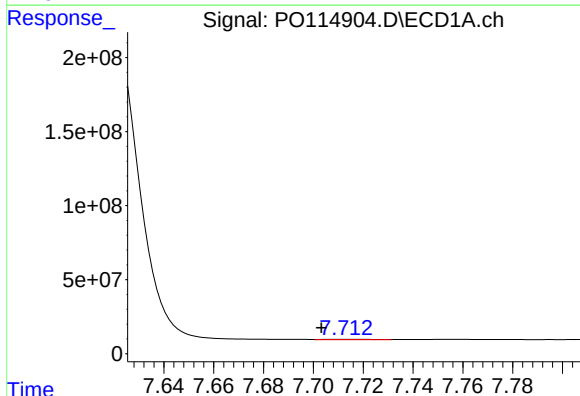


#36 AR-1262-1

R.T.: 7.713 min
Delta R.T.: 0.010 min
Response: 3283204
Conc: 7.24 ng/ml

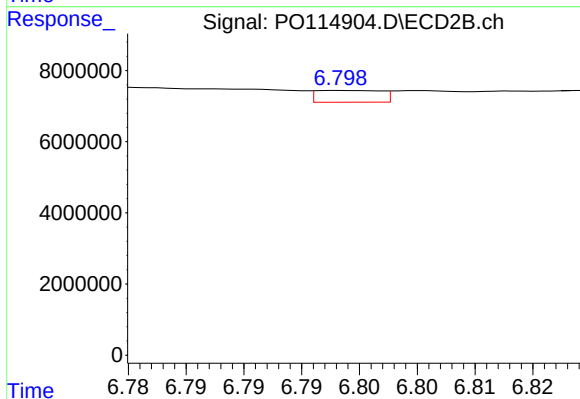

#36 AR-1262-1


R.T.: 6.798 min
Delta R.T.: 0.039 min
Response: 1290033
Conc: 2.61 ng/ml

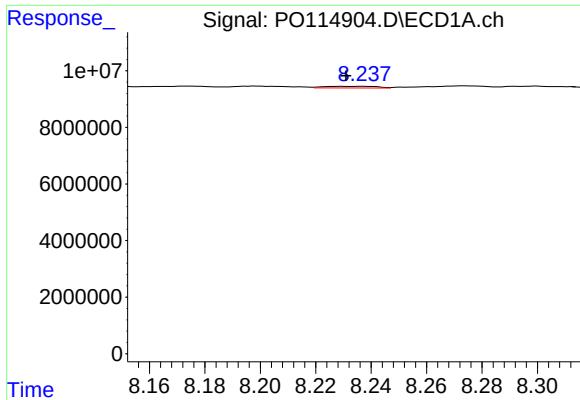

#37 AR-1262-2


R.T.: 8.237 min
Delta R.T.: 0.006 min
Response: 781324
Conc: 1.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

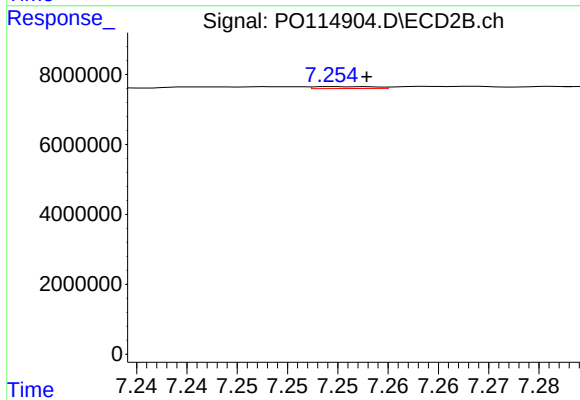


#37 AR-1262-2

R.T.: 7.255 min
Delta R.T.: -0.003 min
Response: 229963
Conc: 0.29 ng/ml

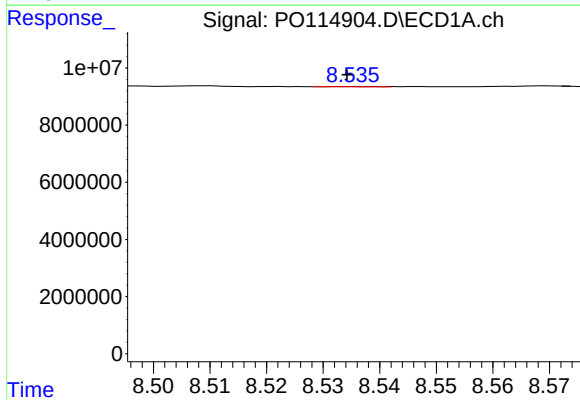


#38 AR-1262-3

R.T.: 8.535 min
Delta R.T.: 0.000 min
Response: 49418
Conc: 0.11 ng/ml

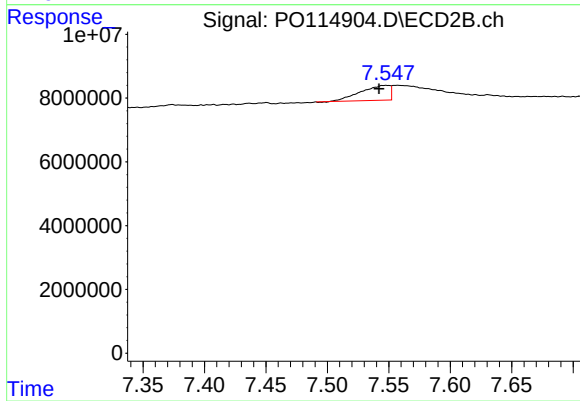

#38 AR-1262-3


R.T.: 7.548 min
Delta R.T.: 0.006 min
Response: 7697694
Conc: 23.40 ng/ml

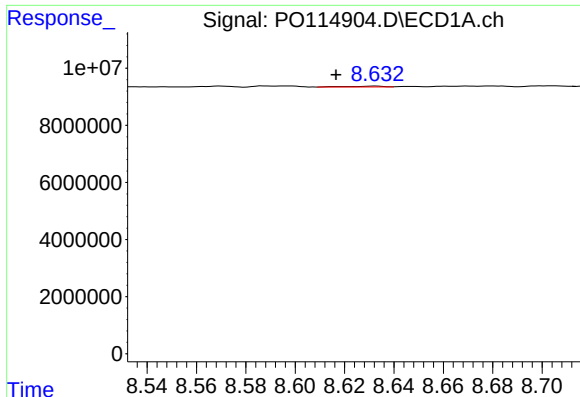

#39 AR-1262-4


R.T.: 8.633 min
Delta R.T.: 0.016 min
Response: 286752
Conc: 0.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

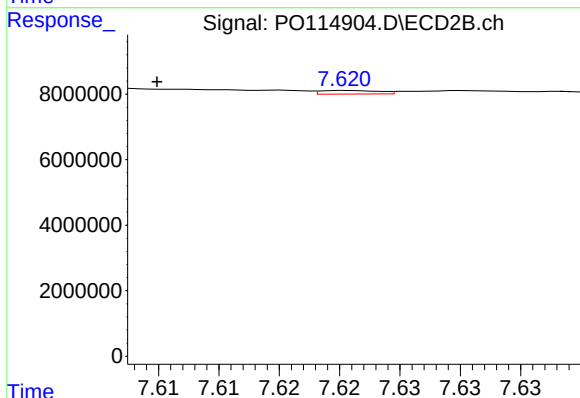


#39 AR-1262-4

R.T.: 7.621 min
Delta R.T.: 0.016 min
Response: 367412
Conc: 0.68 ng/ml

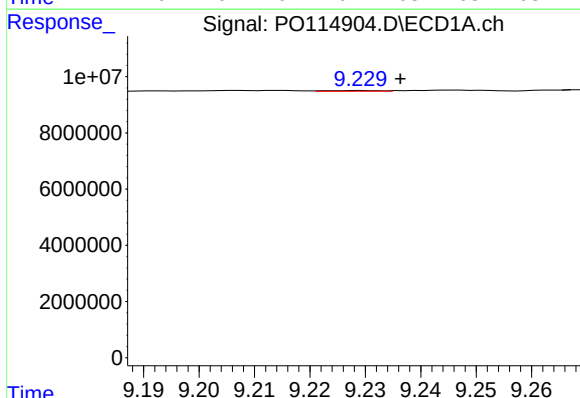


#40 AR-1262-5

R.T.: 9.229 min
Delta R.T.: -0.007 min
Response: 170513
Conc: 0.71 ng/ml

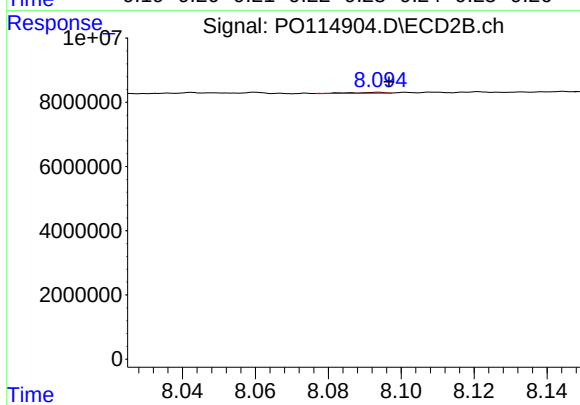

#40 AR-1262-5


R.T.: 8.094 min
Delta R.T.: -0.003 min
Response: 179791
Conc: 0.76 ng/ml

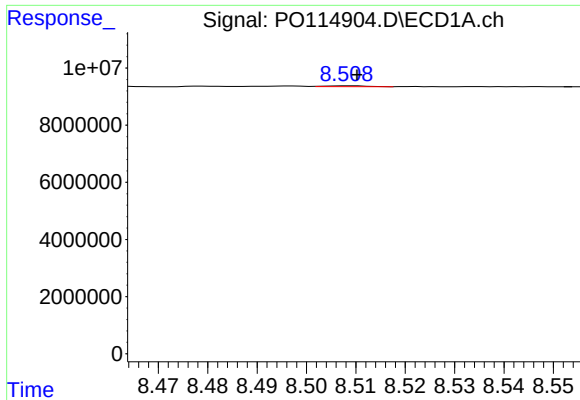

#41 AR-1268-1


R.T.: 8.509 min
Delta R.T.: -0.002 min
Response: 156111
Conc: 0.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

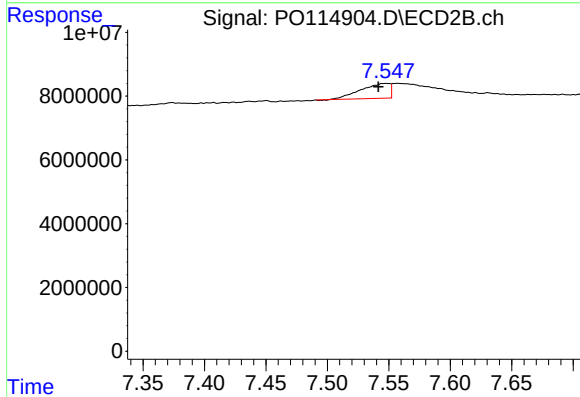


#41 AR-1268-1

R.T.: 7.548 min
Delta R.T.: 0.006 min
Response: 7697694
Conc: 7.89 ng/ml

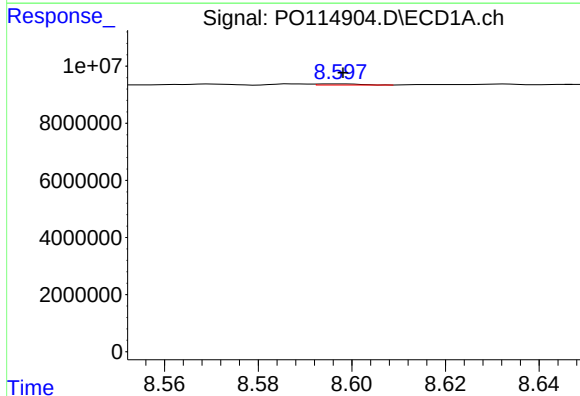


#42 AR-1268-2

R.T.: 8.597 min
Delta R.T.: 0.000 min
Response: 261920
Conc: 0.35 ng/ml

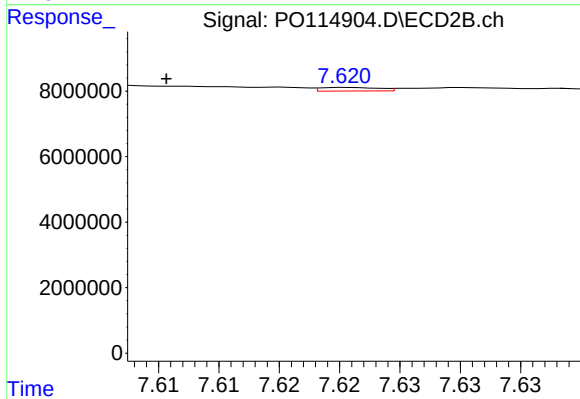

#42 AR-1268-2


R.T.: 7.621 min
Delta R.T.: 0.015 min
Response: 367412
Conc: 0.46 ng/ml

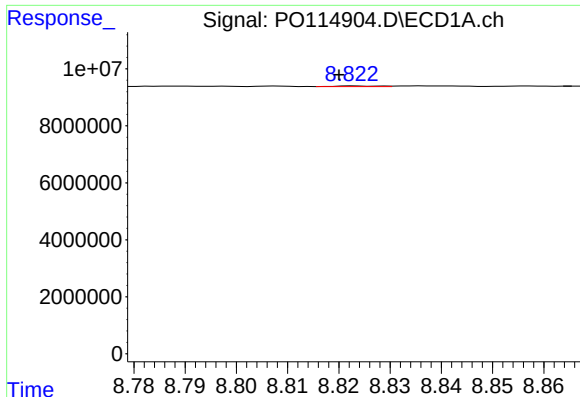

#43 AR-1268-3


R.T.: 8.823 min
Delta R.T.: 0.003 min
Response: 127308
Conc: 0.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

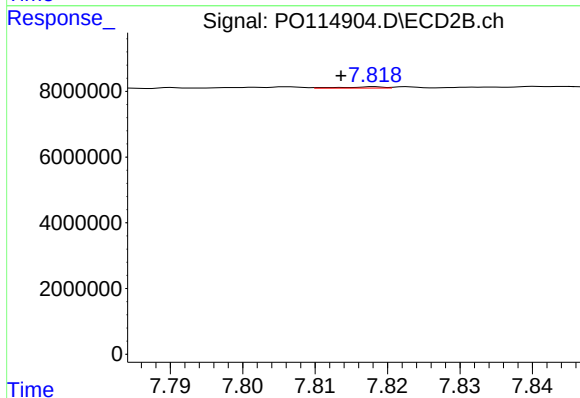


#43 AR-1268-3

R.T.: 7.818 min
Delta R.T.: 0.005 min
Response: 152315
Conc: 0.23 ng/ml

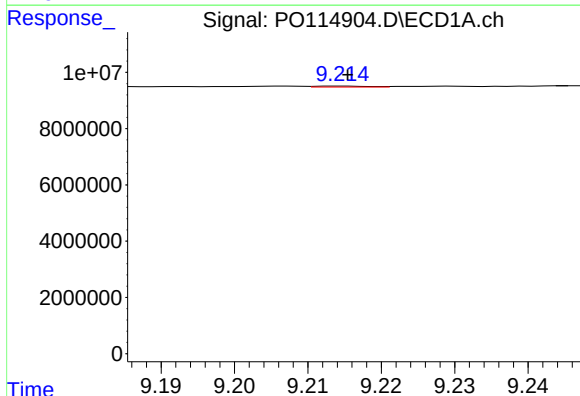


#44 AR-1268-4

R.T.: 9.215 min
Delta R.T.: 0.000 min
Response: 179057
Conc: 0.64 ng/ml

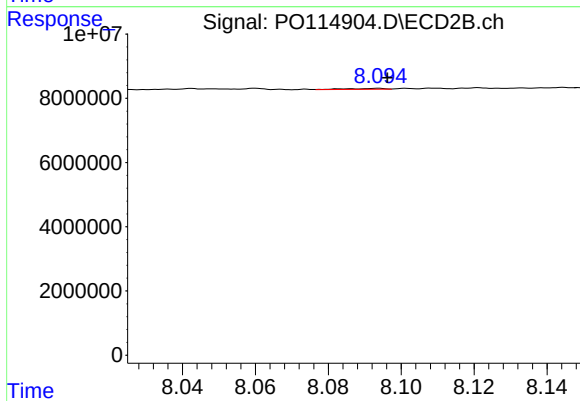

#44 AR-1268-4


R.T.: 8.094 min
Delta R.T.: -0.002 min
Response: 179791
Conc: 0.65 ng/ml

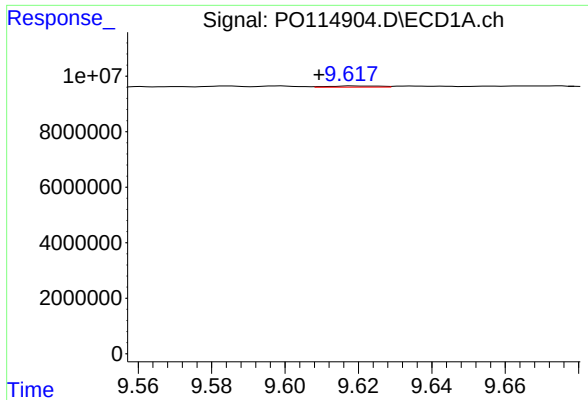

#45 AR-1268-5

R.T.: 9.618 min
Delta R.T.: 0.009 min
Response: 435428
Conc: 0.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

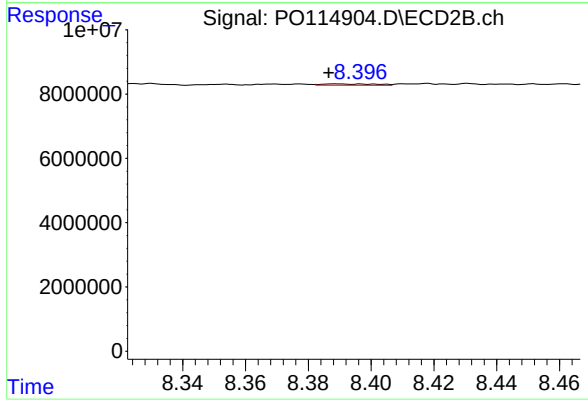

#45 AR-1268-5

R.T.: 8.389 min
Delta R.T.: 0.003 min
Response: 531494
Conc: 0.30 ng/ml