

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110518\
 Data File : PO051094.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 16:13
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 16:28:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 05 12:48:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.345	3.341	11120824	5287842	29.809	26.082
2)	SA Decachlor...	9.992	8.080	7516679	5838397	25.274	26.367
Target Compounds							
7)	L1 AR-1016-5	0.000	4.814	0	320117	N.D.	52.096 #
15)	L3 AR-1232-5	0.000	4.814	0	320117	N.D.	141.035 #
20)	L4 AR-1242-5	0.000	5.136	0	77001	N.D.	11.954 #
24)	L5 AR-1248-4	0.000	4.814	0	320117	N.D.	44.372 #
25)	L5 AR-1248-5	0.000	5.136	0	77001	N.D.	9.853 #
26)	L6 AR-1254-1	0.000	5.136	0	77001	N.D.	5.503 #
43)	L9 AR-1268-3	0.000	7.317	0	46960	N.D.	1.195 #
45)	L9 AR-1268-5	0.000	7.867	0	12417	N.D.	0.123 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110518\
Data File : PO051094.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 16:13
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 16:28:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 05 12:48:11 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

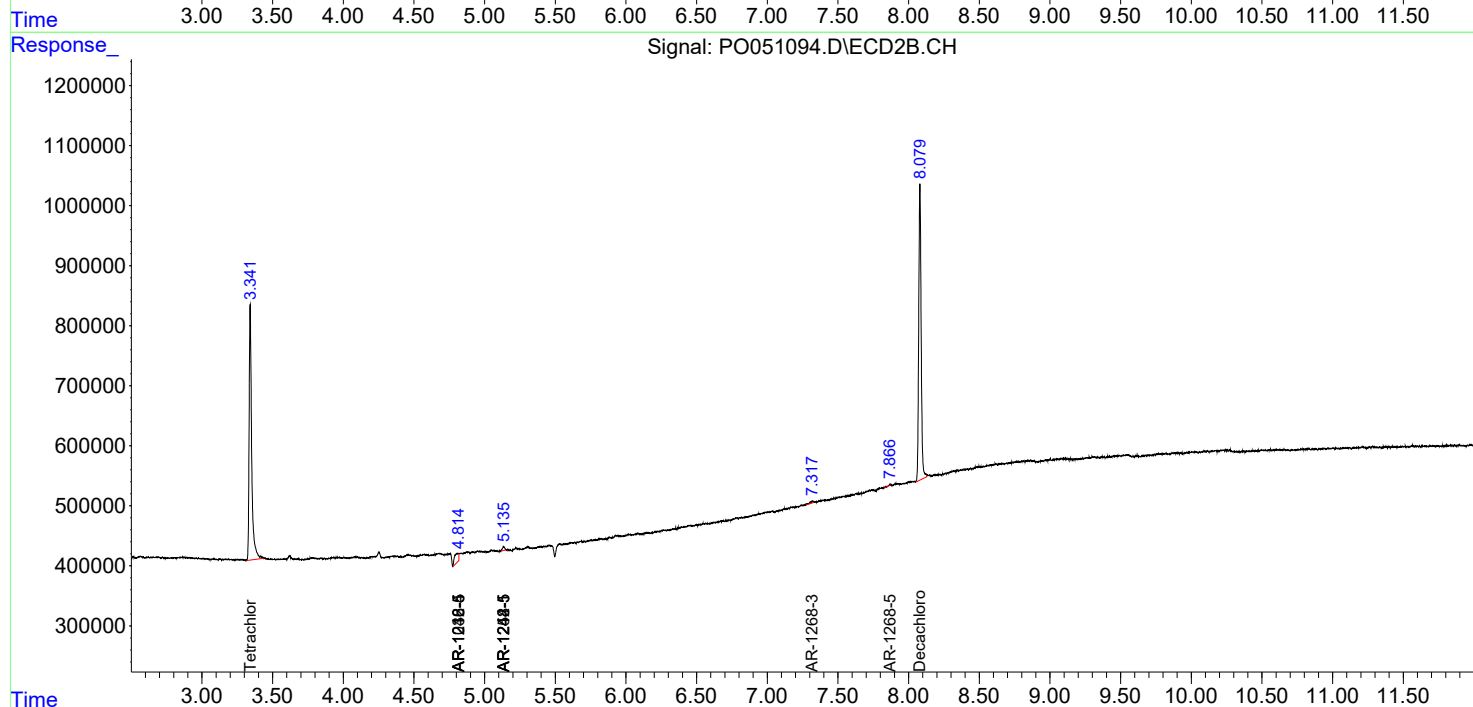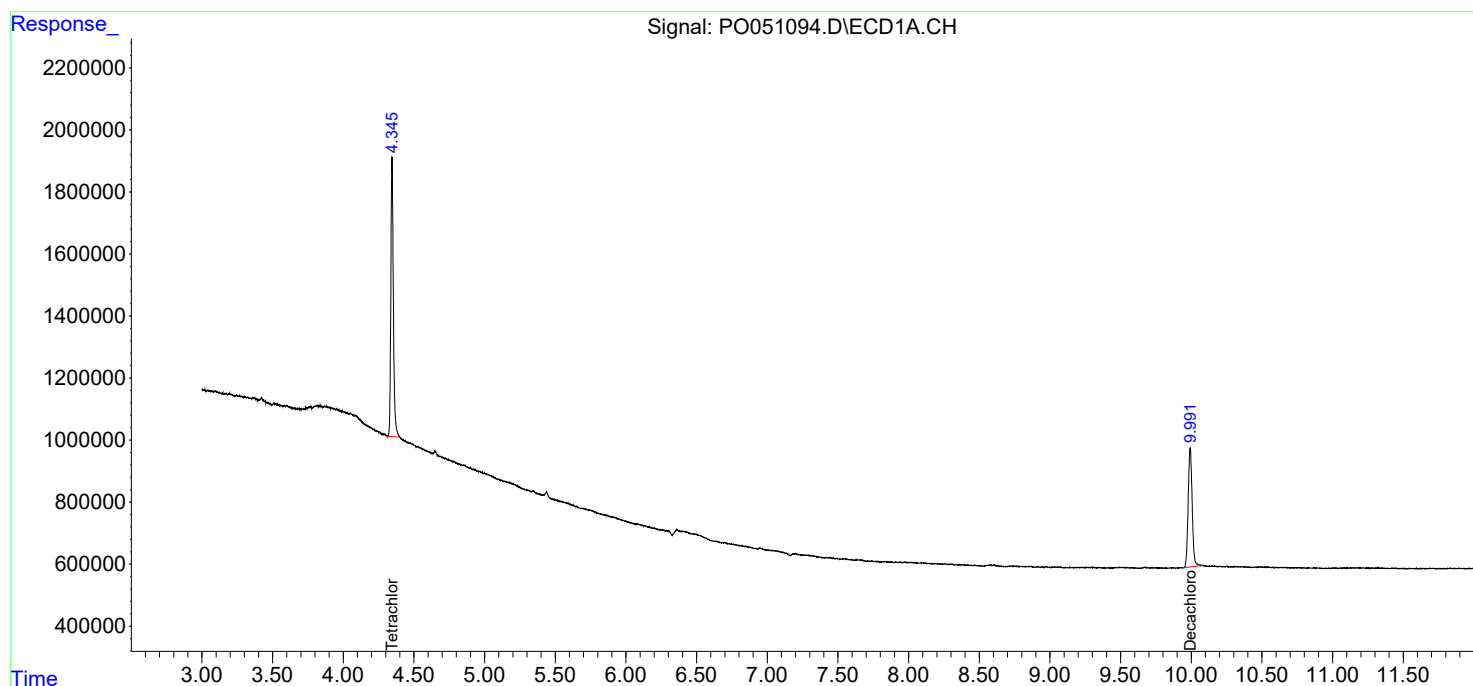


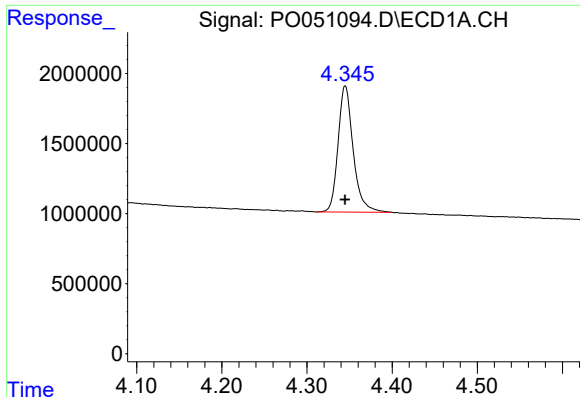

#1 Tetrachloro-m-xylene


R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 11120824
Conc: 29.81 ng/ml

Instrument :
ECD_O
ClientSampleId :

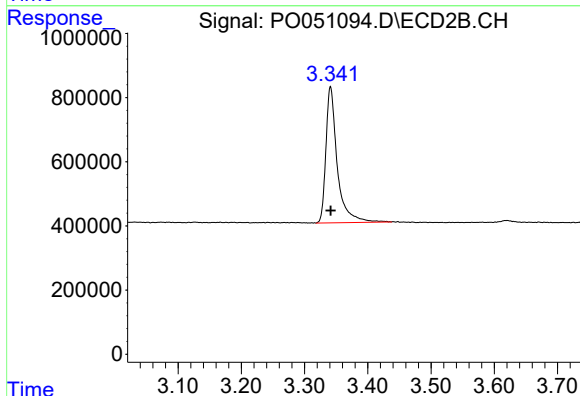


#1 Tetrachloro-m-xylene

R.T.: 3.341 min
Delta R.T.: 0.000 min
Response: 5287842
Conc: 26.08 ng/ml

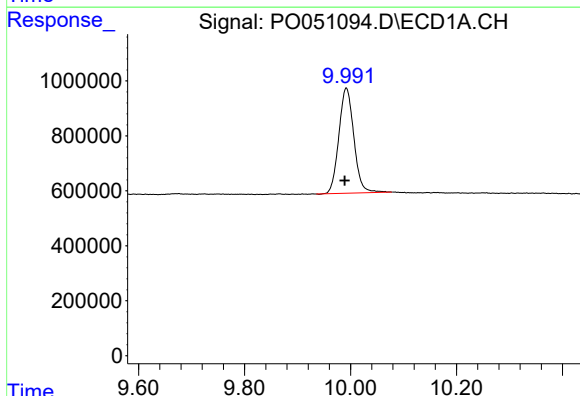


#2 Decachlorobiphenyl

R.T.: 9.992 min
Delta R.T.: 0.003 min
Response: 7516679
Conc: 25.27 ng/ml

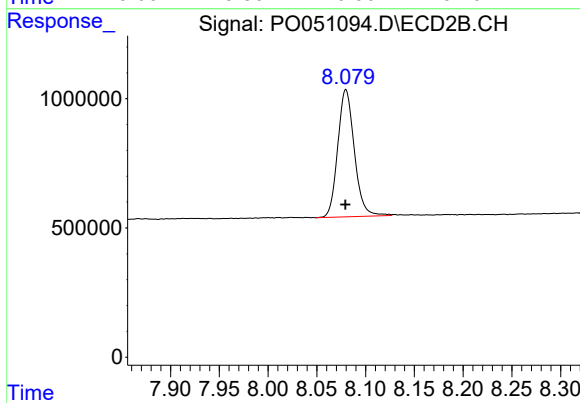

#2 Decachlorobiphenyl


R.T.: 8.080 min
Delta R.T.: 0.000 min
Response: 5838397
Conc: 26.37 ng/ml

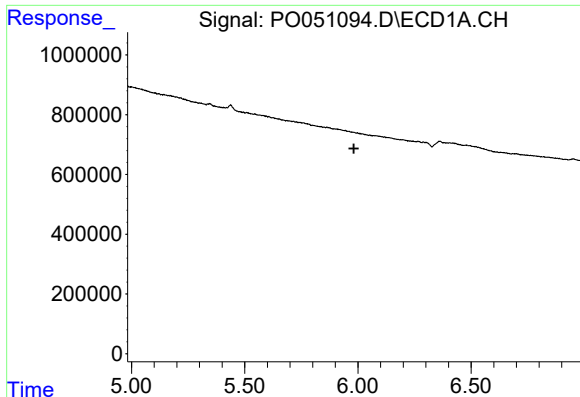

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.982 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

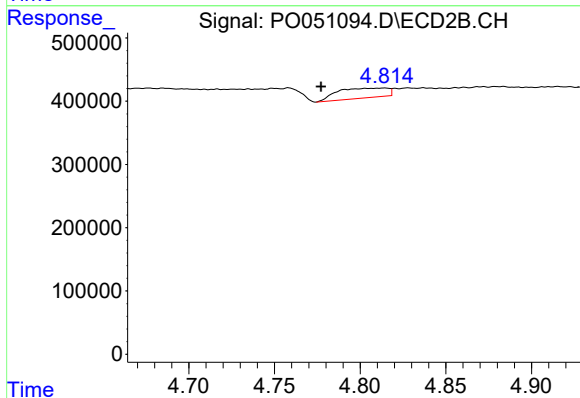


#7 AR-1016-5

R.T.: 4.814 min
Delta R.T.: 0.037 min
Response: 320117
Conc: 52.10 ng/ml

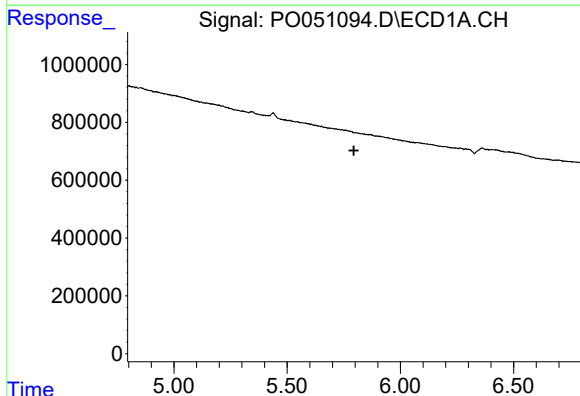


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.794 min
Response: 0
Conc: N.D.

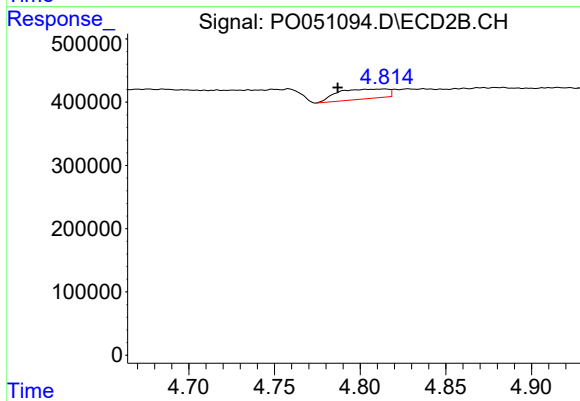

#15 AR-1232-5


R.T.: 4.814 min
Delta R.T.: 0.027 min
Response: 320117
Conc: 141.03 ng/ml

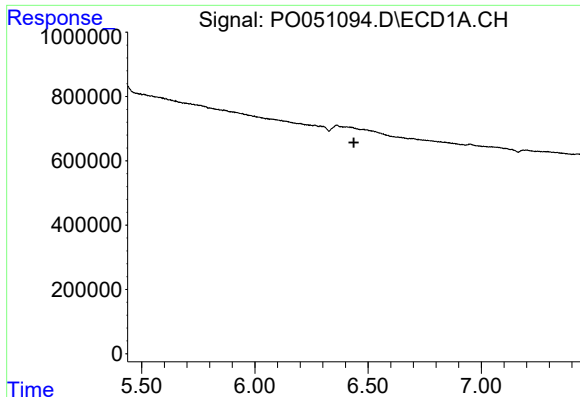

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

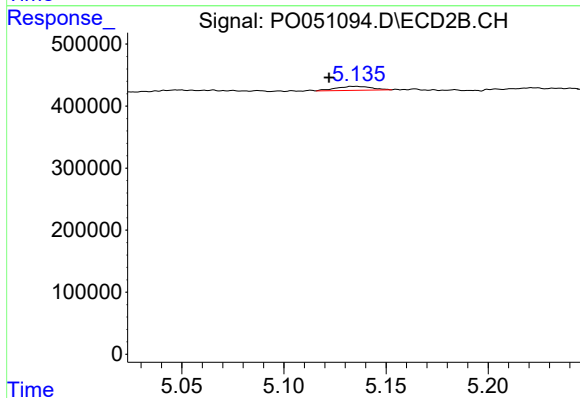


#20 AR-1242-5

R.T.: 5.136 min
Delta R.T.: 0.014 min
Response: 77001
Conc: 11.95 ng/ml

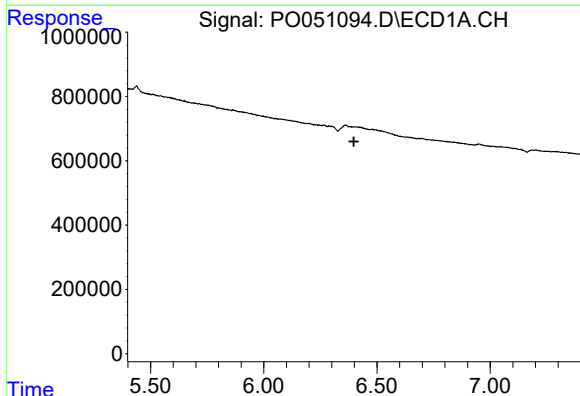


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

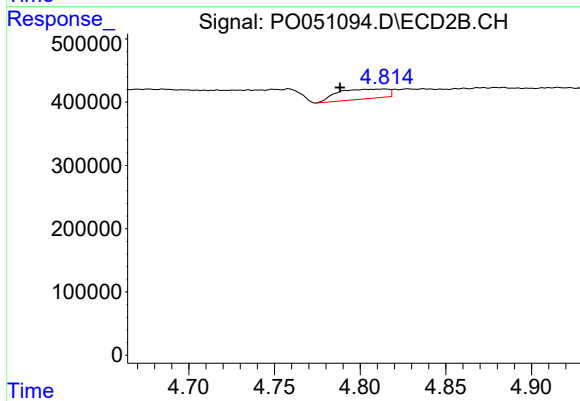

#24 AR-1248-4


R.T.: 4.814 min
Delta R.T.: 0.026 min
Response: 320117
Conc: 44.37 ng/ml

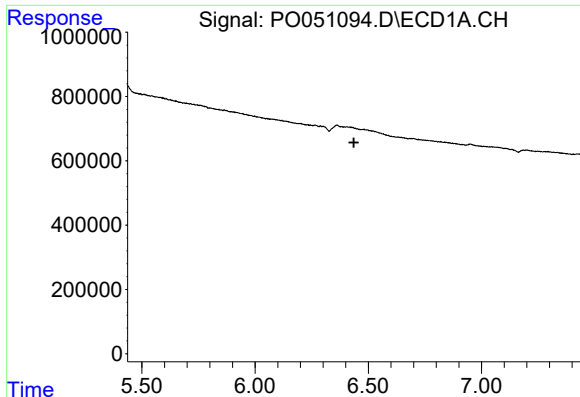

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

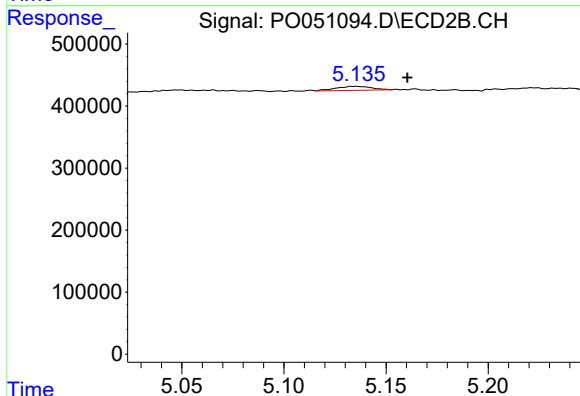


#25 AR-1248-5

R.T.: 5.136 min
Delta R.T.: -0.025 min
Response: 77001
Conc: 9.85 ng/ml

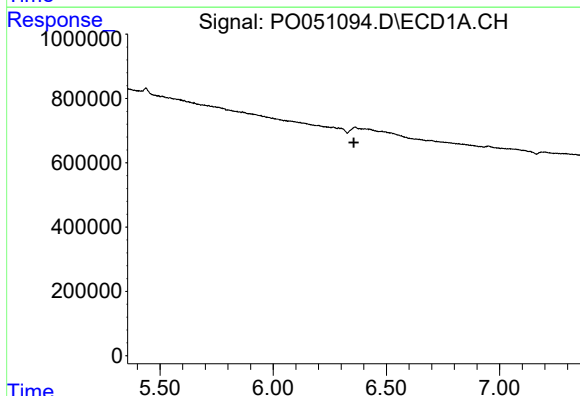


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.356 min
Response: 0
Conc: N.D.

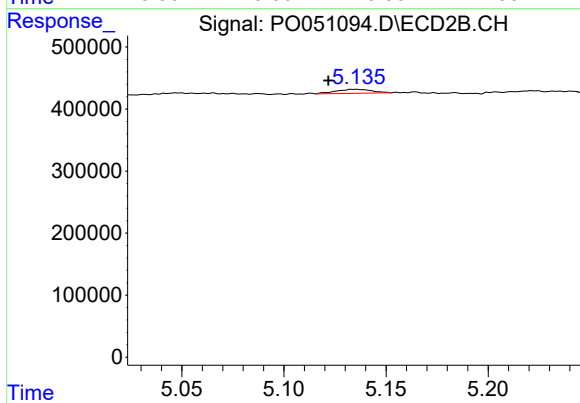

#26 AR-1254-1


R.T.: 5.136 min
Delta R.T.: 0.014 min
Response: 77001
Conc: 5.50 ng/ml

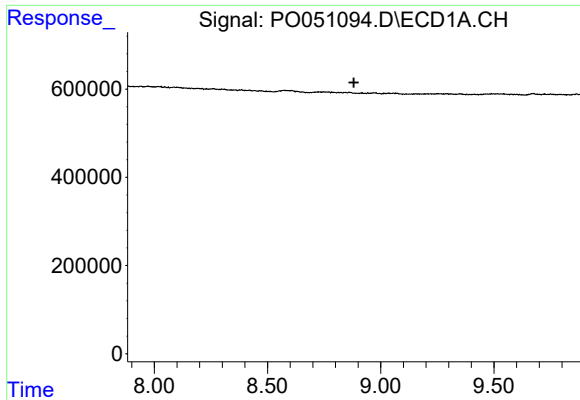

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

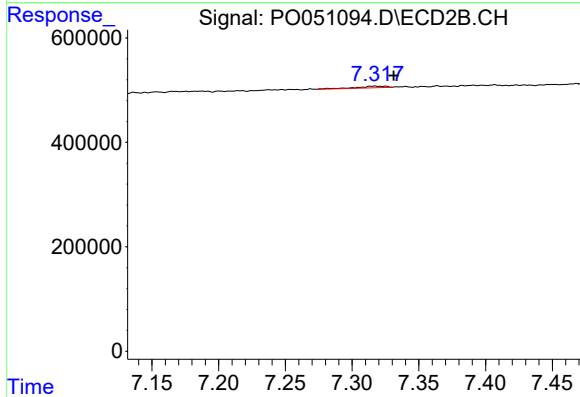


#43 AR-1268-3

R.T.: 7.317 min
Delta R.T.: -0.014 min
Response: 46960
Conc: 1.19 ng/ml

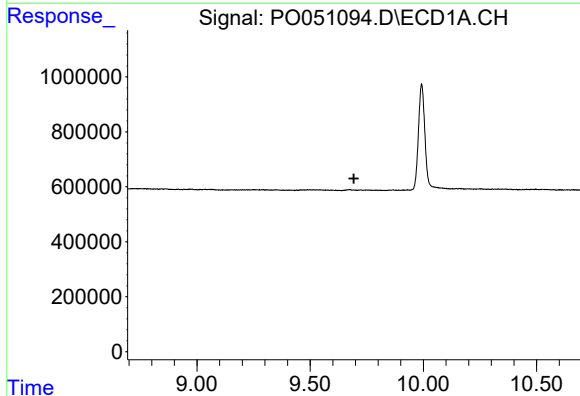

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

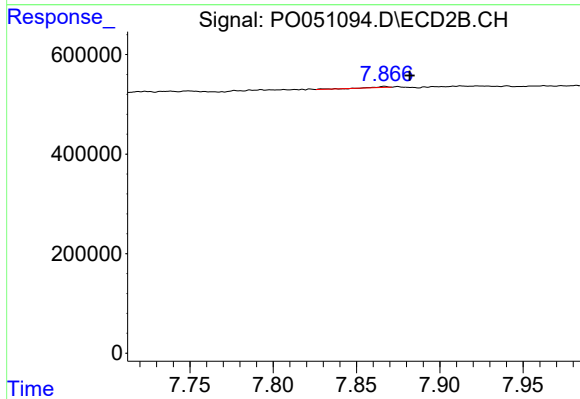

#45 AR-1268-5

R.T.: 7.867 min
Delta R.T.: -0.015 min
Response: 12417
Conc: 0.12 ng/ml