

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110520\
 Data File : PO073099.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2020 11:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:38:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 05:38:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.947	4.021	1269860	818980	23.960	22.919
2)	SA Decachlor...	10.972	9.296	1090255	888521	26.346	26.633
Target Compounds							
24)	L5 AR-1248-4	7.189f	0.000	38228	0	15.812	N.D. #
26)	L6 AR-1254-1	7.189	0.000	38228	0	16.338	N.D. #
28)	L6 AR-1254-3	7.814f	0.000	47277	0	13.146	N.D. #
34)	L7 AR-1260-4	8.850f	0.000	3726	0	1.632	N.D. #
38)	L8 AR-1262-3	9.484f	0.000	67269	0	16.173	N.D. #
41)	L9 AR-1268-1	9.484f	0.000	67269	0	9.492	N.D. #
43)	L9 AR-1268-3	9.783	0.000	66266	0	11.864	N.D. #
45)	L9 AR-1268-5	10.637	0.000	133192	0	8.235	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110520\
Data File : PO073099.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2020 11:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:38:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 05:38:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

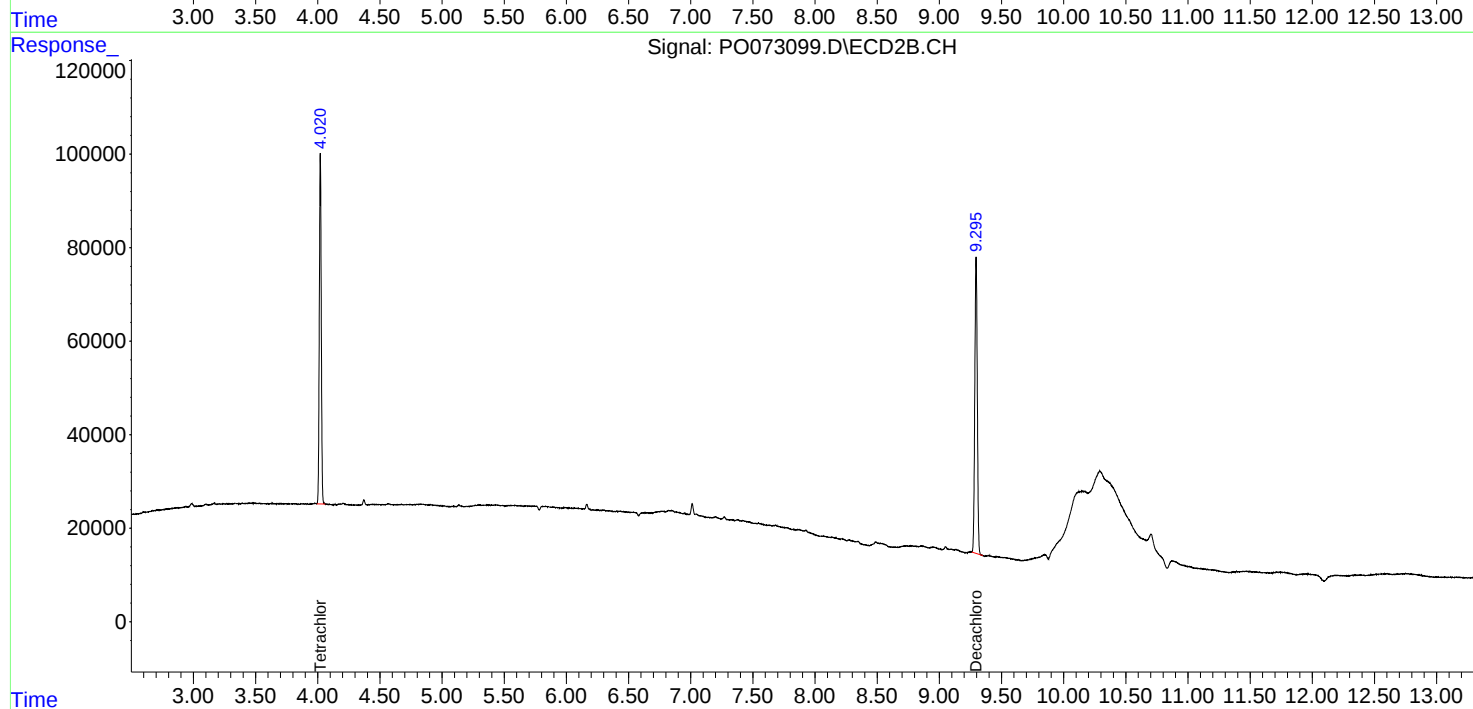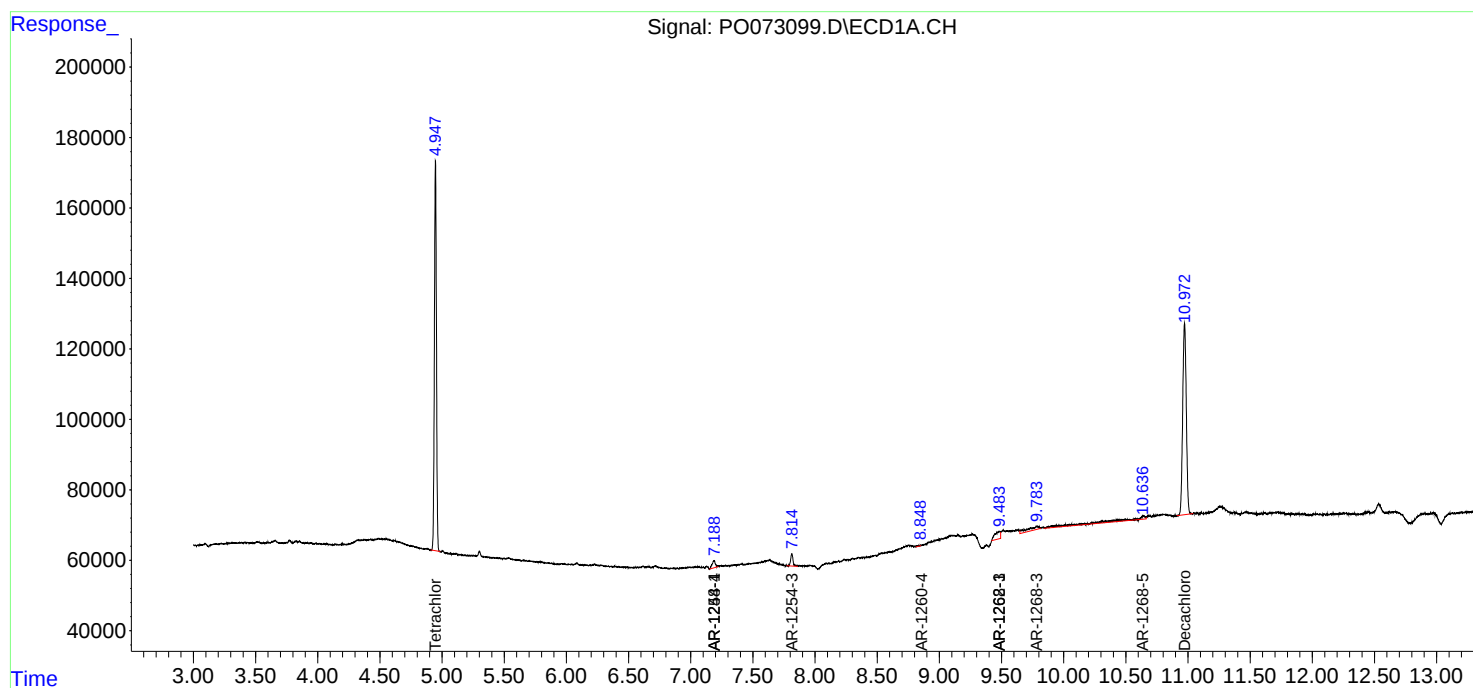


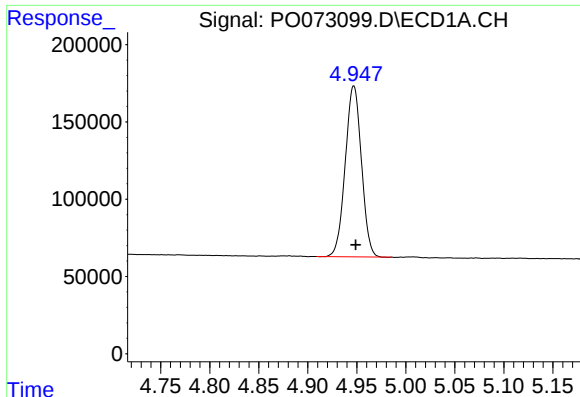

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: -0.002 min
Response: 1269860
Conc: 23.96 ng/ml

Instrument :
ECD_O
ClientSampleId :

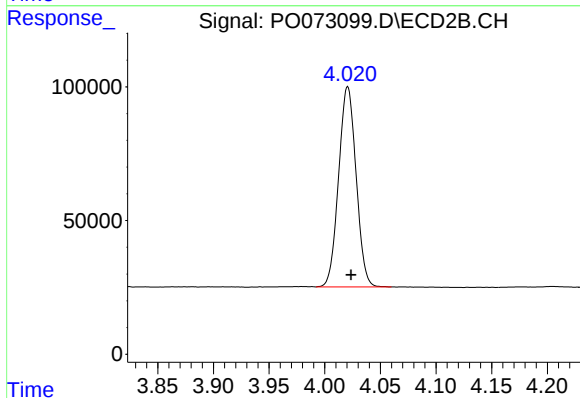


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: -0.003 min
Response: 818980
Conc: 22.92 ng/ml

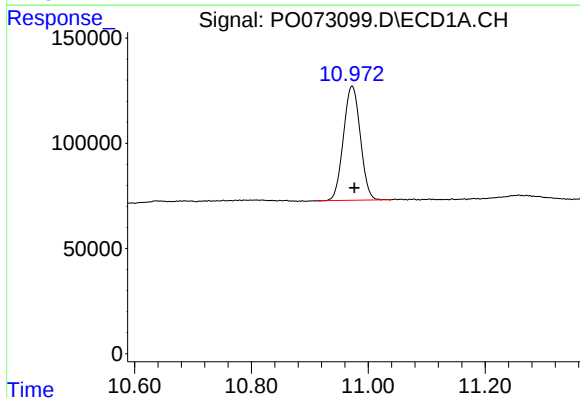


#2 Decachlorobiphenyl

R.T.: 10.972 min
Delta R.T.: -0.004 min
Response: 1090255
Conc: 26.35 ng/ml

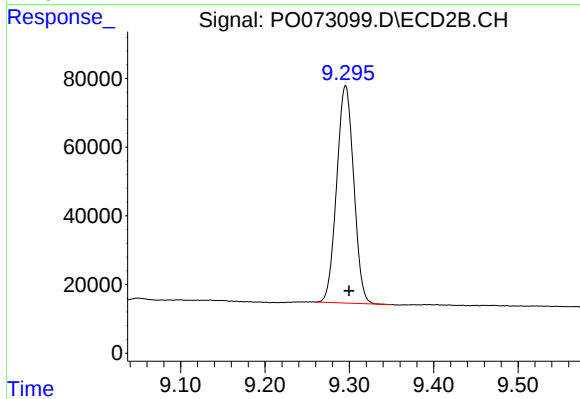

#2 Decachlorobiphenyl


R.T.: 9.296 min
Delta R.T.: -0.004 min
Response: 888521
Conc: 26.63 ng/ml

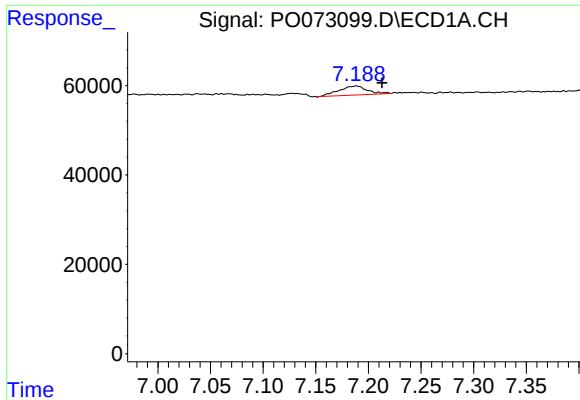

#24 AR-1248-4


R.T.: 7.189 min
Delta R.T.: -0.024 min
Response: 38228
Conc: 15.81 ng/ml

Instrument :
ECD_O
ClientSampleId :

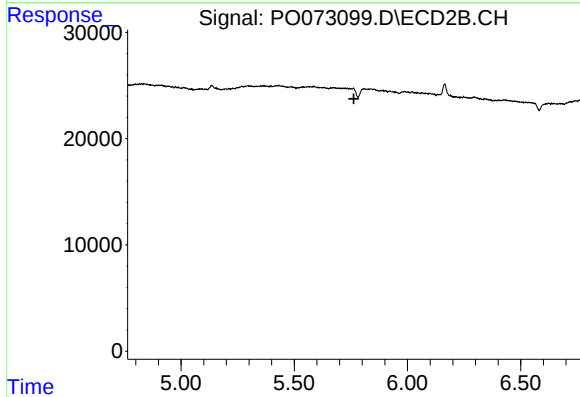


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.763 min
Response: 0
Conc: N.D.

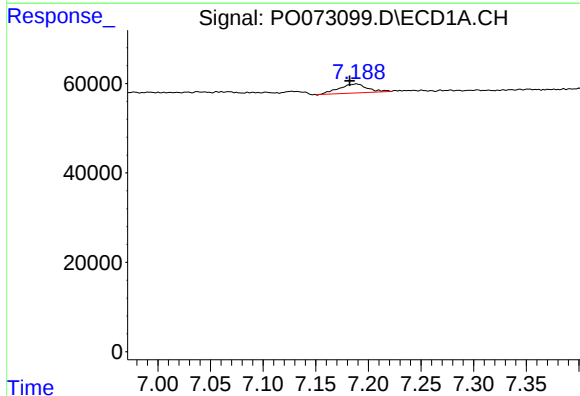


#26 AR-1254-1

R.T.: 7.189 min
Delta R.T.: 0.006 min
Response: 38228
Conc: 16.34 ng/ml

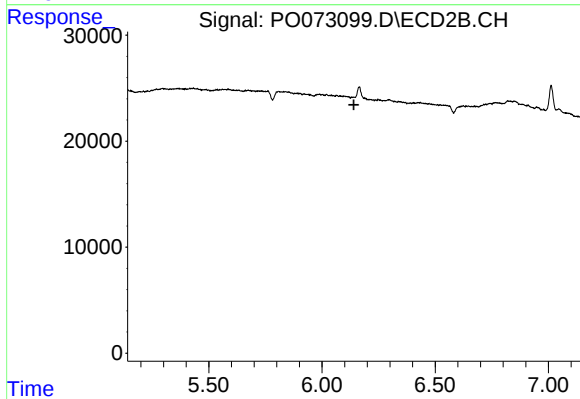

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.

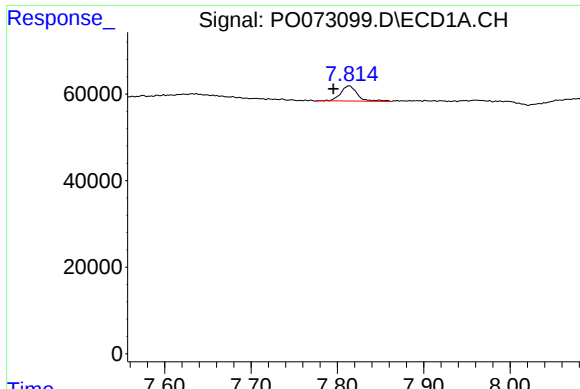

#28 AR-1254-3


R.T.: 7.814 min
Delta R.T.: 0.018 min
Response: 47277
Conc: 13.15 ng/ml

Instrument :
ECD_O
ClientSampleId :

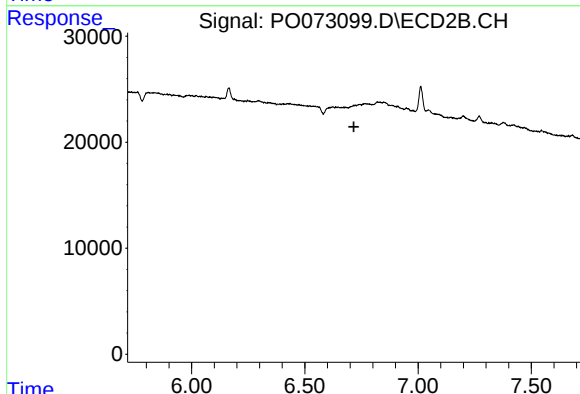


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.717 min
Response: 0
Conc: N.D.

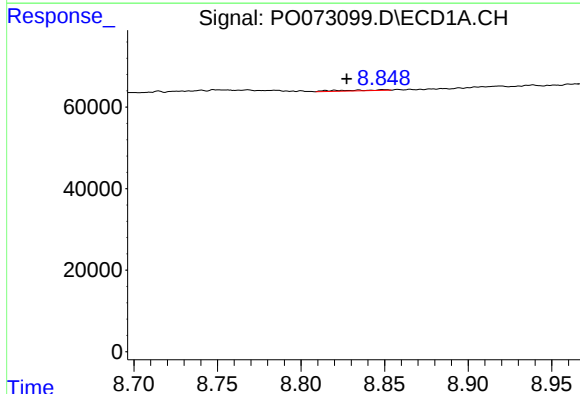


#34 AR-1260-4

R.T.: 8.850 min
Delta R.T.: 0.022 min
Response: 3726
Conc: 1.63 ng/ml

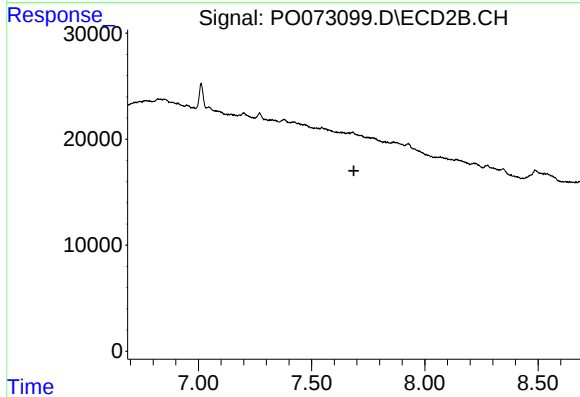

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.687 min
Response: 0
Conc: N.D.

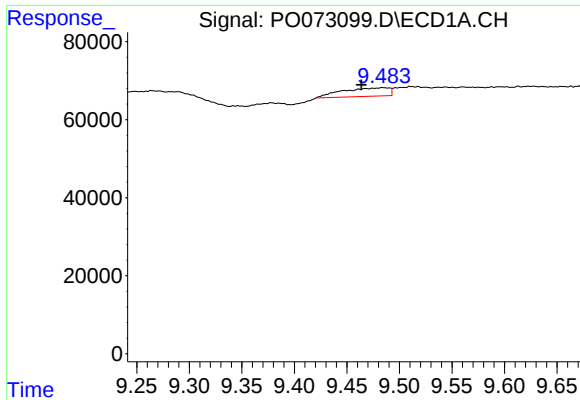

#38 AR-1262-3


R.T.: 9.484 min
Delta R.T.: 0.020 min
Response: 67269
Conc: 16.17 ng/ml

Instrument :
ECD_O
ClientSampleId :

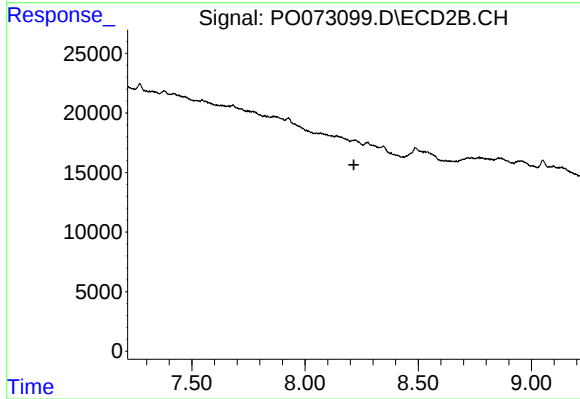


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.216 min
Response: 0
Conc: N.D.

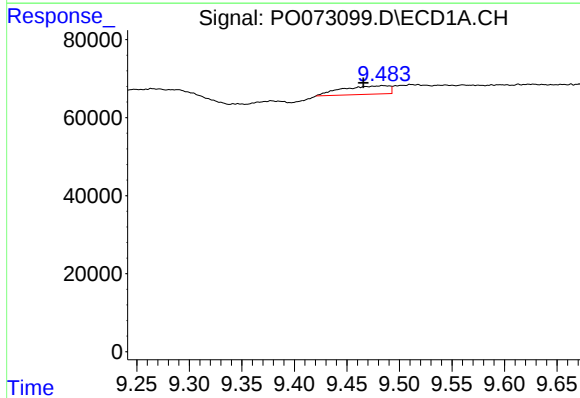


#41 AR-1268-1

R.T.: 9.484 min
Delta R.T.: 0.018 min
Response: 67269
Conc: 9.49 ng/ml

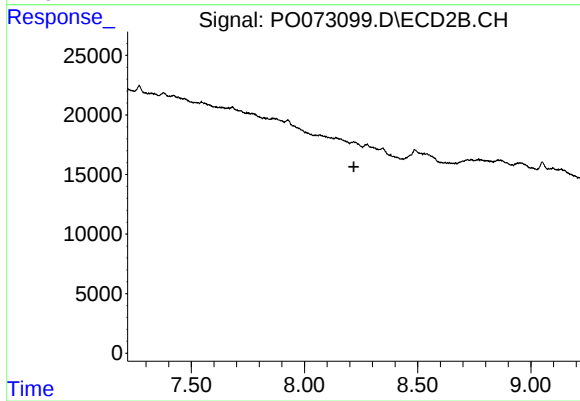

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.218 min
Response: 0
Conc: N.D.

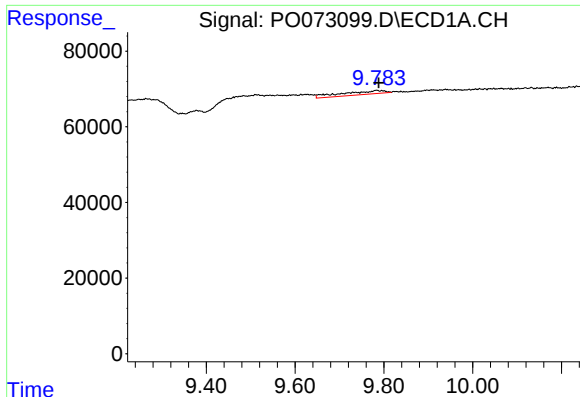

#43 AR-1268-3


R.T.: 9.783 min
Delta R.T.: -0.005 min
Response: 66266
Conc: 11.86 ng/ml

Instrument :
ECD_O
ClientSampleId :

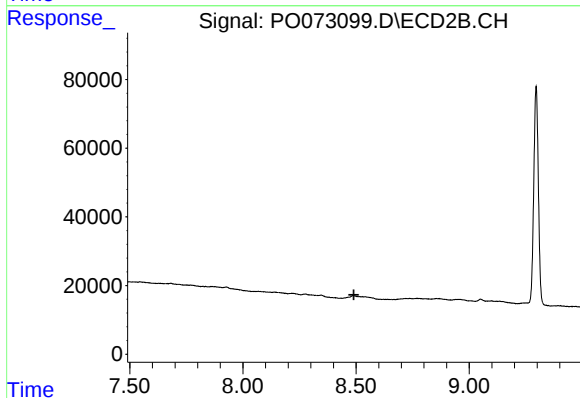


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.490 min
Response: 0
Conc: N.D.

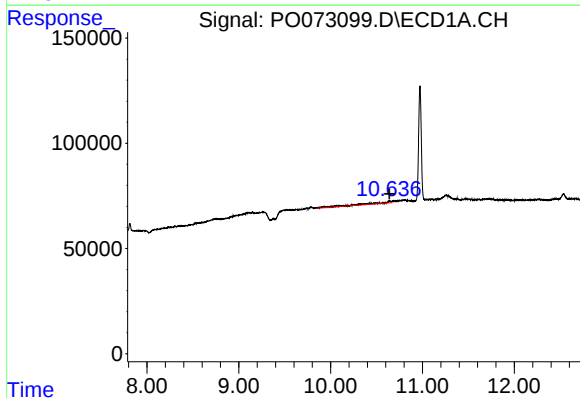

#45 AR-1268-5

R.T.: 10.637 min
Delta R.T.: -0.003 min
Response: 133192
Conc: 8.24 ng/ml

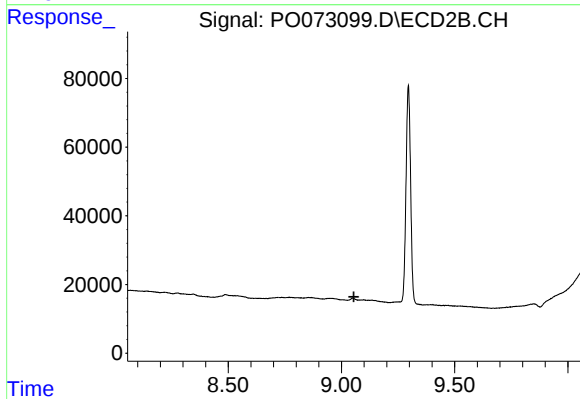

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.055 min
Response: 0
Conc: N.D.