

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110520\
 Data File : PO073103.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2020 13:07
 Operator : DD\AJ
 Sample : L4565-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-063-ARE

Manual Integrations
 APPROVED

Ankita
 11/6/2020 3:12:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 00:40:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 05:38:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.948	4.021	1663677	1092231	31.391	30.565
2) SA Decachlor...	10.975	9.296	1163091	1026327	28.106m	30.763

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110520\
Data File : PO073103.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2020 13:07
Operator : DD\AJ
Sample : L4565-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-GF-02-063-ARE


Manual Integrations
APPROVED

Ankita
11/6/2020 3:12:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 00:40:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 05:38:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

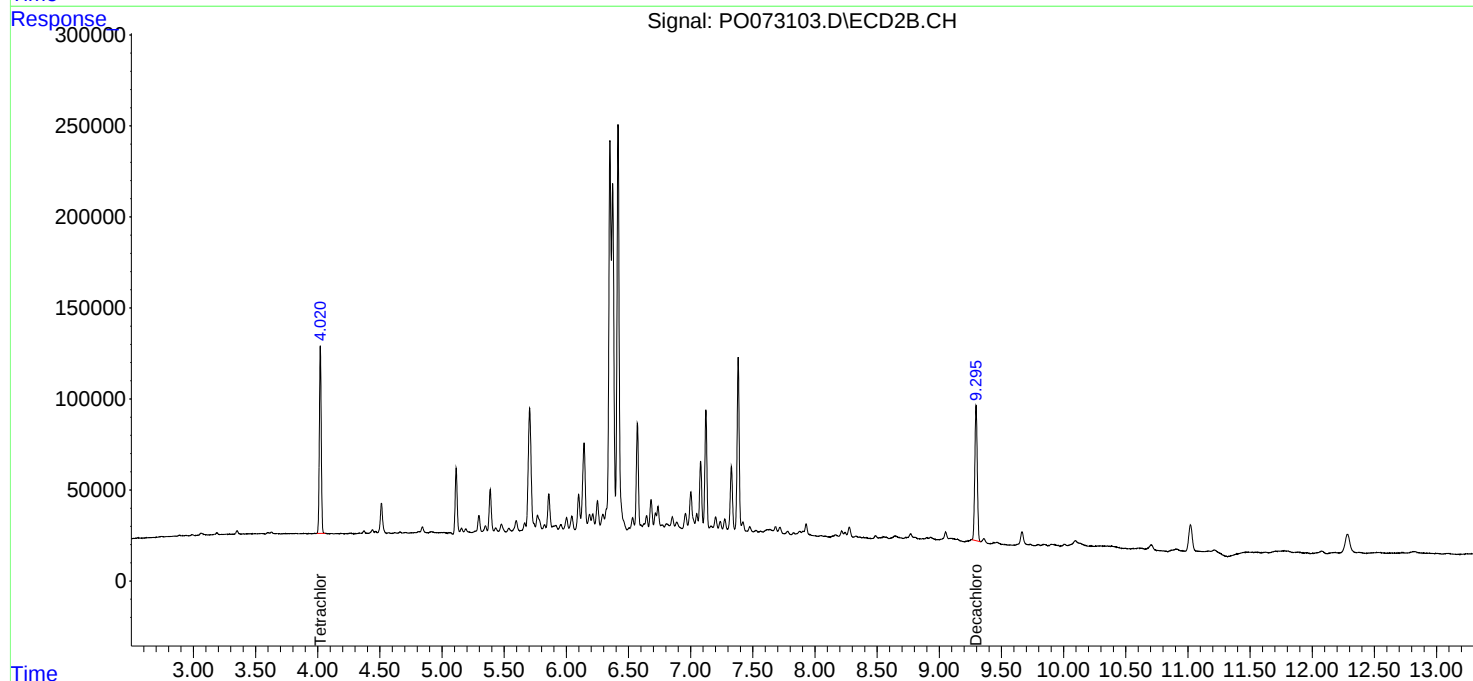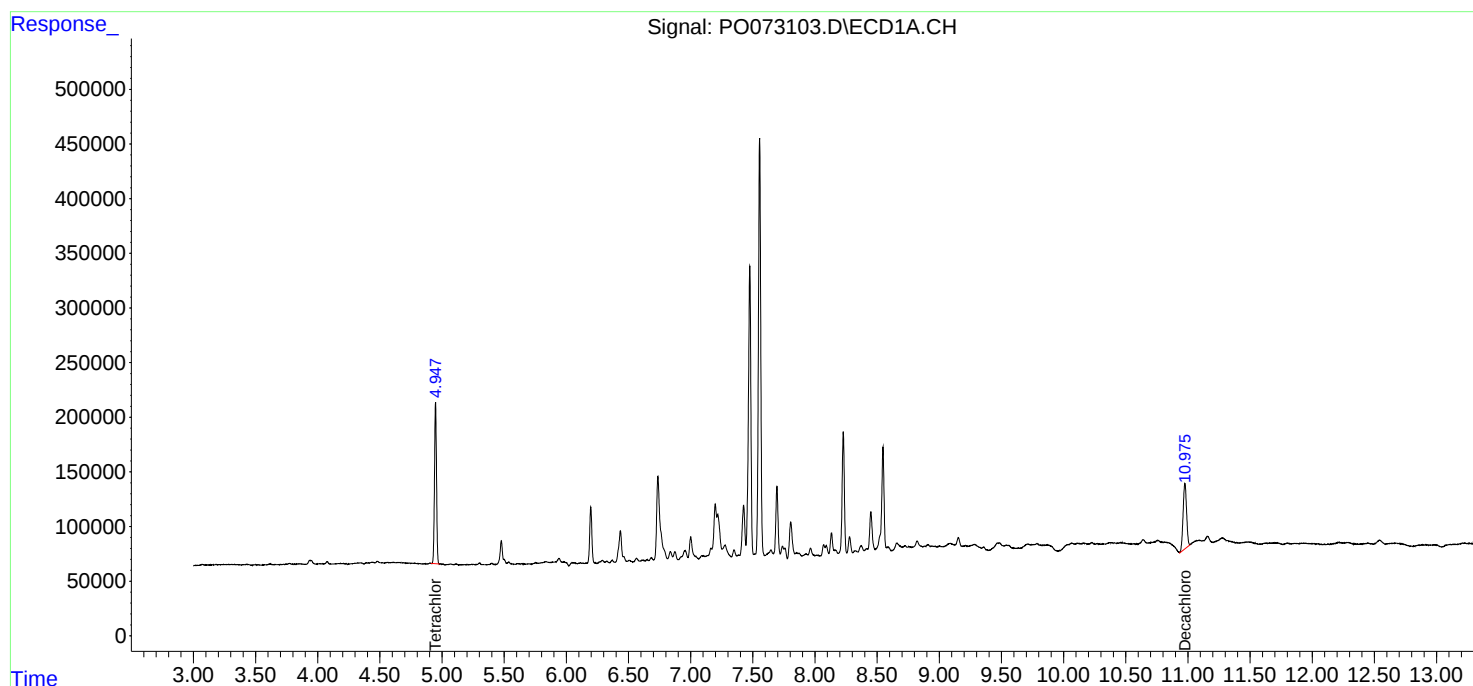

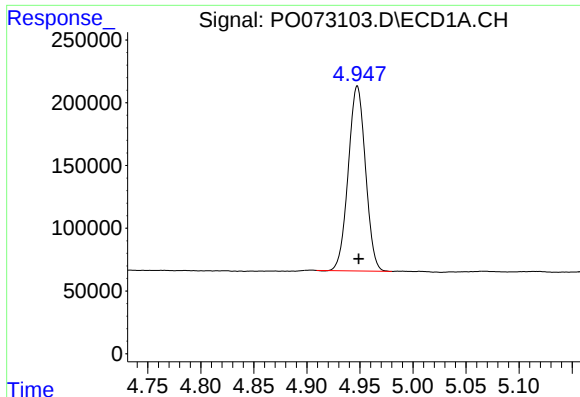


#1 Tetrachloro-m-xylene

R.T.: 4.948 min
Delta R.T.: -0.001 min
Response: 1663677
Conc: 31.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-063-ARE


Manual Integrations
APPROVED

Ankita
11/6/2020 3:12:22 PM

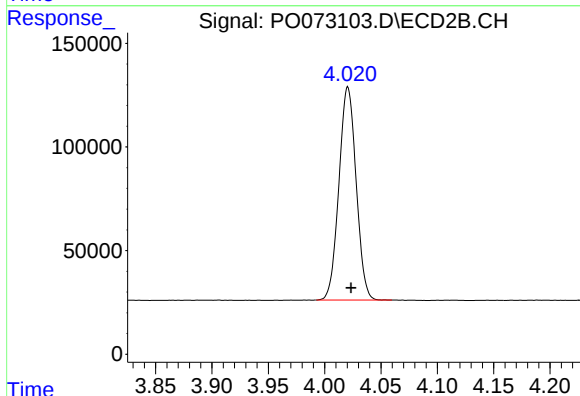


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: -0.003 min
Response: 1092231
Conc: 30.57 ng/ml

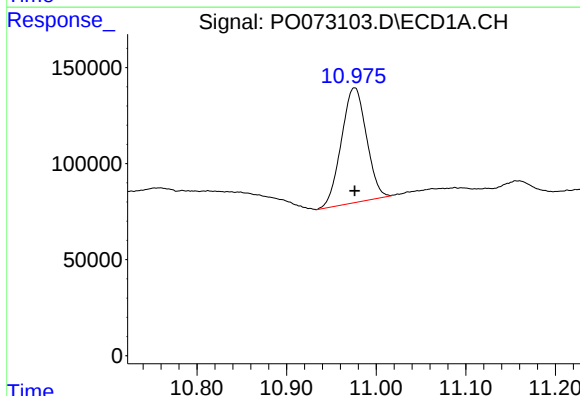

#2 Decachlorobiphenyl

R.T.: 10.975 min
Delta R.T.: 0.000 min
Response: 1163091
Conc: 28.11 ng/ml m

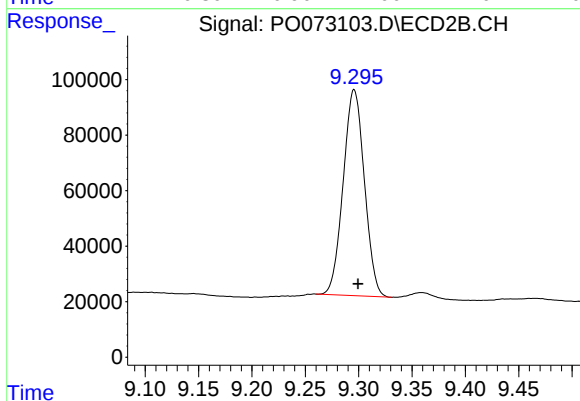

#2 Decachlorobiphenyl

R.T.: 9.296 min
Delta R.T.: -0.004 min
Response: 1026327
Conc: 30.76 ng/ml