

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO110521\
 Data File : PO082562.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Nov 2021 18:46
 Operator : AJ\MA
 Sample : M4498-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 01:04:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.963	1769135	665002	20.212	21.489
2)	SA Decachlor...	11.070	9.276	1219998	573509	19.319	19.919
Target Compounds							
8)	L2 AR-1221-1	5.220	0.000	191403	0	202.959	N.D. #
9)	L2 AR-1221-2	5.322	4.316	23040	8562	35.546	29.493
28)	L6 AR-1254-3	7.849	0.000	18517	0	4.329	N.D. #
30)	L6 AR-1254-5	8.560	0.000	6721	0	2.090	N.D. #
33)	L7 AR-1260-3	8.636	0.000	2095	0	0.740	N.D. #
35)	L7 AR-1260-5	9.218	0.000	7420	0	1.183	N.D. #
36)	L8 AR-1262-1	8.636	0.000	2095	0	0.565	N.D. #
37)	L8 AR-1262-2	9.218	0.000	7420	0	1.162	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO110521\
Data File : PO082562.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Nov 2021 18:46
Operator : AJ\MA
Sample : M4498-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:04:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

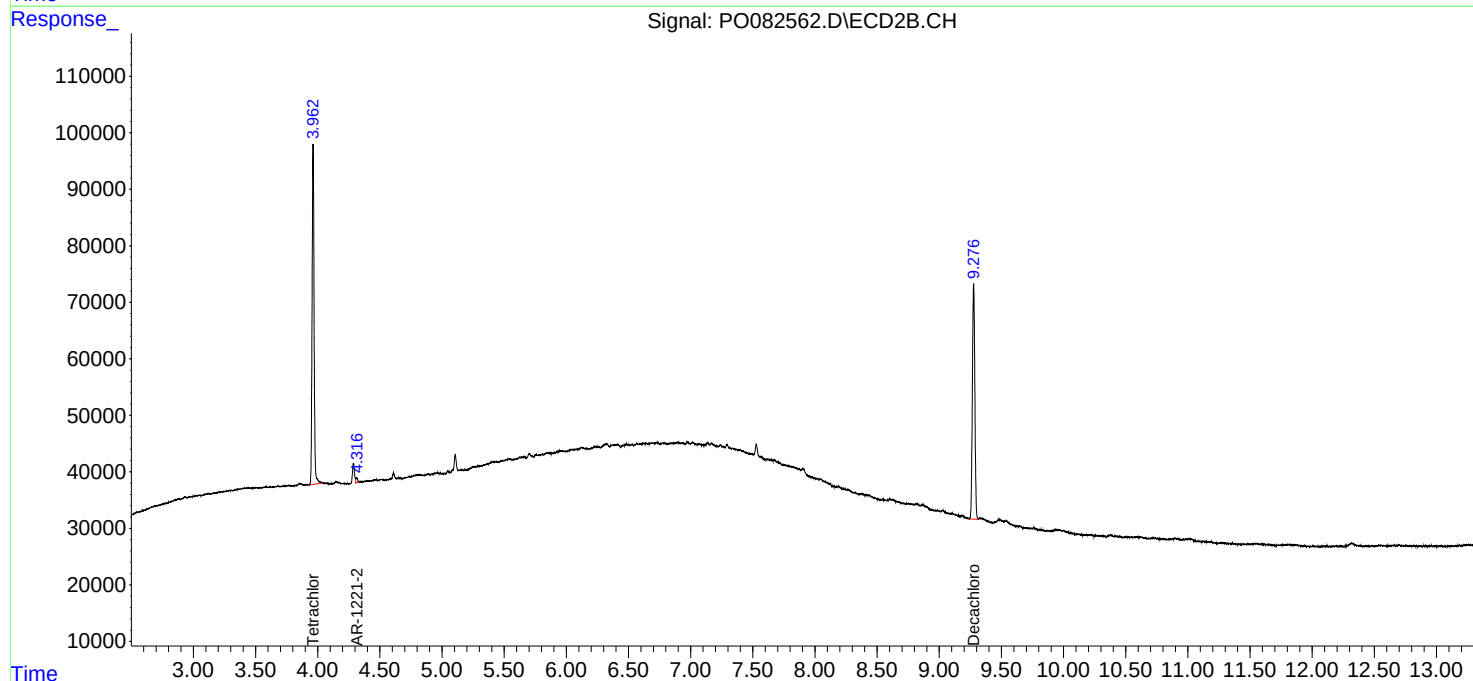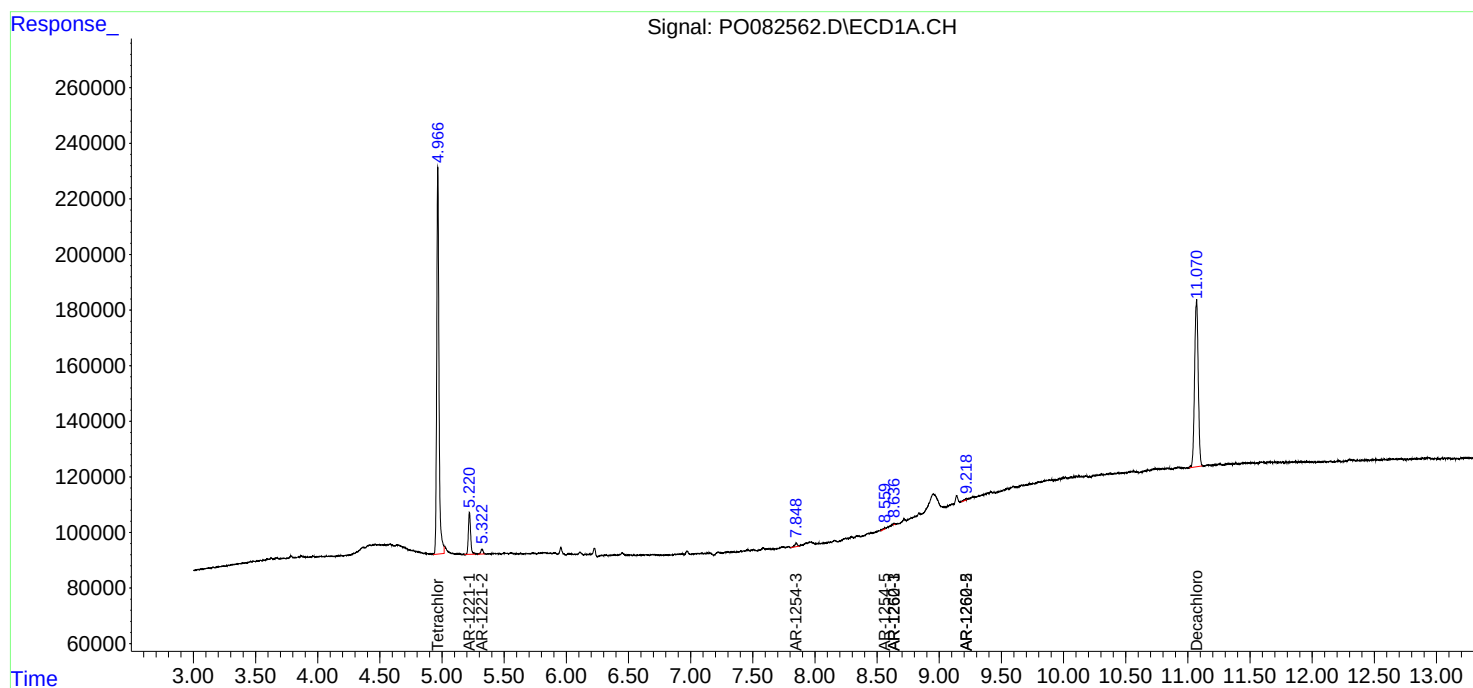


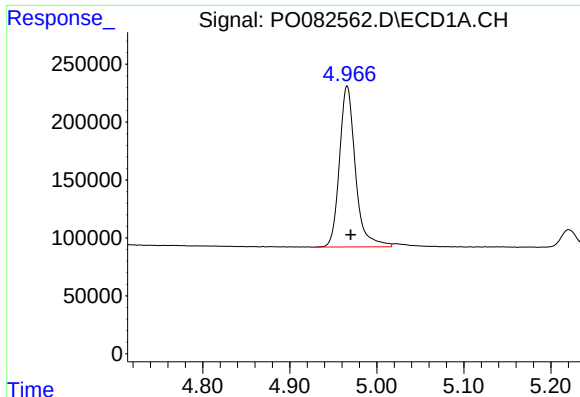

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: -0.004 min
Response: 1769135
Conc: 20.21 ng/ml

Instrument :
ECD_O
ClientSampleId :

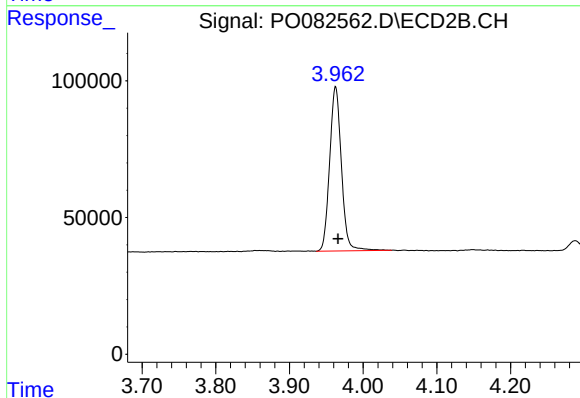


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.003 min
Response: 665002
Conc: 21.49 ng/ml

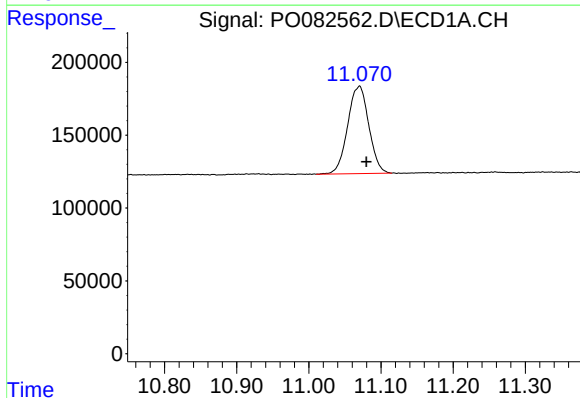


#2 Decachlorobiphenyl

R.T.: 11.070 min
Delta R.T.: -0.009 min
Response: 1219998
Conc: 19.32 ng/ml

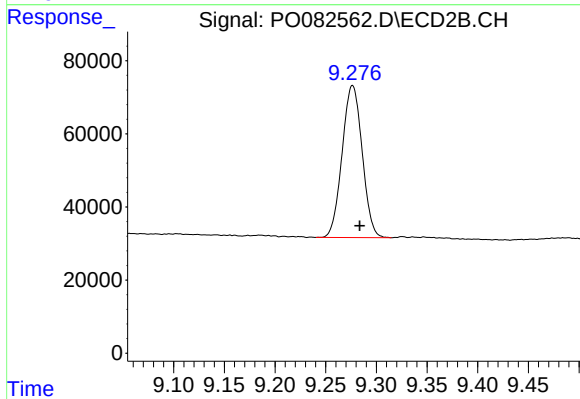

#2 Decachlorobiphenyl


R.T.: 9.276 min
Delta R.T.: -0.007 min
Response: 573509
Conc: 19.92 ng/ml

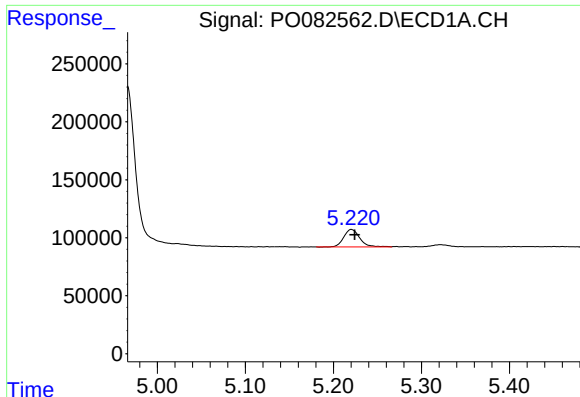

#8 AR-1221-1


R.T.: 5.220 min
Delta R.T.: -0.004 min
Response: 191403
Conc: 202.96 ng/ml

Instrument :
ECD_O
ClientSampleId :

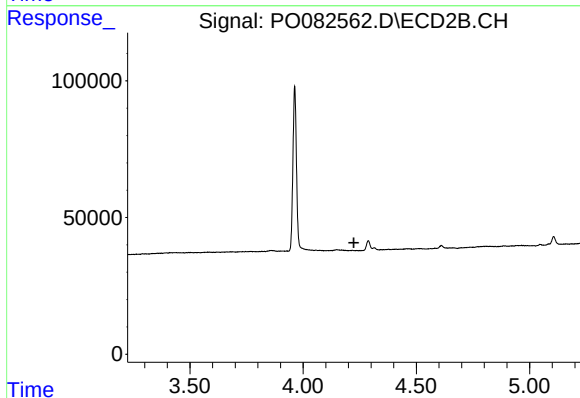


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.224 min
Response: 0
Conc: N.D.

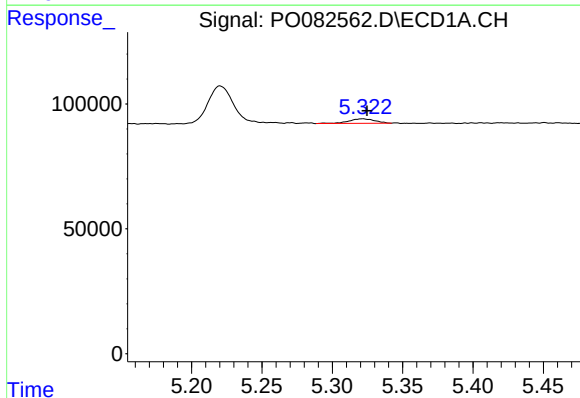


#9 AR-1221-2

R.T.: 5.322 min
Delta R.T.: -0.003 min
Response: 23040
Conc: 35.55 ng/ml

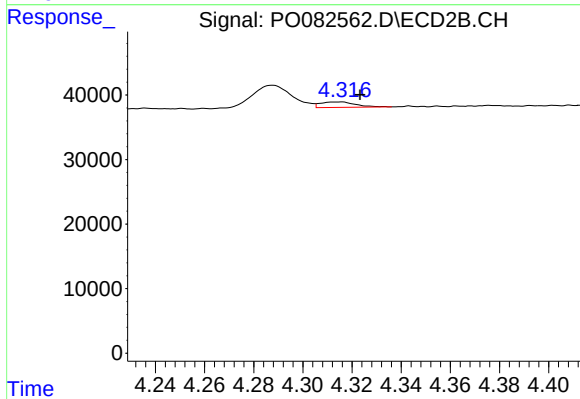

#9 AR-1221-2


R.T.: 4.316 min
Delta R.T.: -0.007 min
Response: 8562
Conc: 29.49 ng/ml

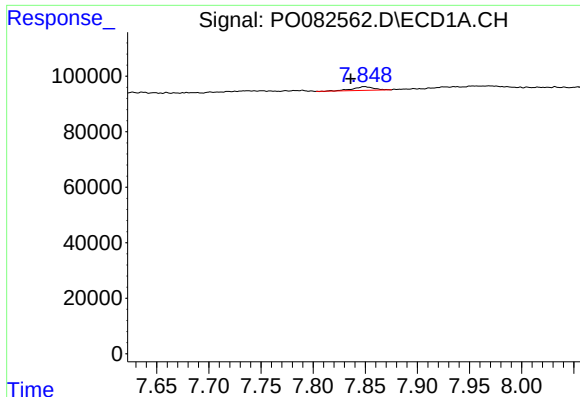

#28 AR-1254-3


R.T.: 7.849 min
Delta R.T.: 0.013 min
Response: 18517
Conc: 4.33 ng/ml

Instrument :
ECD_O
ClientSampleId :

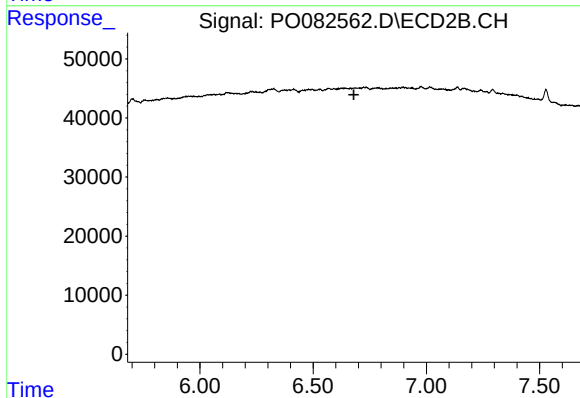


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

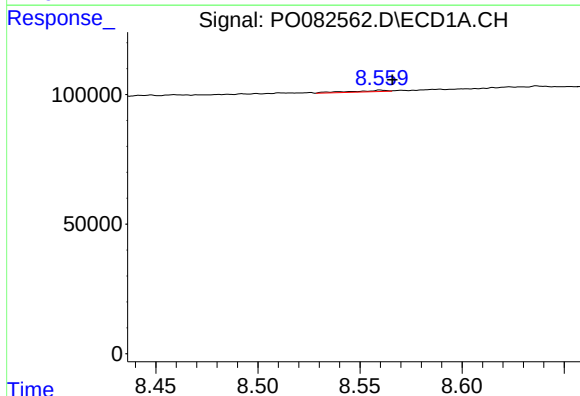


#30 AR-1254-5

R.T.: 8.560 min
Delta R.T.: -0.006 min
Response: 6721
Conc: 2.09 ng/ml

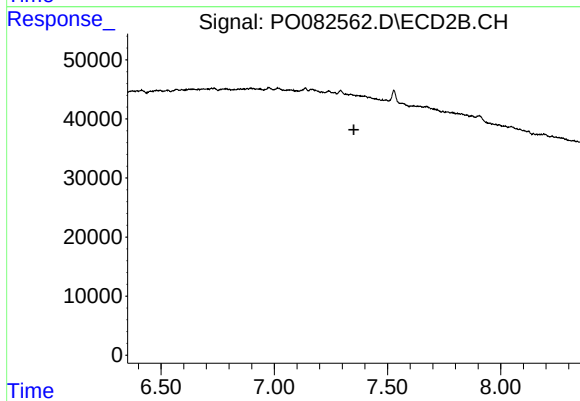

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.351 min
Response: 0
Conc: N.D.

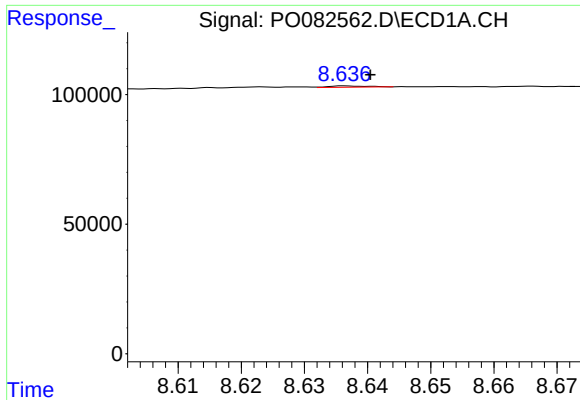

#33 AR-1260-3


R.T.: 8.636 min
Delta R.T.: -0.004 min
Response: 2095
Conc: 0.74 ng/ml

Instrument :
ECD_O
ClientSampleId :

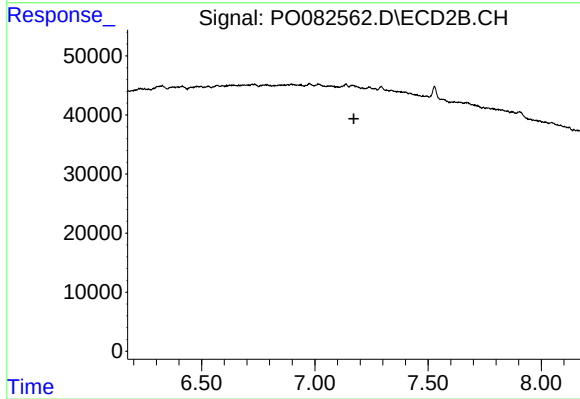


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.172 min
Response: 0
Conc: N.D.

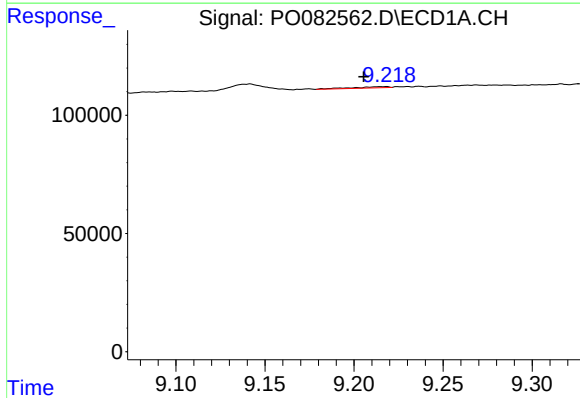


#35 AR-1260-5

R.T.: 9.218 min
Delta R.T.: 0.013 min
Response: 7420
Conc: 1.18 ng/ml

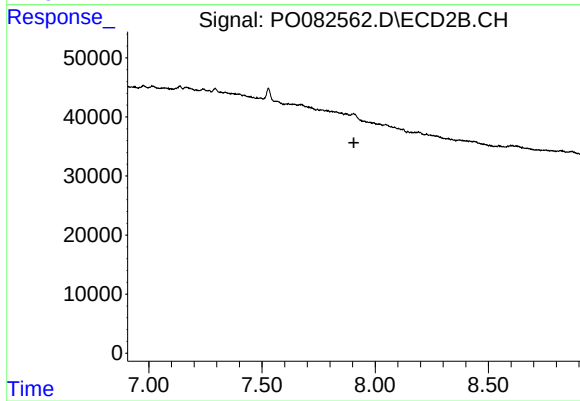

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.906 min
Response: 0
Conc: N.D.

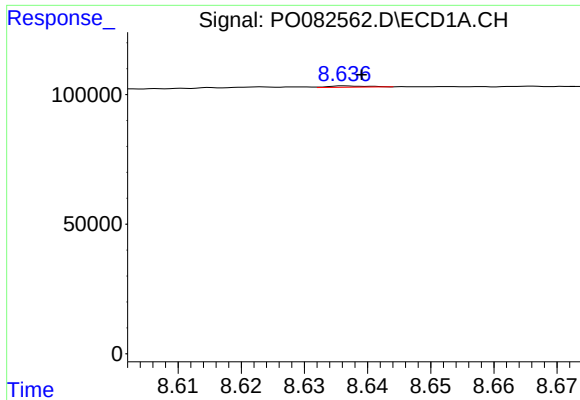

#36 AR-1262-1


R.T.: 8.636 min
Delta R.T.: -0.003 min
Response: 2095
Conc: 0.56 ng/ml

Instrument :
ECD_O
ClientSampleId :

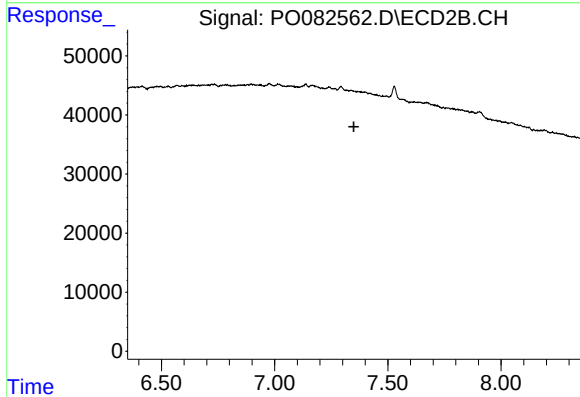


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.

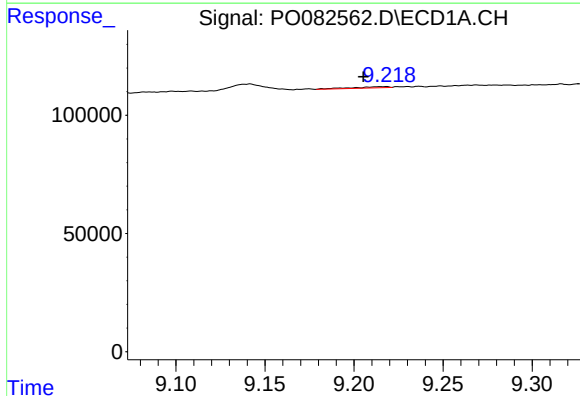

#37 AR-1262-2

R.T.: 9.218 min
Delta R.T.: 0.013 min
Response: 7420
Conc: 1.16 ng/ml

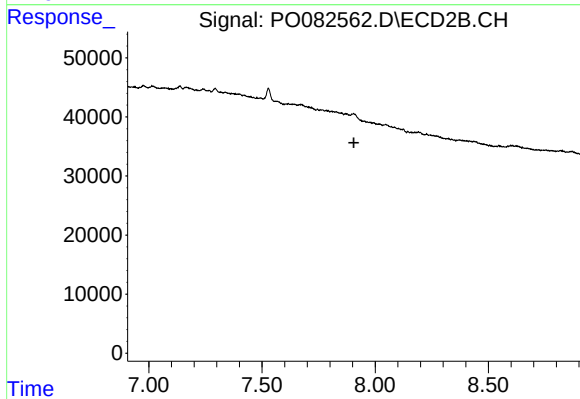

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.905 min
Response: 0
Conc: N.D.