

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110521\
Data File : PO082542.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Nov 2021 12:45
Operator : AJ\MA
Sample : PB140490BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140490BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:00:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.967	3.964	1638541	606574	18.720	19.601
2) SA Decachlor...	11.071	9.278	1287440	602323	20.386	20.920

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110521\
Data File : PO082542.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Nov 2021 12:45
Operator : AJ\MA
Sample : PB140490BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140490BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 01:00:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

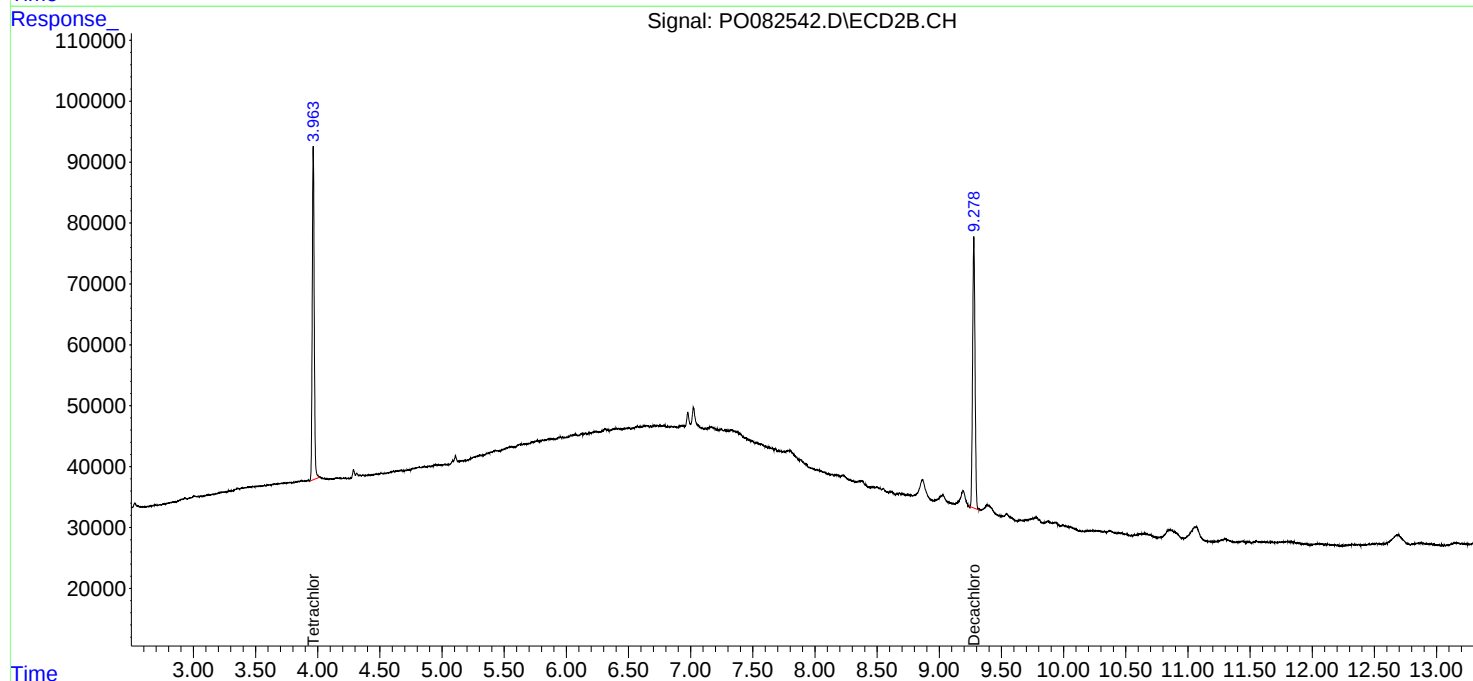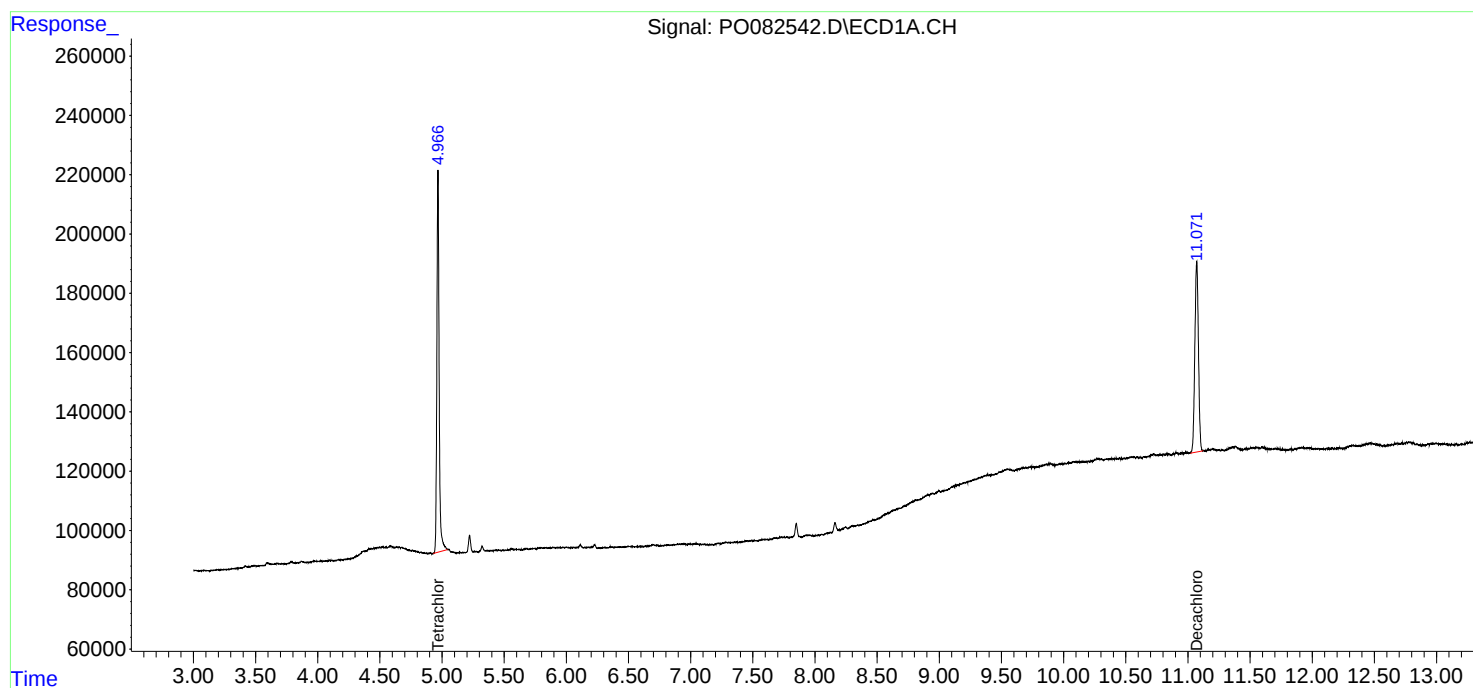


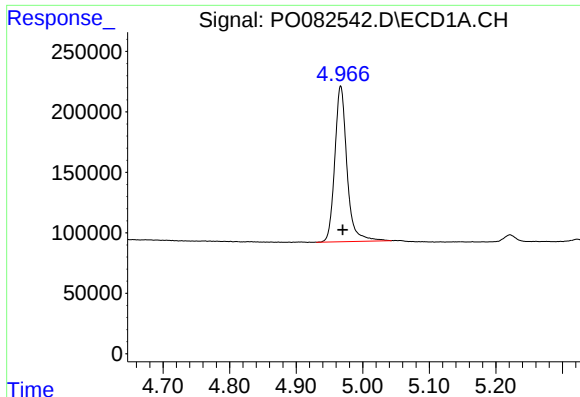

#1 Tetrachloro-m-xylene


R.T.: 4.967 min
Delta R.T.: -0.003 min
Response: 1638541
Conc: 18.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB140490BL

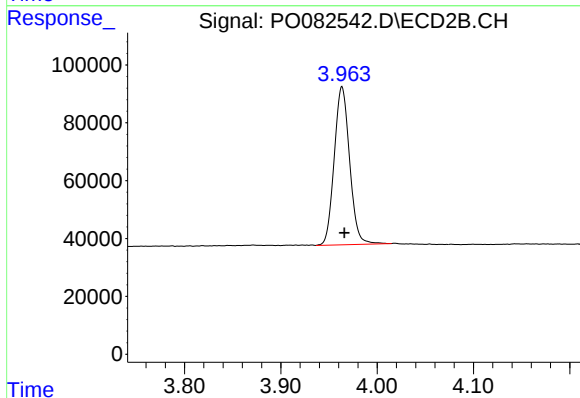


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: -0.002 min
Response: 606574
Conc: 19.60 ng/ml

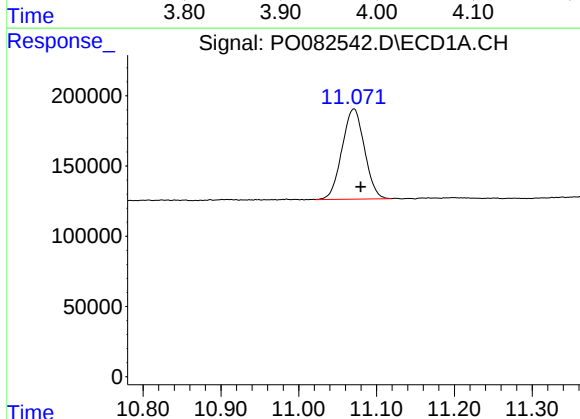

#2 Decachlorobiphenyl

R.T.: 11.071 min
Delta R.T.: -0.009 min
Response: 1287440
Conc: 20.39 ng/ml

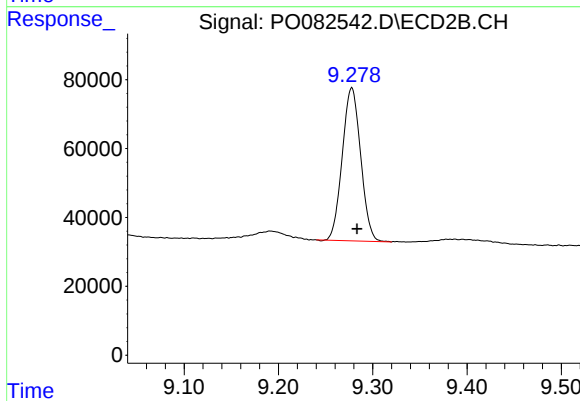

#2 Decachlorobiphenyl

R.T.: 9.278 min
Delta R.T.: -0.006 min
Response: 602323
Conc: 20.92 ng/ml