

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110525\
 Data File : PO114920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2025 15:36
 Operator : YP/AJ
 Sample : Q3543-01 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRE-25-0073

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/06/2025
 Supervised By :Yogesh Patel 11/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 23:26:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.349	3.649	15636431	7074198	2.222	1.584m#
2) SA Decachlor...	9.937	8.645	8352040	7600241	1.889m	1.947

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110525\
Data File : PO114920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2025 15:36
Operator : YP/AJ
Sample : Q3543-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TRE-25-0073


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/06/2025
Supervised By :Yogesh Patel 11/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 23:26:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

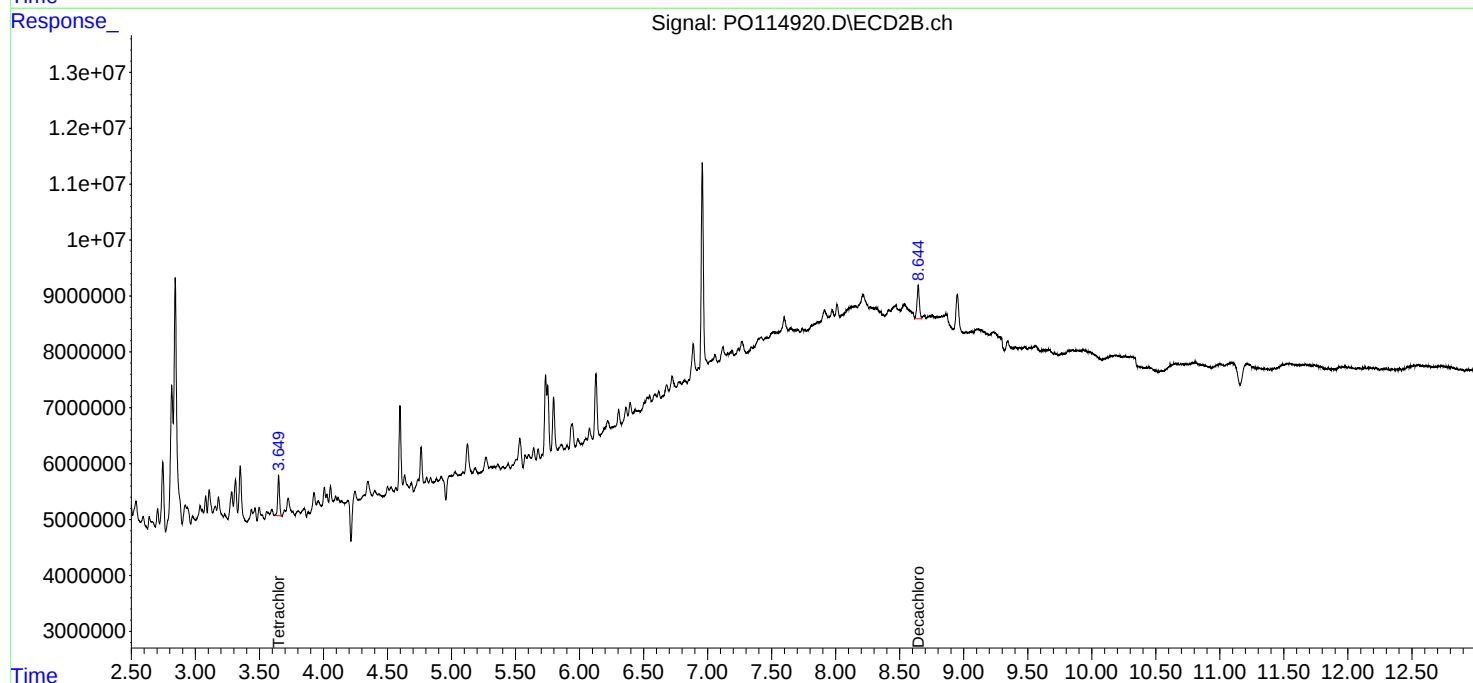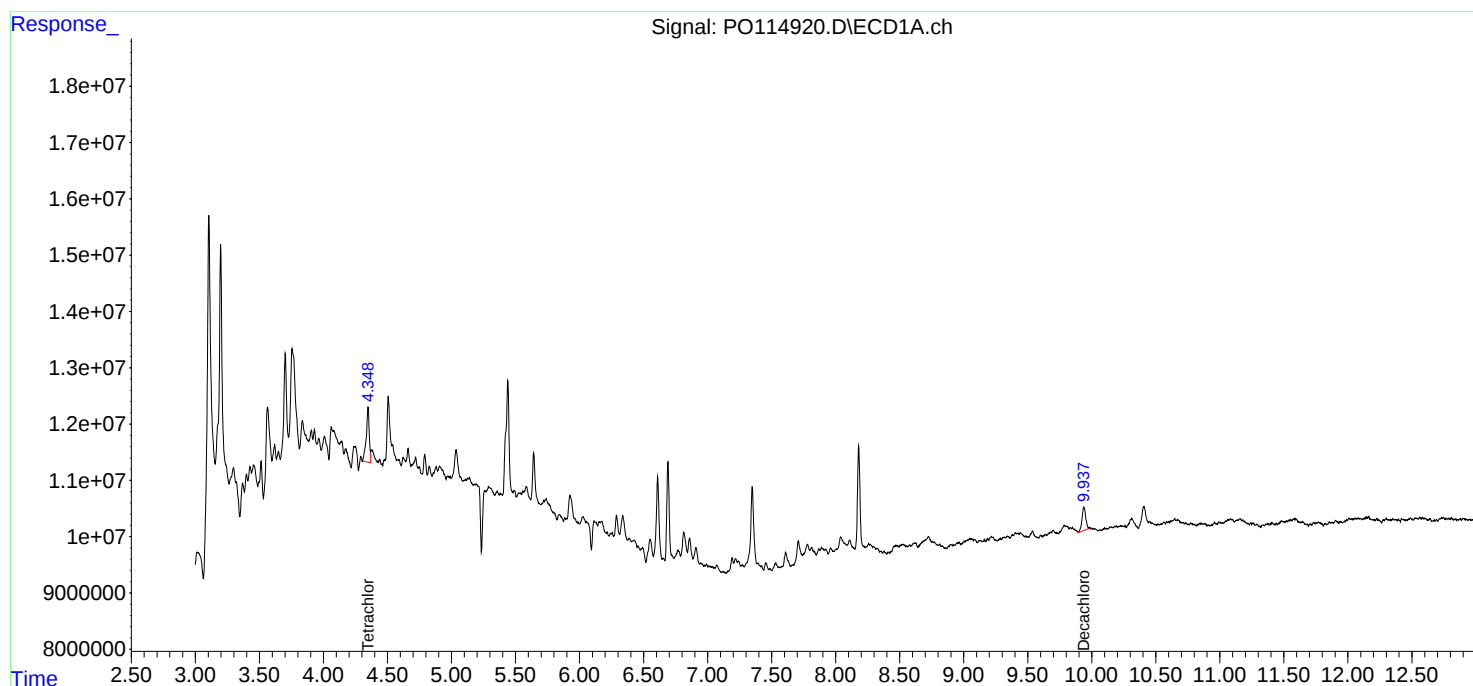

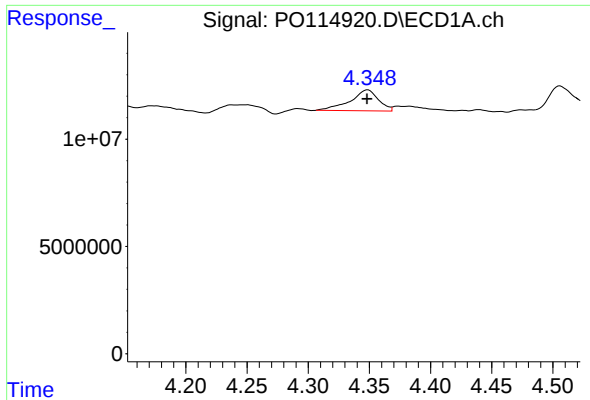


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 15636431
Conc: 2.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-25-0073


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/06/2025
Supervised By :Yogesh Patel 11/06/2025

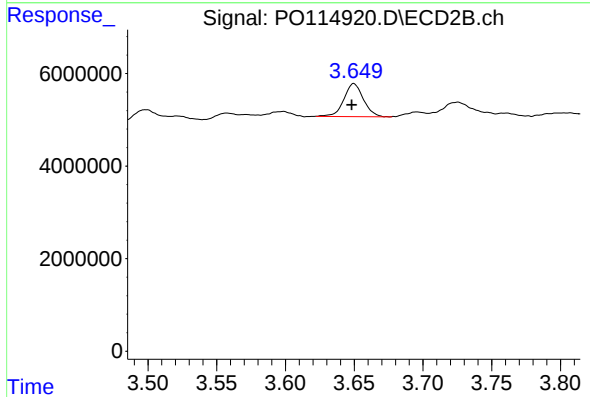


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: 0.001 min
Response: 7074198
Conc: 1.58 ng/ml m

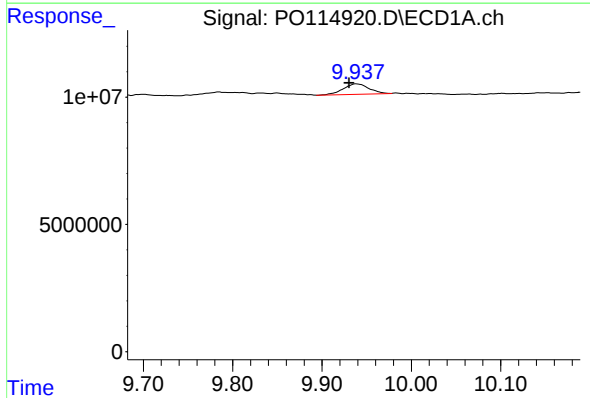

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: 0.007 min
Response: 8352040
Conc: 1.89 ng/ml m

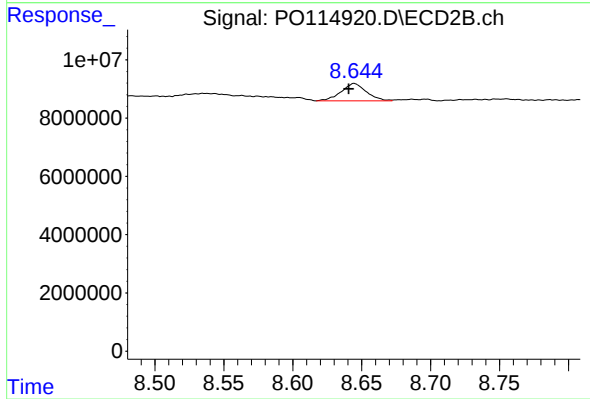

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: 0.004 min
Response: 7600241
Conc: 1.95 ng/ml