

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110620\
 Data File : PO073133.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Nov 2020 14:19
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 15:13:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 05:38:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.948	4.022	1434908	901114	27.074	25.217
2)	SA Decachlor...	10.977	9.297	1232347	934276	29.779	28.004
Target Compounds							
20)	L4 AR-1242-5	7.222f	0.000	20994	0	16.040	N.D. #
24)	L5 AR-1248-4	7.222	0.000	20994	0	8.683	N.D. #
26)	L6 AR-1254-1	7.188	0.000	80732	0	34.505	N.D. #
27)	L6 AR-1254-2	7.419	0.000	79446	0	22.547	N.D. #
28)	L6 AR-1254-3	7.815f	0.000	41555	0	11.555	N.D. #
43)	L9 AR-1268-3	9.792	0.000	314131	0	56.239	N.D. #
45)	L9 AR-1268-5	10.652	0.000	770650	0	47.648	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110620\
Data File : PO073133.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Nov 2020 14:19
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 15:13:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 05:38:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

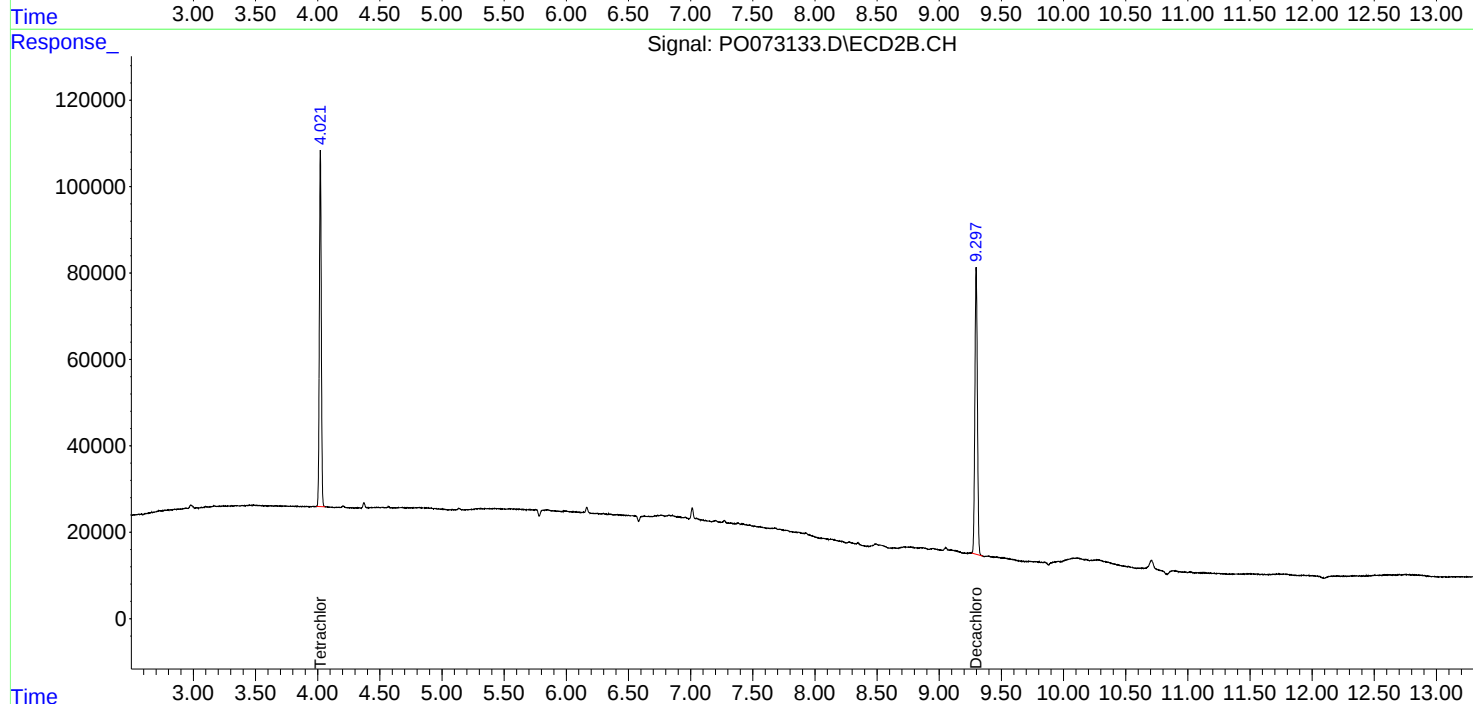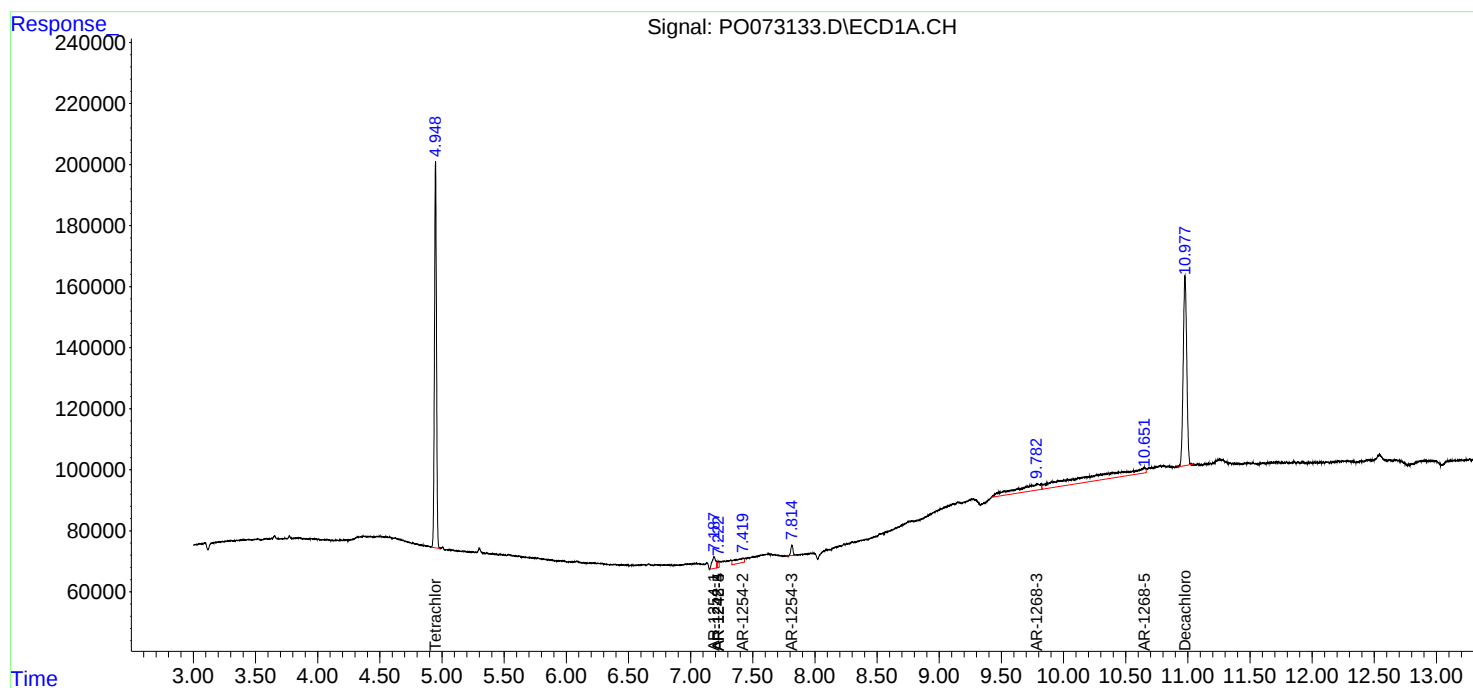


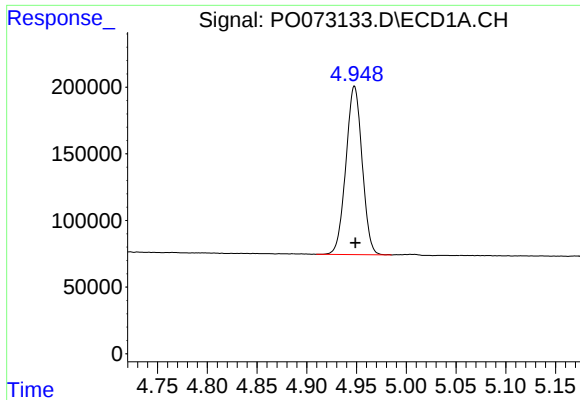

#1 Tetrachloro-m-xylene


R.T.: 4.948 min
Delta R.T.: -0.001 min
Response: 1434908
Conc: 27.07 ng/ml

Instrument :
ECD_O
ClientSampleId :

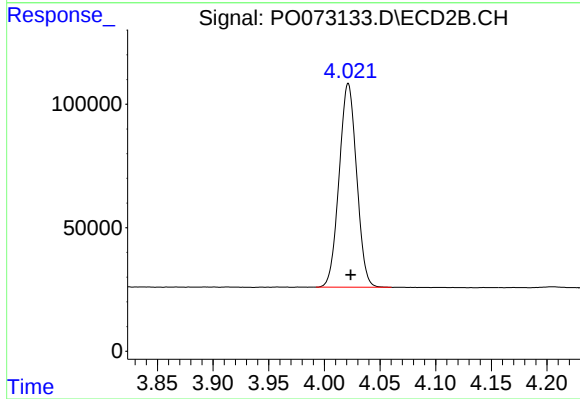


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: -0.002 min
Response: 901114
Conc: 25.22 ng/ml

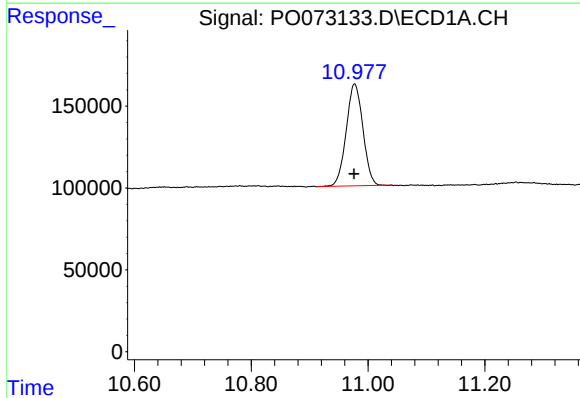


#2 Decachlorobiphenyl

R.T.: 10.977 min
Delta R.T.: 0.000 min
Response: 1232347
Conc: 29.78 ng/ml

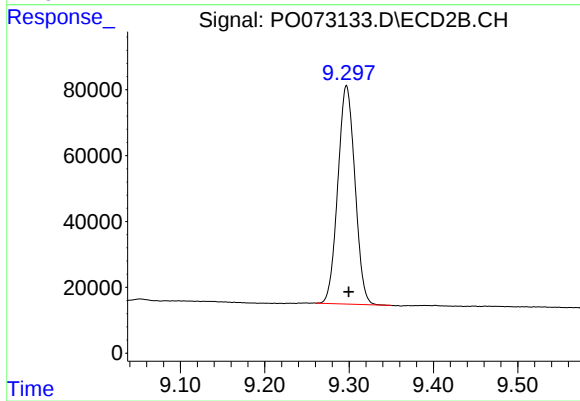

#2 Decachlorobiphenyl


R.T.: 9.297 min
Delta R.T.: -0.003 min
Response: 934276
Conc: 28.00 ng/ml

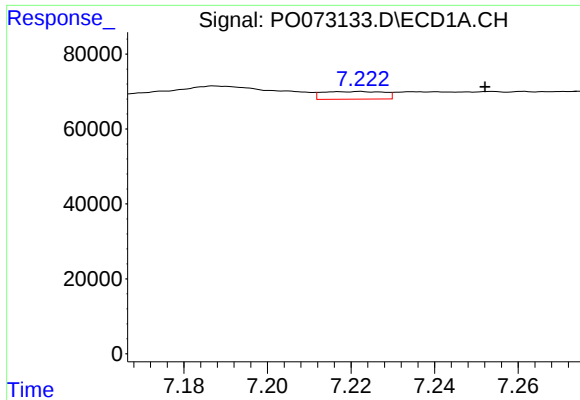

#20 AR-1242-5


R.T.: 7.222 min
Delta R.T.: -0.030 min
Response: 20994
Conc: 16.04 ng/ml

Instrument :
ECD_O
ClientSampleId :

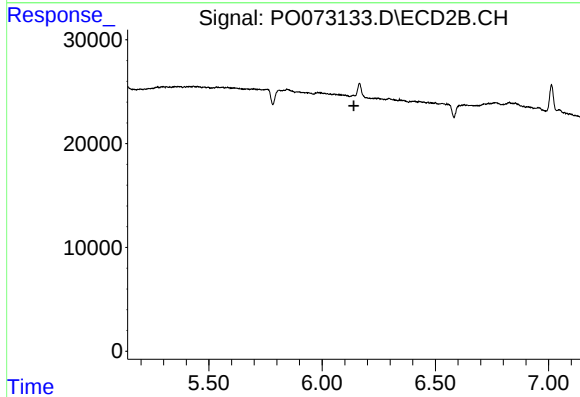


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.

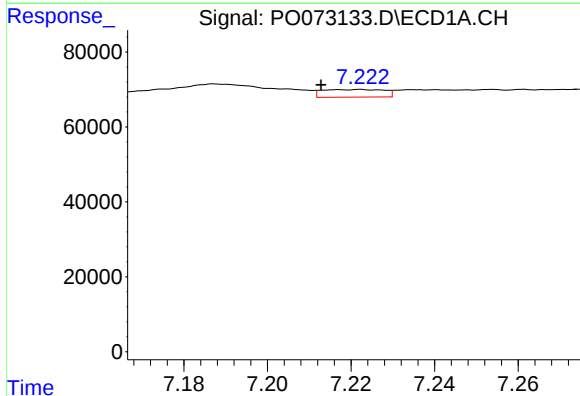


#24 AR-1248-4

R.T.: 7.222 min
Delta R.T.: 0.009 min
Response: 20994
Conc: 8.68 ng/ml

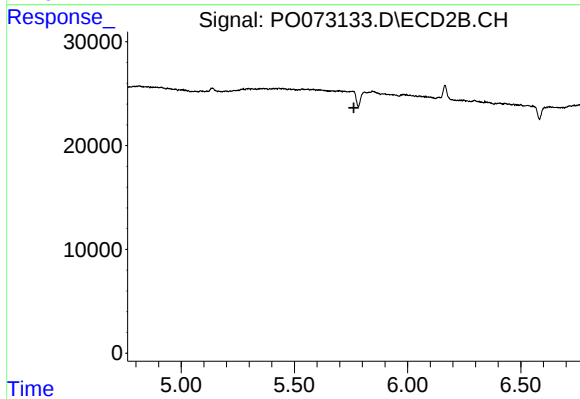

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.763 min
Response: 0
Conc: N.D.

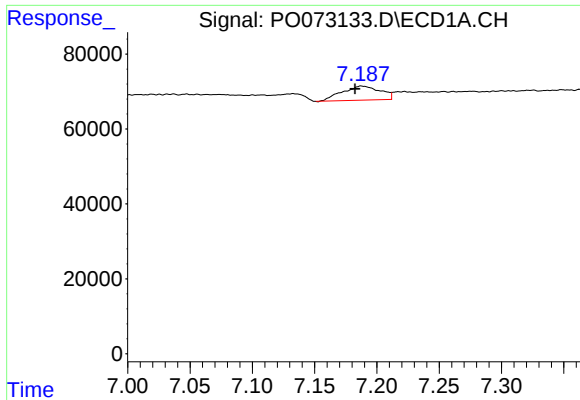

#26 AR-1254-1


R.T.: 7.188 min
Delta R.T.: 0.005 min
Response: 80732
Conc: 34.50 ng/ml

Instrument :
ECD_O
ClientSampleId :

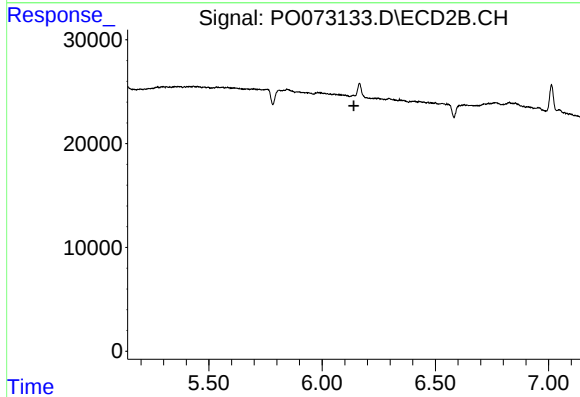


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.

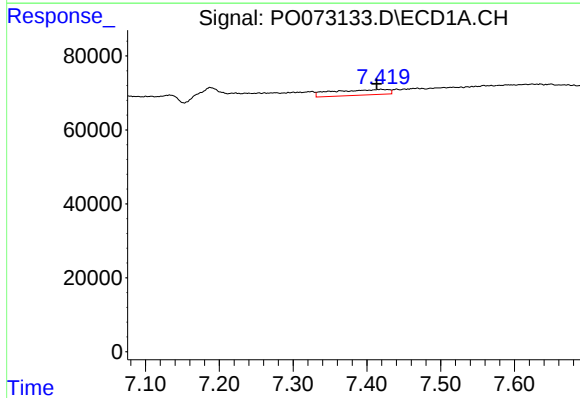


#27 AR-1254-2

R.T.: 7.419 min
Delta R.T.: 0.006 min
Response: 79446
Conc: 22.55 ng/ml

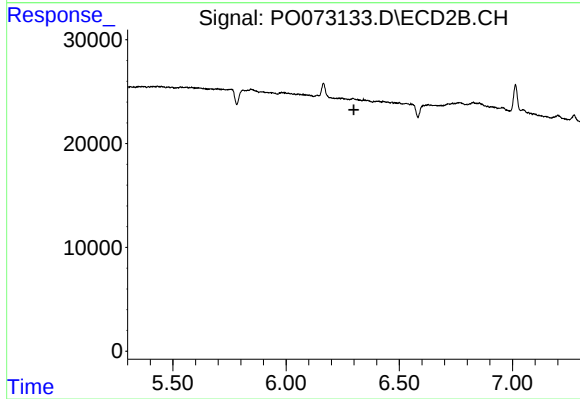

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.299 min
Response: 0
Conc: N.D.

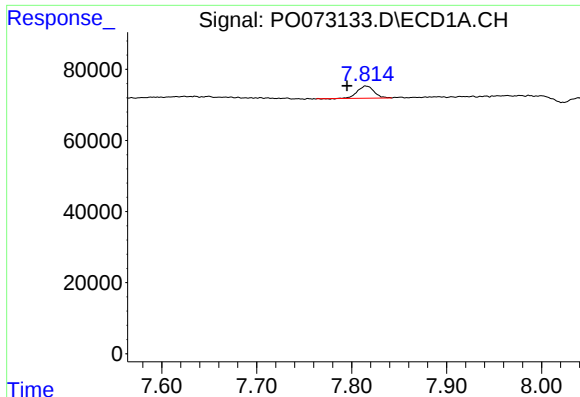

#28 AR-1254-3


R.T.: 7.815 min
Delta R.T.: 0.020 min
Response: 41555
Conc: 11.55 ng/ml

Instrument :
ECD_O
ClientSampleId :

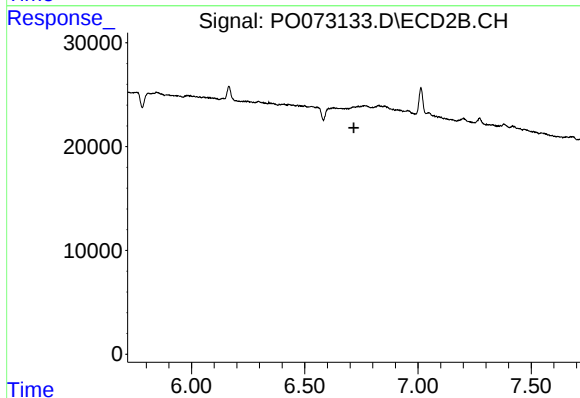


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.717 min
Response: 0
Conc: N.D.

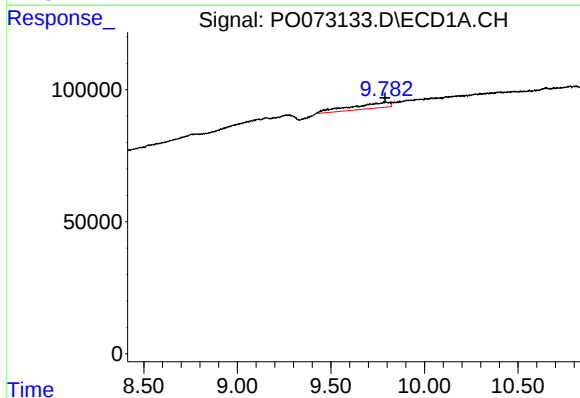


#43 AR-1268-3

R.T.: 9.792 min
Delta R.T.: 0.004 min
Response: 314131
Conc: 56.24 ng/ml

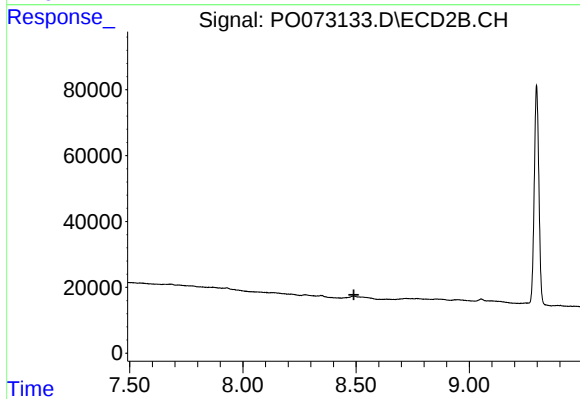

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.490 min
Response: 0
Conc: N.D.

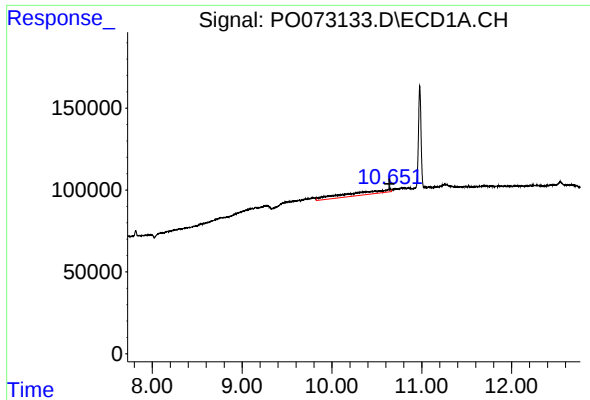

#45 AR-1268-5

R.T.: 10.652 min
Delta R.T.: 0.012 min
Response: 770650
Conc: 47.65 ng/ml

Instrument :
ECD_O
ClientSampleId :

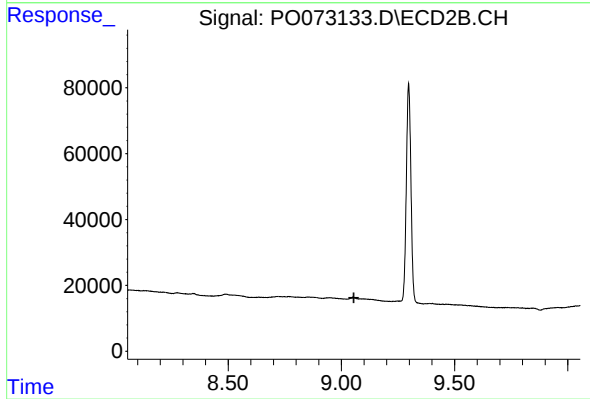

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.055 min
Response: 0
Conc: N.D.