

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110620\
 Data File : PO073149.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Nov 2020 19:09
 Operator : DD\AJ
 Sample : L4636-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRUM-COMP-1-AU

Manual Integrations
 APPROVED

Ankita
 11/9/2020 3:02:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 23:53:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 05:38:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.947	4.021	743756	465907	14.033m	13.038m
2) SA Decachlor...	10.975	9.295	548873	189995	13.263	5.695 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110620\
Data File : PO073149.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Nov 2020 19:09
Operator : DD\AJ
Sample : L4636-09
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DRUM-COMP-1-AU


Manual Integrations
APPROVED

Ankita
11/9/2020 3:02:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 23:53:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 05:38:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

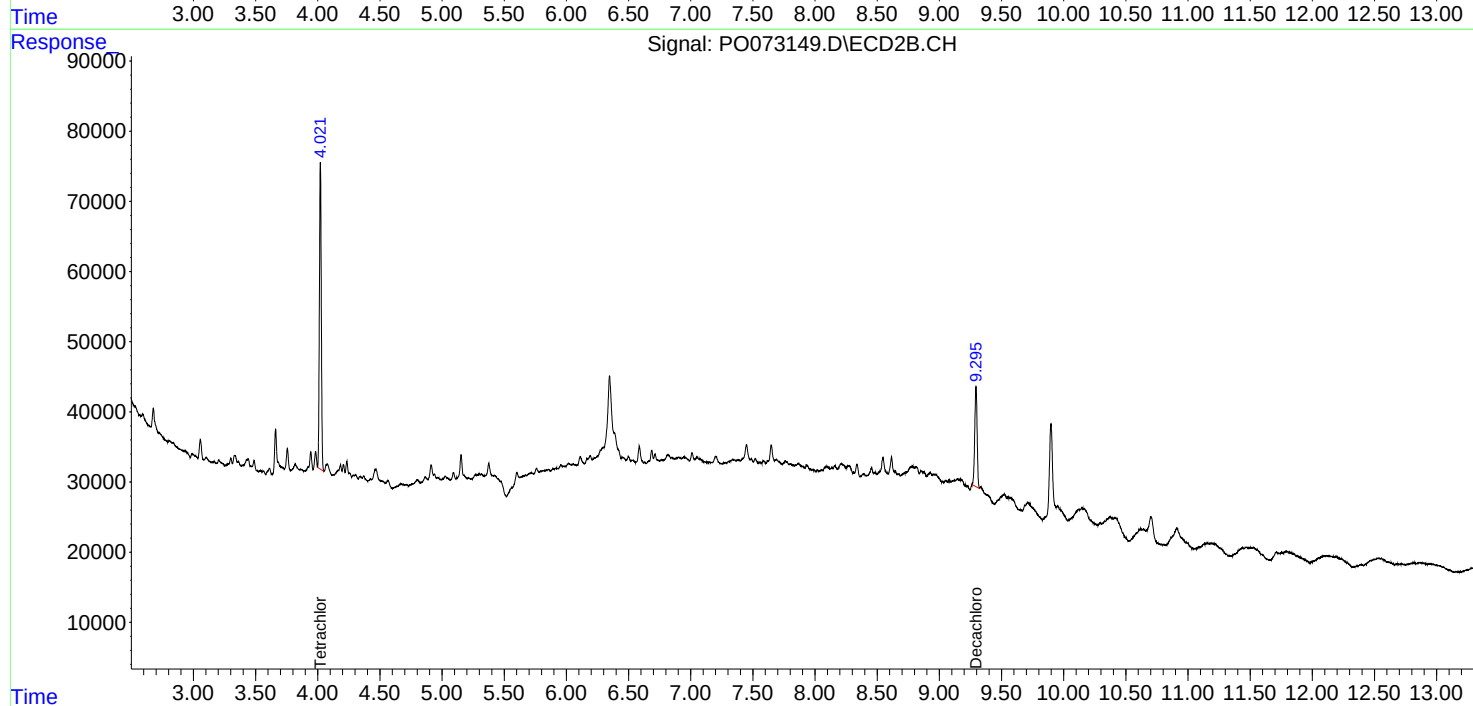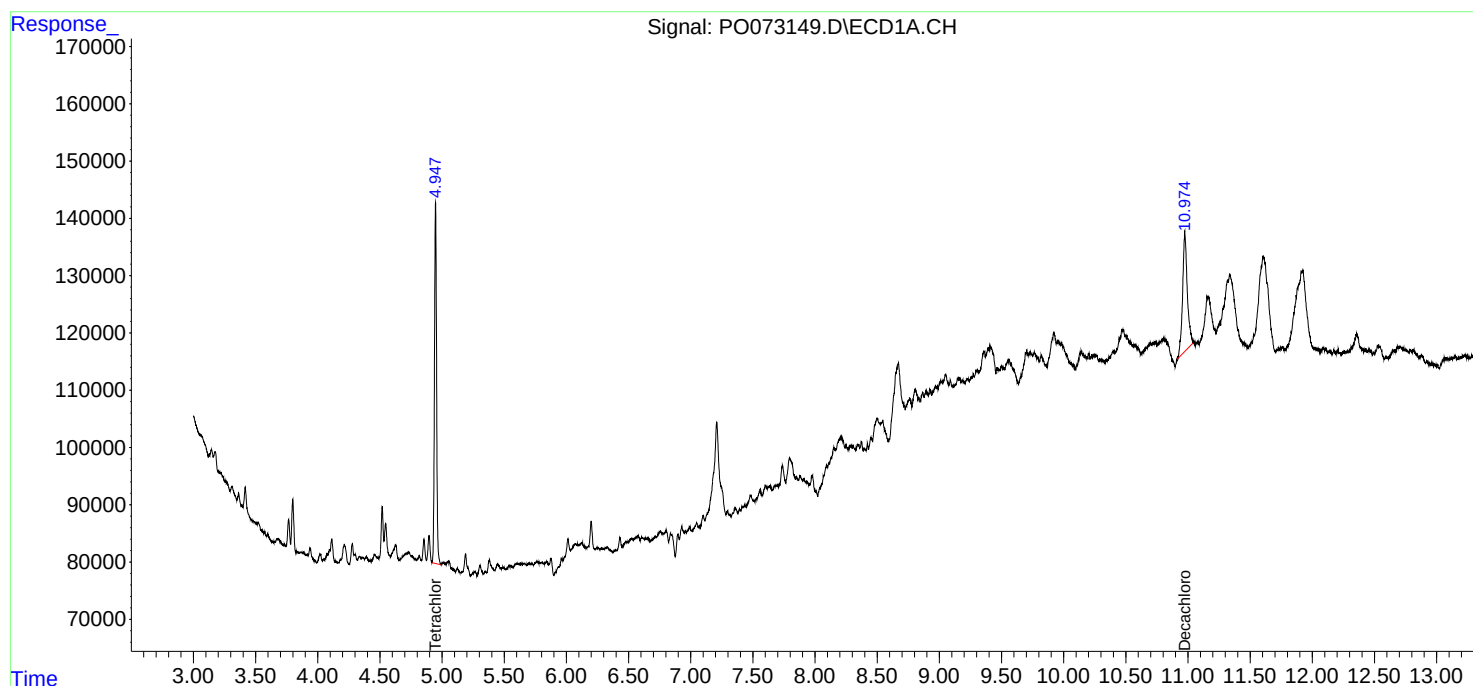

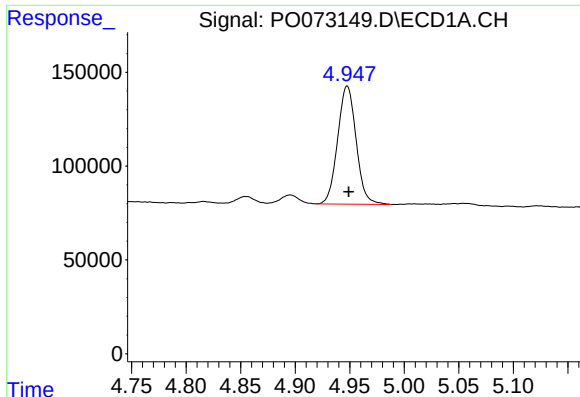


#1 Tetrachloro-m-xylene

R.T.: 4.947 min
Delta R.T.: -0.002 min
Response: 743756
Conc: 14.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DRUM-COMP-1-AU


Manual Integrations
APPROVED

Ankita
11/9/2020 3:02:55 PM

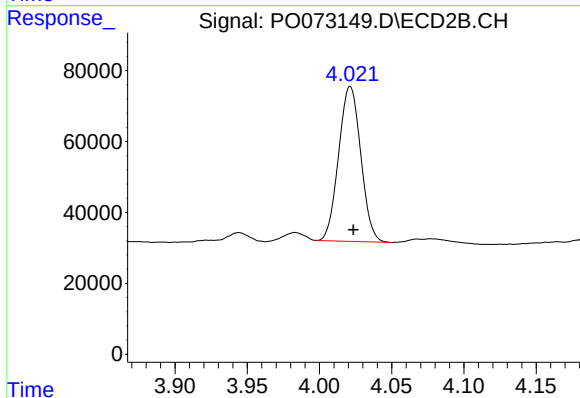


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: -0.003 min
Response: 465907
Conc: 13.04 ng/ml m

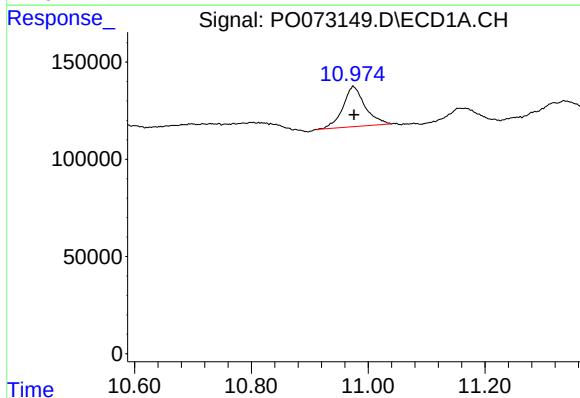

#2 Decachlorobiphenyl

R.T.: 10.975 min
Delta R.T.: -0.001 min
Response: 548873
Conc: 13.26 ng/ml

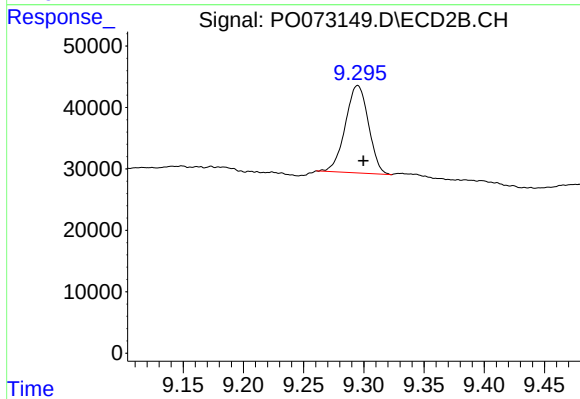

#2 Decachlorobiphenyl

R.T.: 9.295 min
Delta R.T.: -0.005 min
Response: 189995
Conc: 5.69 ng/ml