

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110623\
 Data File : PO099392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2023 11:12
 Operator : YP/AJ
 Sample : PB156872BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB156872BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/07/2023
 Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 12:35:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.467	3.623	40602005	14528346	20.548	20.187m
2) SA Decachlor...	10.260	8.613	30281188	12061055	26.730	22.480

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110623\
Data File : PO099392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2023 11:12
Operator : YP/AJ
Sample : PB156872BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB156872BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 12:35:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

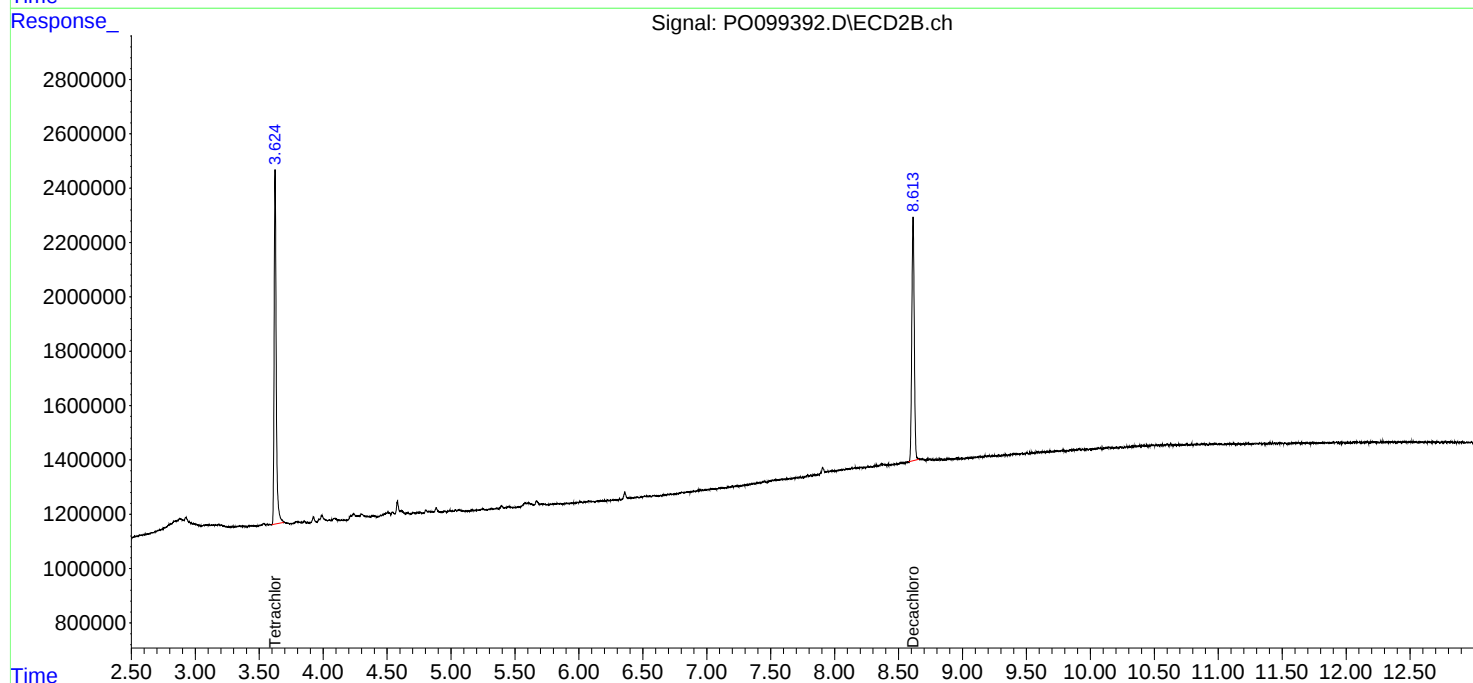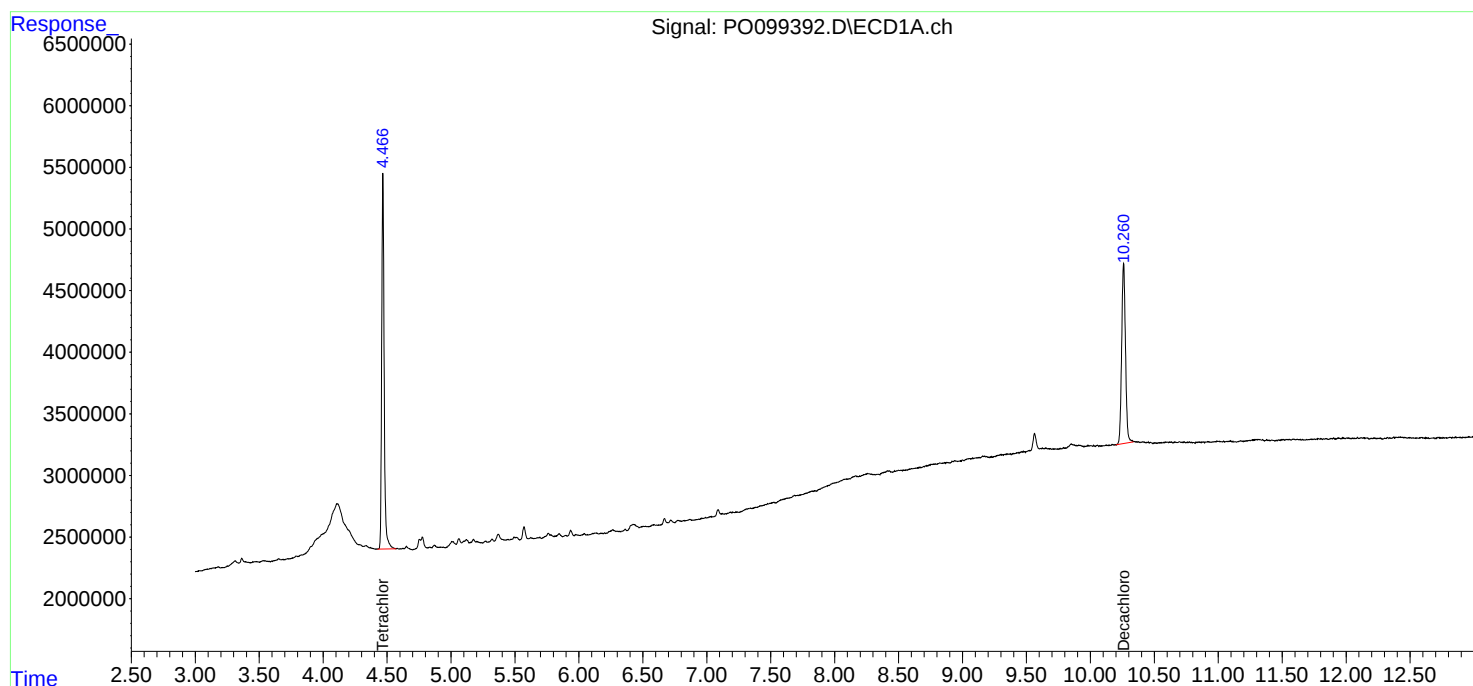

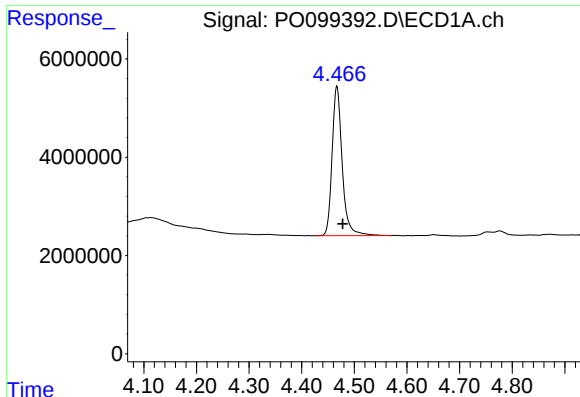


#1 Tetrachloro-m-xylene

R.T.: 4.467 min
Delta R.T.: -0.011 min
Response: 40602005
Conc: 20.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB156872BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

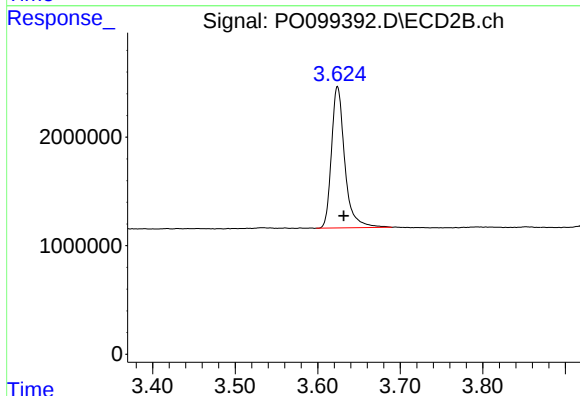


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.008 min
Response: 14528346
Conc: 20.19 ng/ml m

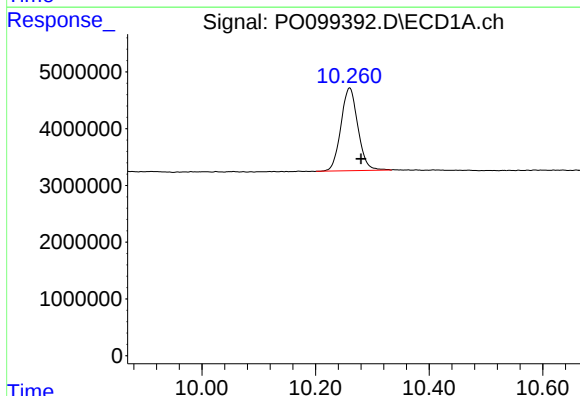

#2 Decachlorobiphenyl

R.T.: 10.260 min
Delta R.T.: -0.020 min
Response: 30281188
Conc: 26.73 ng/ml

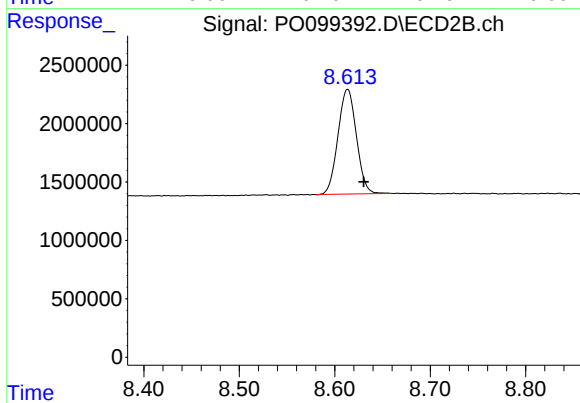

#2 Decachlorobiphenyl

R.T.: 8.613 min
Delta R.T.: -0.017 min
Response: 12061055
Conc: 22.48 ng/ml