

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110623\
 Data File : PO099396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2023 12:20
 Operator : YP/AJ
 Sample : 05234-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/07/2023
 Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 23:06:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.467	3.623	41046052	14602939	20.773	20.291m
2) SA Decachlor...	10.259	8.613	28237075	11035587	24.925	20.568
Target Compounds						
31) L7 AR-1260-1	7.247	6.182	2765294	1299808	38.589	36.847
32) L7 AR-1260-2	7.505	6.370	1774022	1112542	22.485	27.754
33) L7 AR-1260-3	7.865	6.524	2363474	1185687	43.277	31.357 #
34) L7 AR-1260-4	8.090	6.995	3105410	1328838	49.562m	45.986
35) L7 AR-1260-5	8.414	7.237	5530627	2451745	51.681	40.740

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110623\
Data File : PO099396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2023 12:20
Operator : YP/AJ
Sample : 05234-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 23:06:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

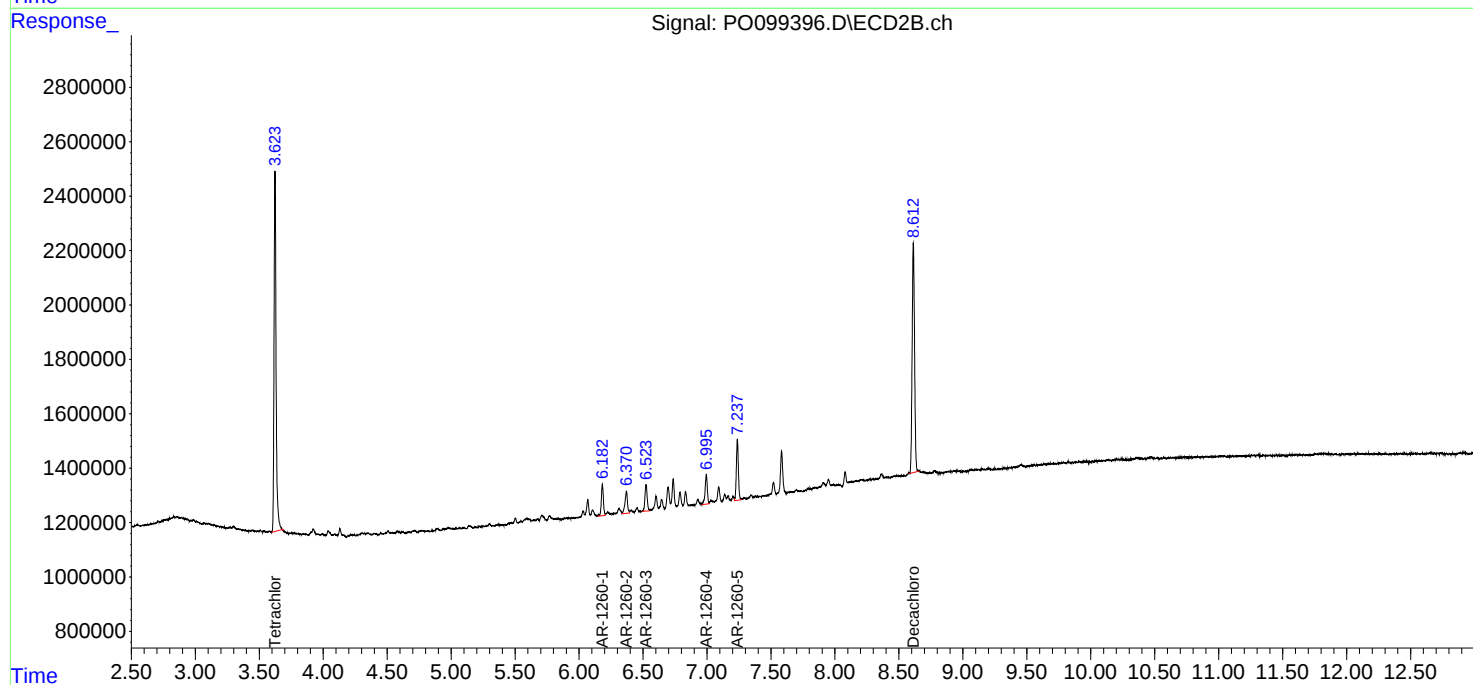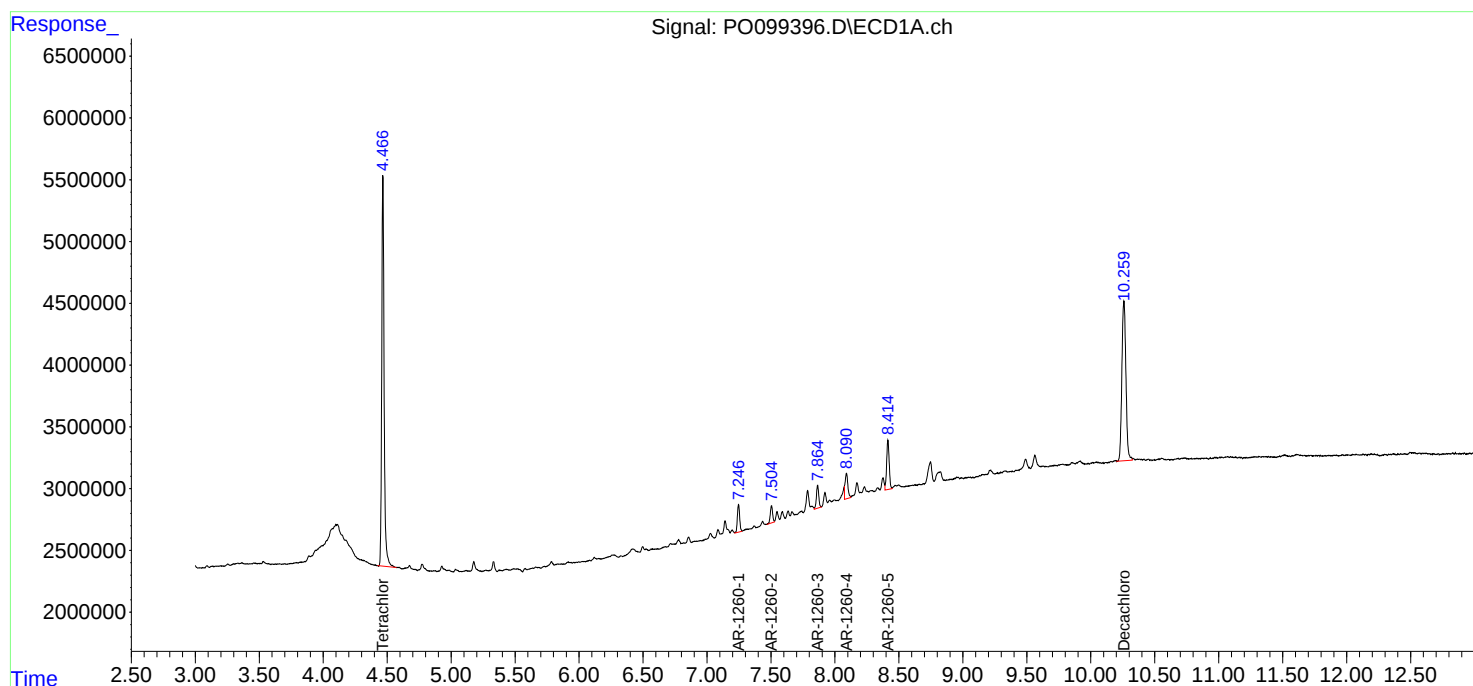

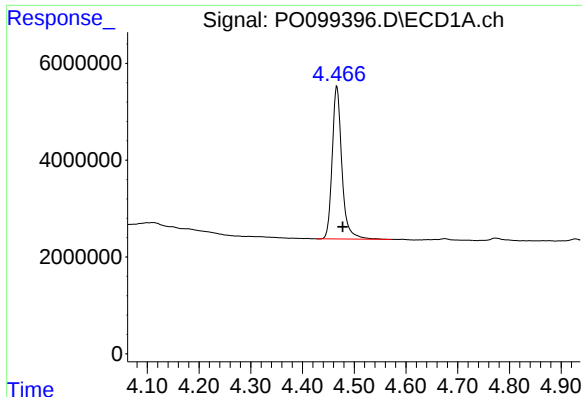


#1 Tetrachloro-m-xylene

R.T.: 4.467 min
Delta R.T.: -0.011 min
Response: 41046052
Conc: 20.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

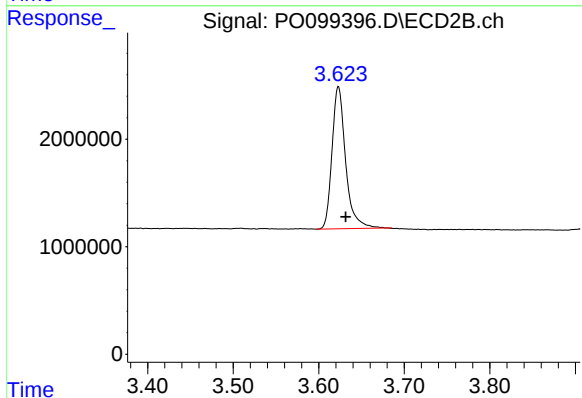


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.009 min
Response: 14602939
Conc: 20.29 ng/ml m

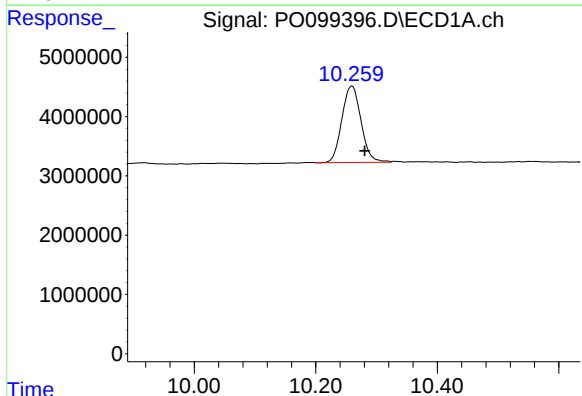


#2 Decachlorobiphenyl

R.T.: 10.259 min
Delta R.T.: -0.021 min
Response: 28237075
Conc: 24.93 ng/ml

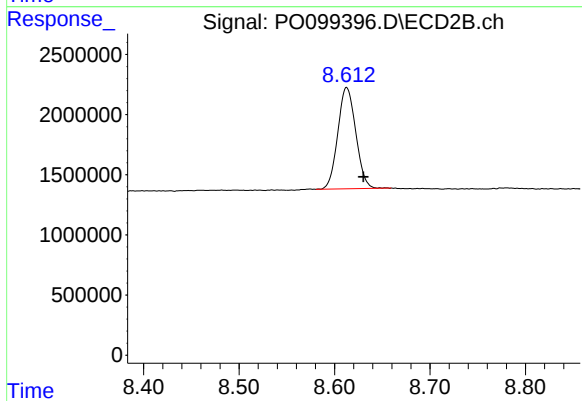

#2 Decachlorobiphenyl

R.T.: 8.613 min
Delta R.T.: -0.017 min
Response: 11035587
Conc: 20.57 ng/ml

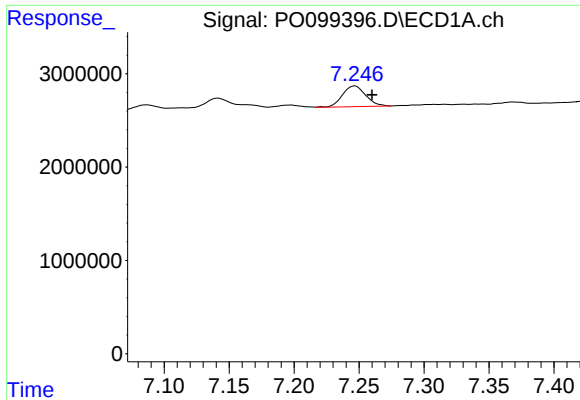


#31 AR-1260-1

R.T.: 7.247 min
Delta R.T.: -0.013 min
Response: 2765294
Conc: 38.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

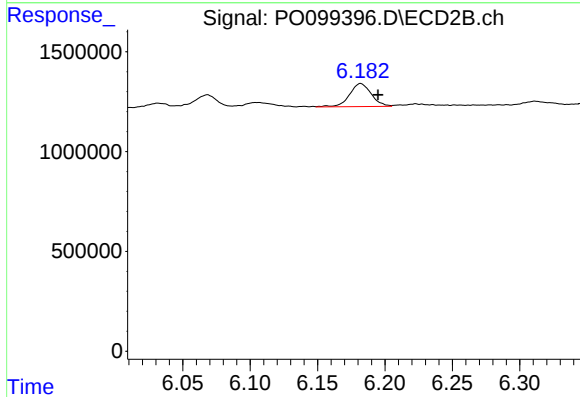


#31 AR-1260-1

R.T.: 6.182 min
Delta R.T.: -0.013 min
Response: 1299808
Conc: 36.85 ng/ml

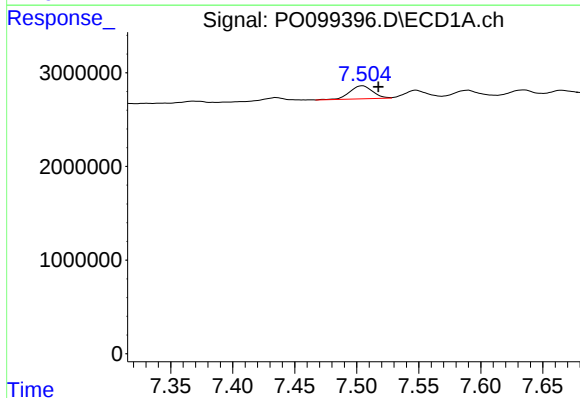


#32 AR-1260-2

R.T.: 7.505 min
Delta R.T.: -0.013 min
Response: 1774022
Conc: 22.49 ng/ml

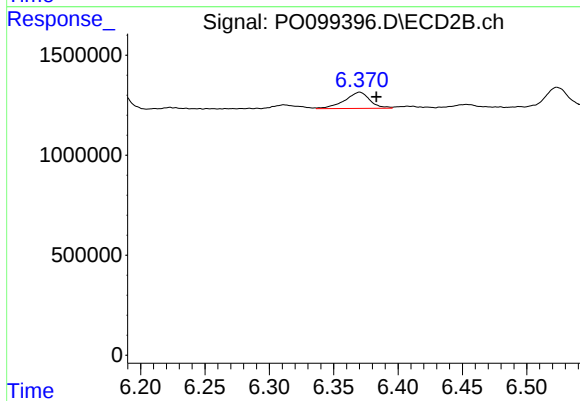

#32 AR-1260-2

R.T.: 6.370 min
Delta R.T.: -0.013 min
Response: 1112542
Conc: 27.75 ng/ml

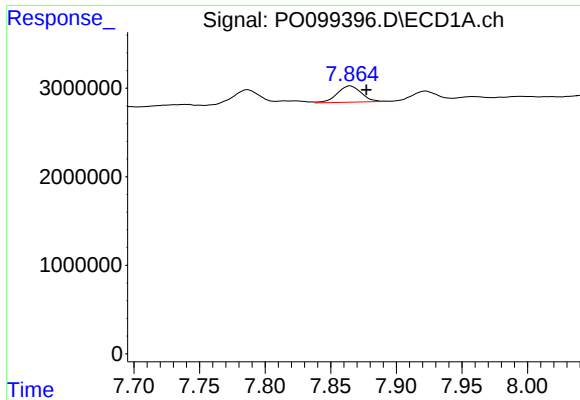


#33 AR-1260-3

R.T.: 7.865 min
Delta R.T.: -0.012 min
Response: 2363474
Conc: 43.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

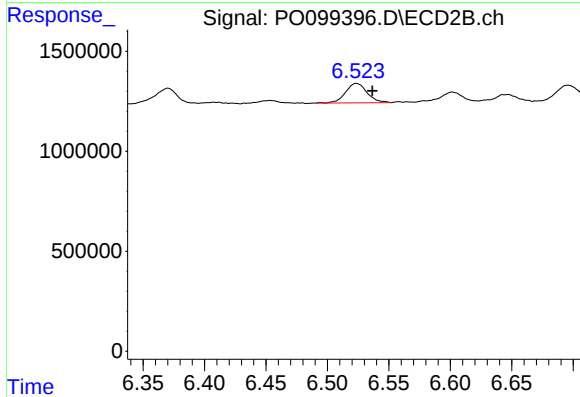


#33 AR-1260-3

R.T.: 6.524 min
Delta R.T.: -0.013 min
Response: 1185687
Conc: 31.36 ng/ml

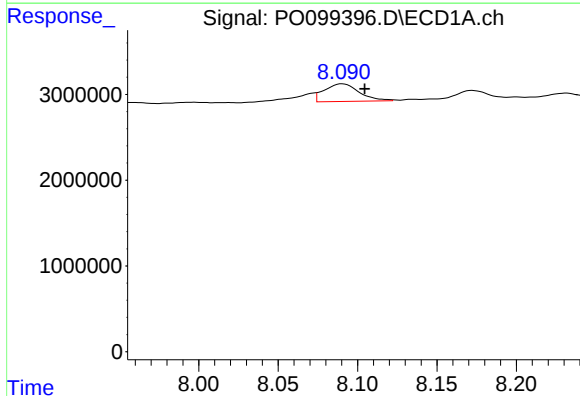


#34 AR-1260-4

R.T.: 8.090 min
Delta R.T.: -0.015 min
Response: 3105410
Conc: 49.56 ng/ml m

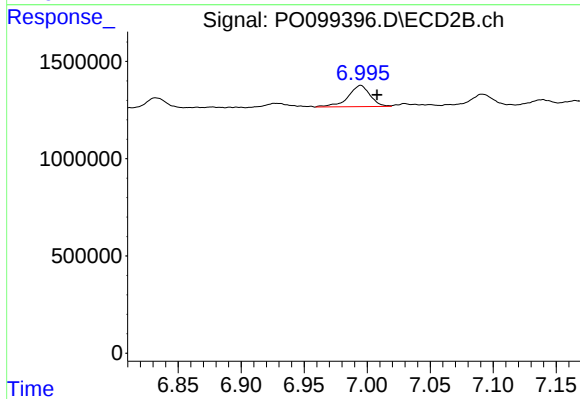

#34 AR-1260-4

R.T.: 6.995 min
Delta R.T.: -0.013 min
Response: 1328838
Conc: 45.99 ng/ml

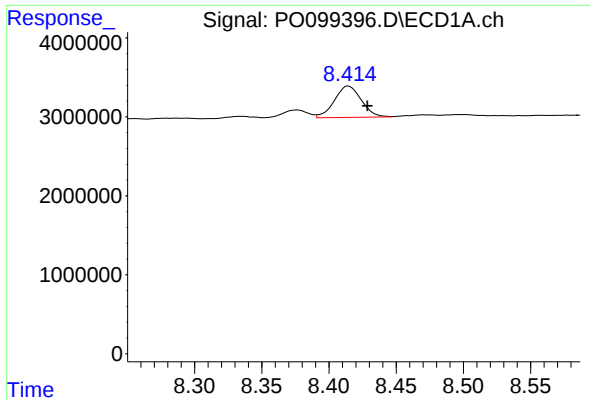


#35 AR-1260-5

R.T.: 8.414 min
Delta R.T.: -0.014 min
Response: 5530627
Conc: 51.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

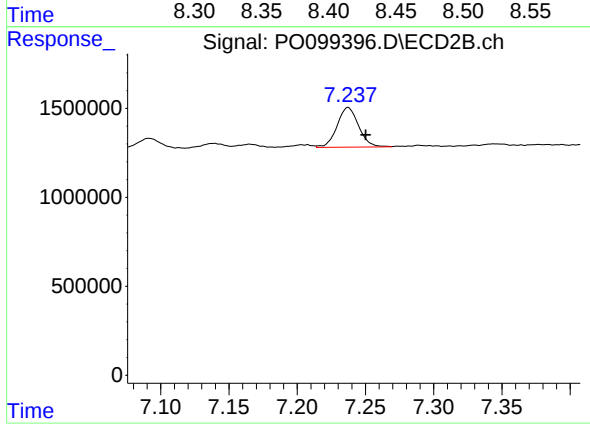

#35 AR-1260-5

R.T.: 7.237 min
Delta R.T.: -0.013 min
Response: 2451745
Conc: 40.74 ng/ml