

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO110623\
 Data File : PO099421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2023 20:39
 Operator : YP/AJ
 Sample : 05244-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 5A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/07/2023
 Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 04:04:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.467	3.623	40281085	14828306	20.386	20.604m
2) SA Decachlor...	10.262	8.613	19900586	8143500	17.567	15.178
Target Compounds						
31) L7 AR-1260-1	7.249	6.183	3787864	1396509	52.858	39.589m#
32) L7 AR-1260-2	7.501	6.371	18042420	1964865	228.684	49.016m#
33) L7 AR-1260-3	7.866	6.524	3870339	1699617	70.869	44.948 #
34) L7 AR-1260-4	8.092	6.995	5133134	1831081	81.925	63.367
35) L7 AR-1260-5	8.417	7.237	6877500	4026174	64.266	66.903

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110623\
Data File : PO099421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2023 20:39
Operator : YP/AJ
Sample : 05244-13
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
5A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 04:04:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

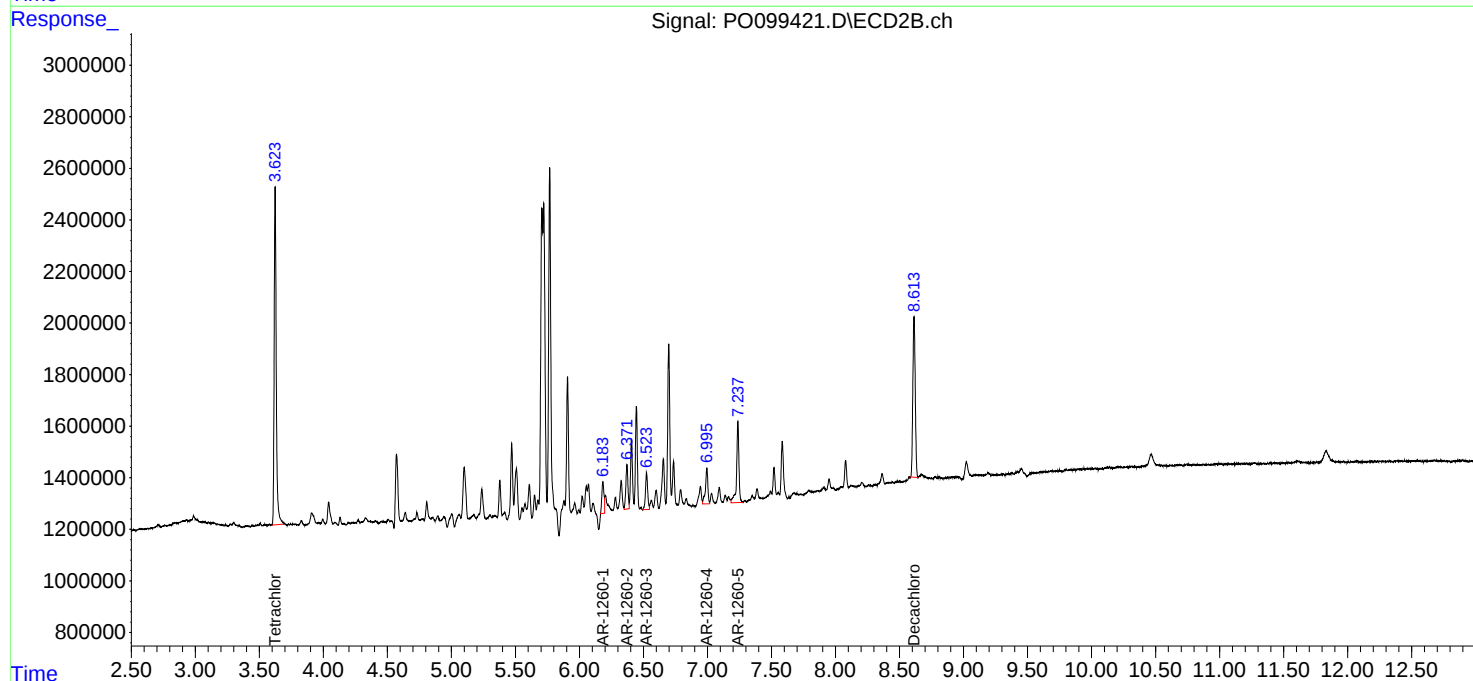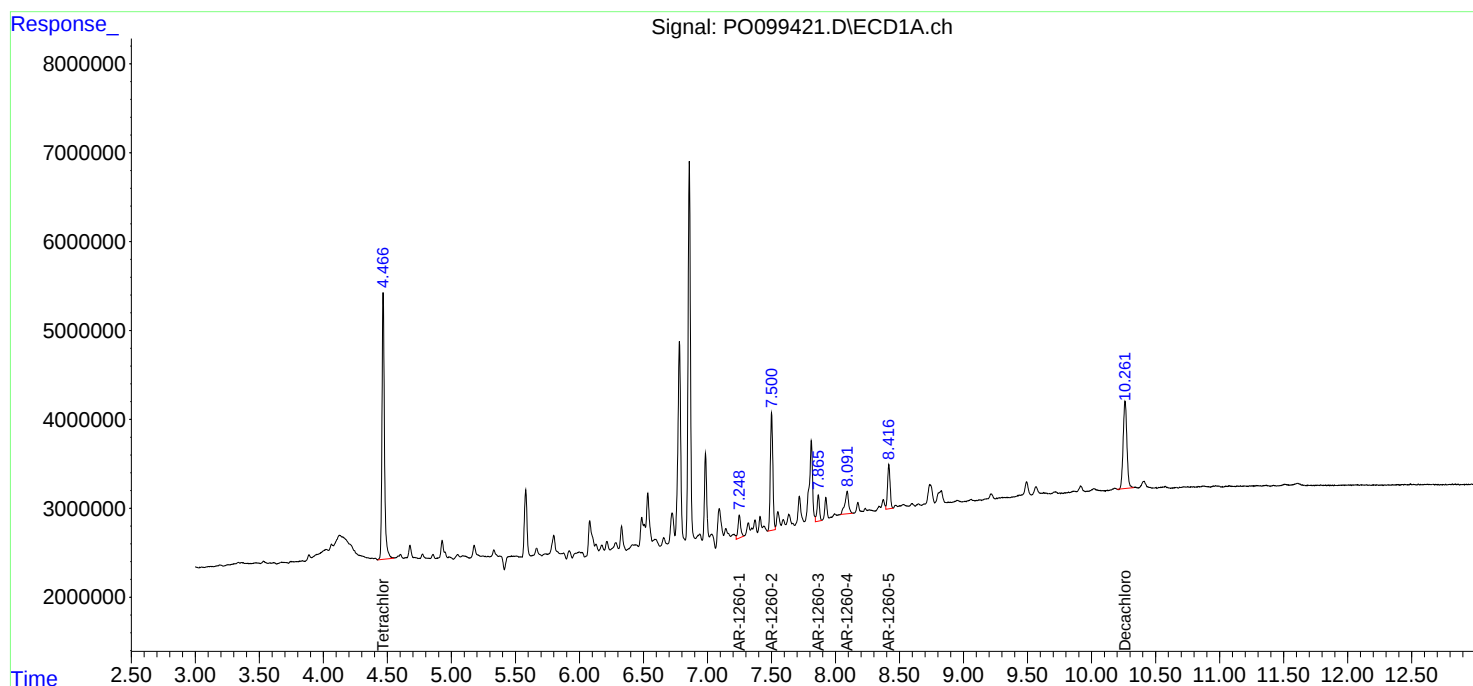

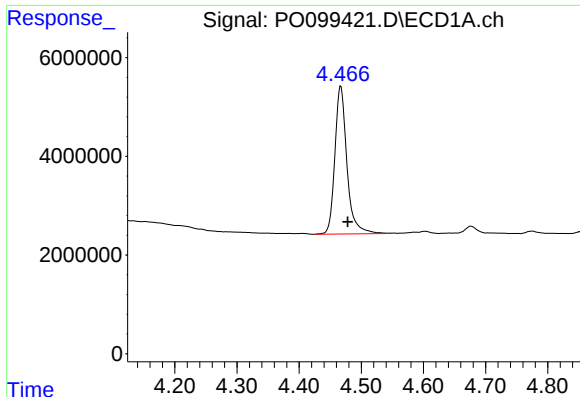


#1 Tetrachloro-m-xylene

R.T.: 4.467 min
Delta R.T.: -0.011 min
Response: 40281085
Conc: 20.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
5A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

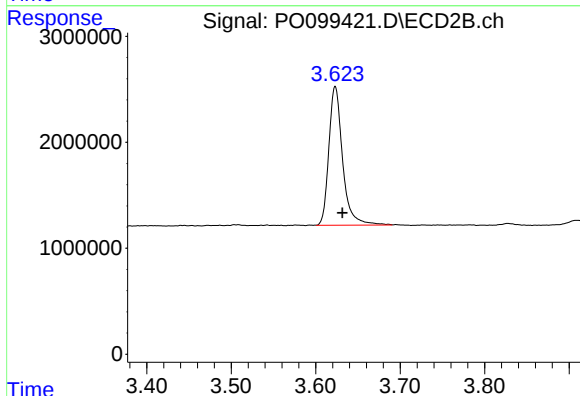


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.009 min
Response: 14828306
Conc: 20.60 ng/ml m

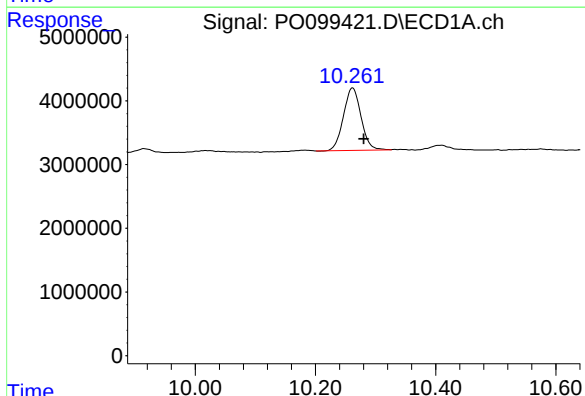


#2 Decachlorobiphenyl

R.T.: 10.262 min
Delta R.T.: -0.018 min
Response: 19900586
Conc: 17.57 ng/ml

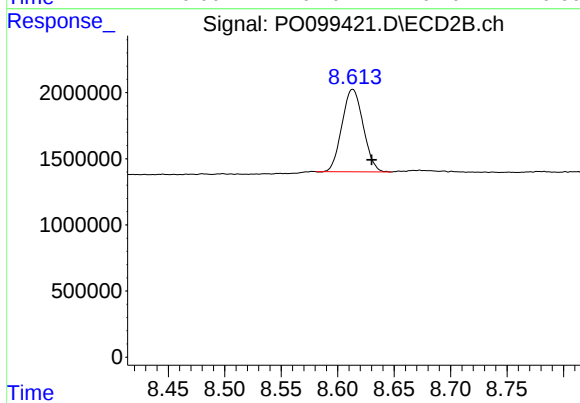

#2 Decachlorobiphenyl

R.T.: 8.613 min
Delta R.T.: -0.017 min
Response: 8143500
Conc: 15.18 ng/ml

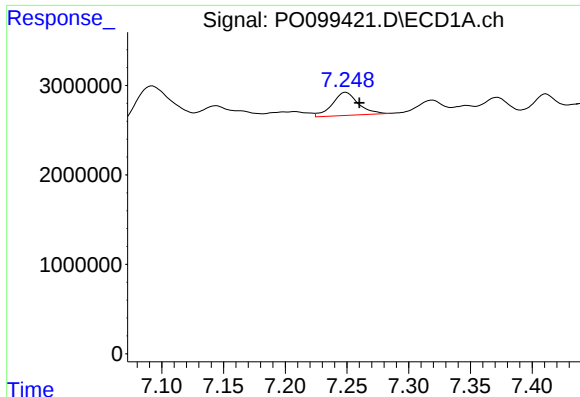


#31 AR-1260-1

R.T.: 7.249 min
Delta R.T.: -0.011 min
Response: 3787864
Conc: 52.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
5A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

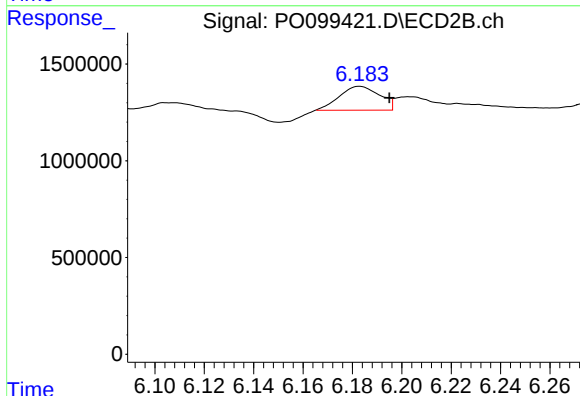


#31 AR-1260-1

R.T.: 6.183 min
Delta R.T.: -0.012 min
Response: 1396509
Conc: 39.59 ng/ml m

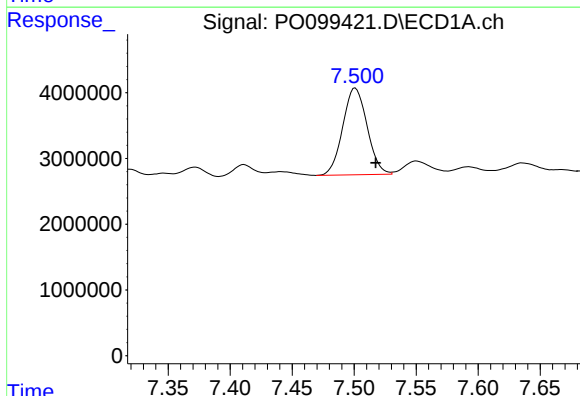


#32 AR-1260-2

R.T.: 7.501 min
Delta R.T.: -0.016 min
Response: 18042420
Conc: 228.68 ng/ml

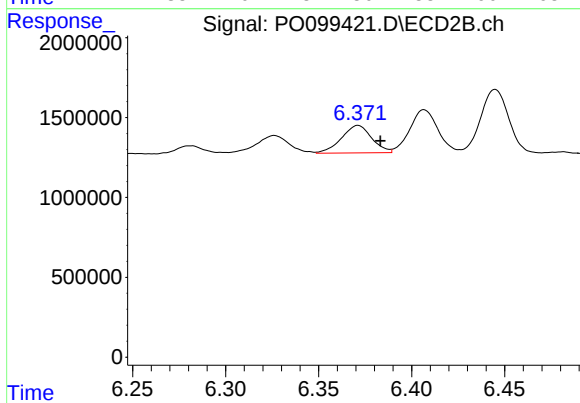

#32 AR-1260-2

R.T.: 6.371 min
Delta R.T.: -0.012 min
Response: 1964865
Conc: 49.02 ng/ml m

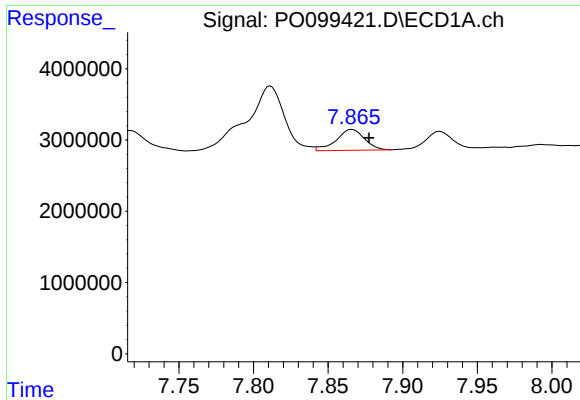


#33 AR-1260-3

R.T.: 7.866 min
Delta R.T.: -0.011 min
Response: 3870339
Conc: 70.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
5A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

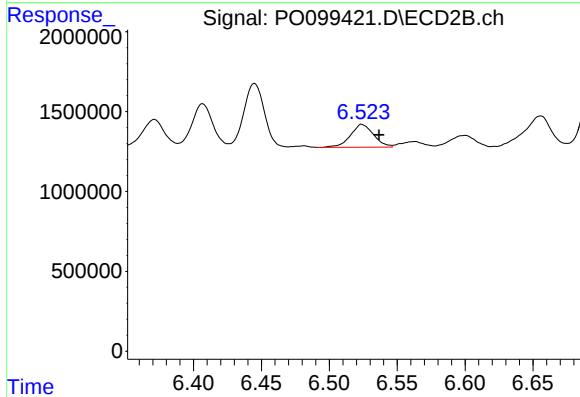


#33 AR-1260-3

R.T.: 6.524 min
Delta R.T.: -0.013 min
Response: 1699617
Conc: 44.95 ng/ml

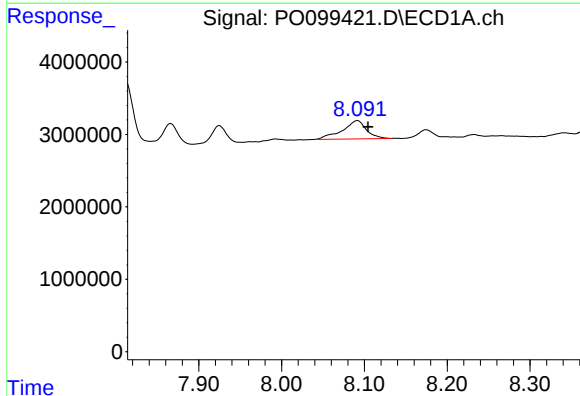


#34 AR-1260-4

R.T.: 8.092 min
Delta R.T.: -0.013 min
Response: 5133134
Conc: 81.92 ng/ml

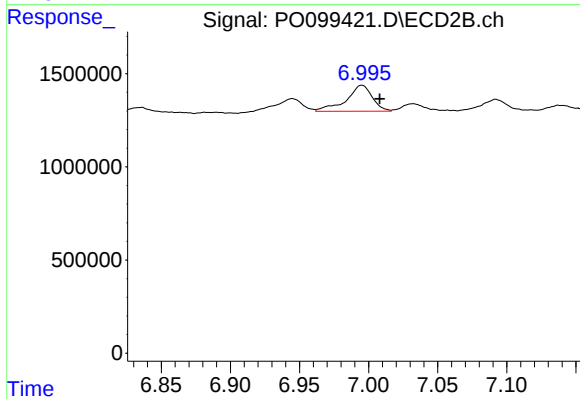

#34 AR-1260-4

R.T.: 6.995 min
Delta R.T.: -0.013 min
Response: 1831081
Conc: 63.37 ng/ml

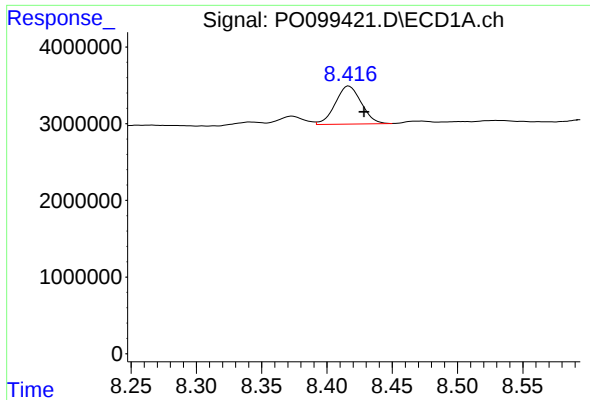


#35 AR-1260-5

R.T.: 8.417 min
Delta R.T.: -0.012 min
Response: 6877500
Conc: 64.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
5A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

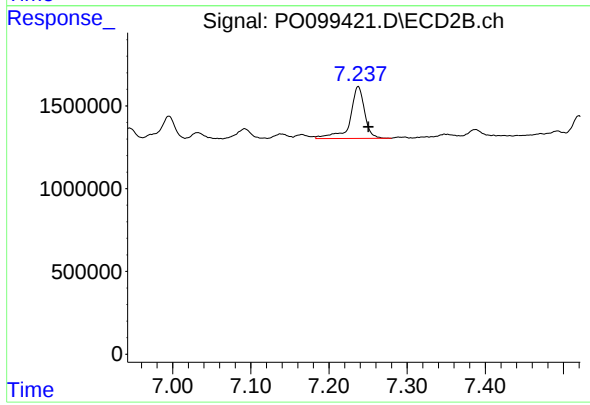

#35 AR-1260-5

R.T.: 7.237 min
Delta R.T.: -0.013 min
Response: 4026174
Conc: 66.90 ng/ml