

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO110623\
 Data File : PO099426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2023 22:04
 Operator : YP/AJ
 Sample : 05245-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 11A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/07/2023
 Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 23:18:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.466	3.622	34924959	12540578	17.675	17.425m
2) SA Decachlor...	10.259	8.612	18346198	7585379	16.194	14.138
Target Compounds						
31) L7 AR-1260-1	7.248	6.181	3651405	1894674	50.954	53.711m
32) L7 AR-1260-2	7.499	6.369	23347673	2890799	295.927	72.114 #
33) L7 AR-1260-3	7.864	6.522	5165071	2421050	94.576	64.027 #
34) L7 AR-1260-4	8.090	6.994	7010270	2153797	111.884	74.535 #
35) L7 AR-1260-5	8.414	7.237	10047288	5433177	93.886	90.283

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110623\
Data File : PO099426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2023 22:04
Operator : YP/AJ
Sample : 05245-11
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
11A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 23:18:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

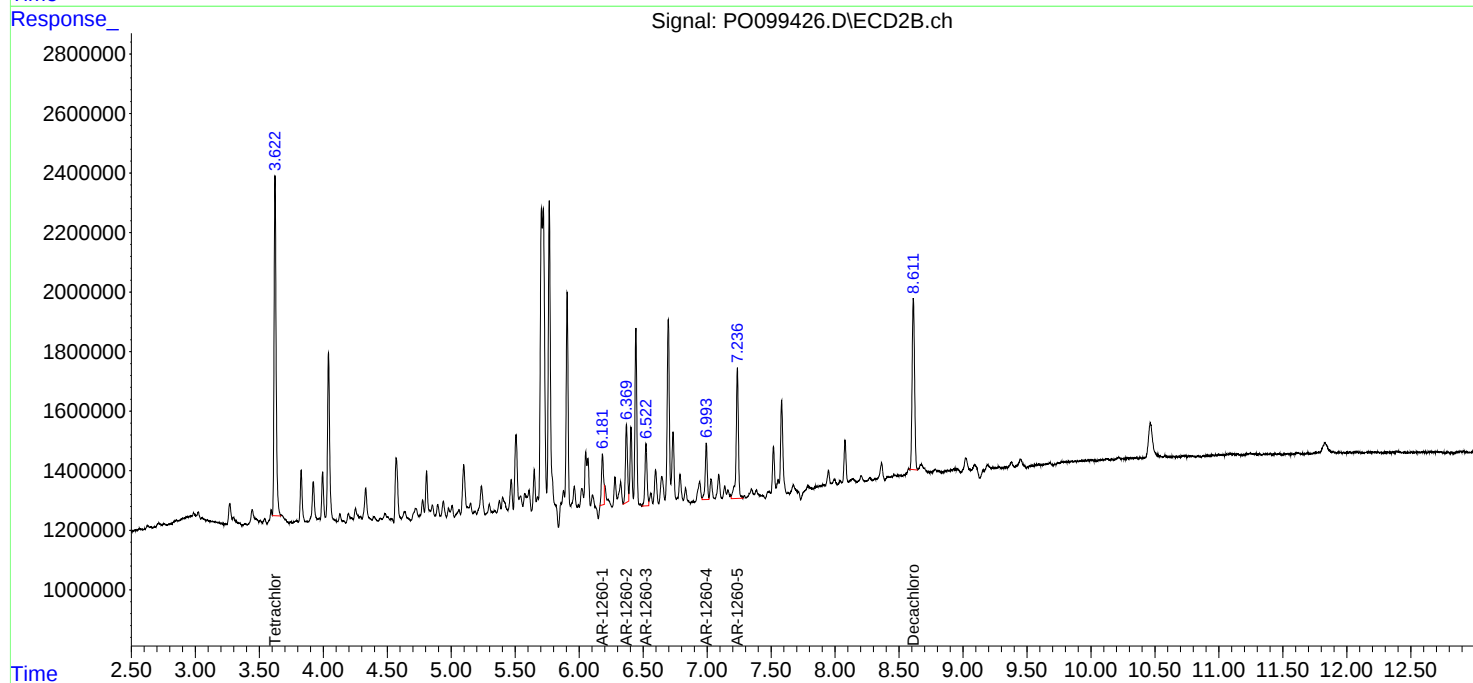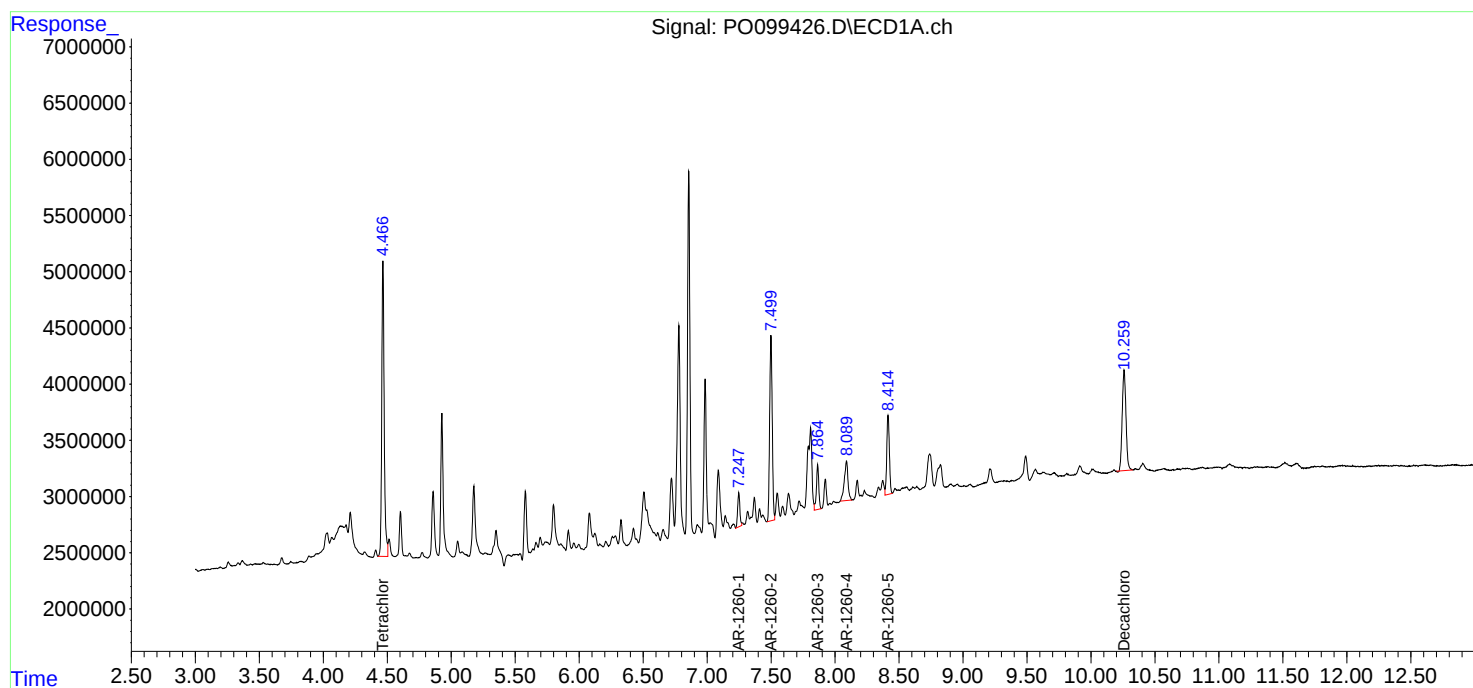

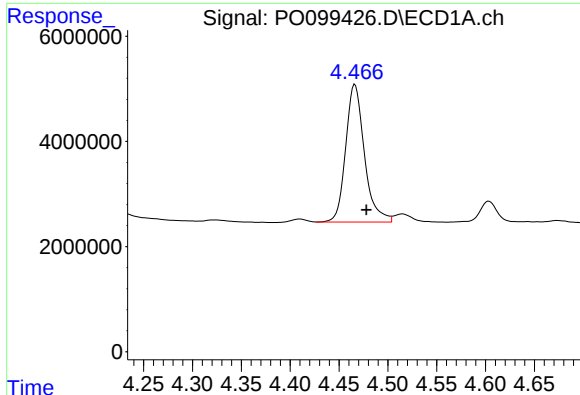


#1 Tetrachloro-m-xylene

R.T.: 4.466 min
Delta R.T.: -0.012 min
Response: 34924959
Conc: 17.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
11A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

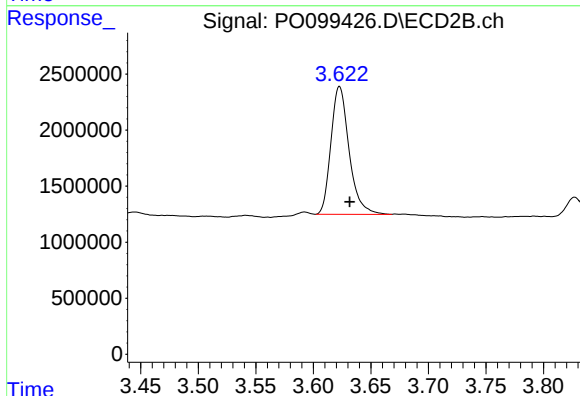


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.009 min
Response: 12540578
Conc: 17.43 ng/ml m

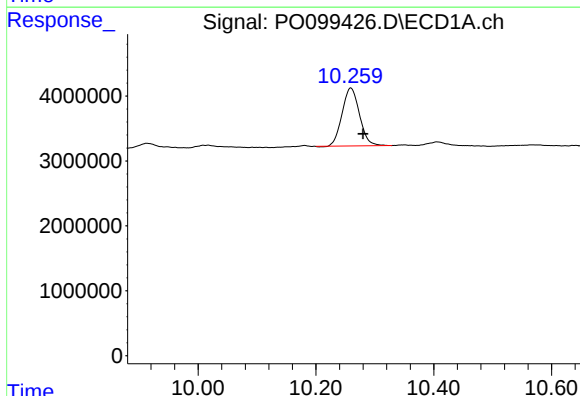


#2 Decachlorobiphenyl

R.T.: 10.259 min
Delta R.T.: -0.021 min
Response: 18346198
Conc: 16.19 ng/ml

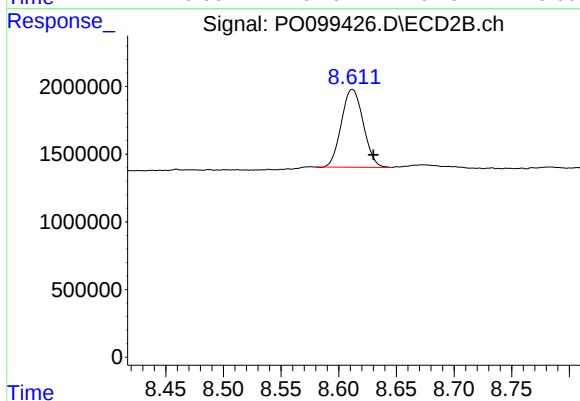

#2 Decachlorobiphenyl

R.T.: 8.612 min
Delta R.T.: -0.018 min
Response: 7585379
Conc: 14.14 ng/ml

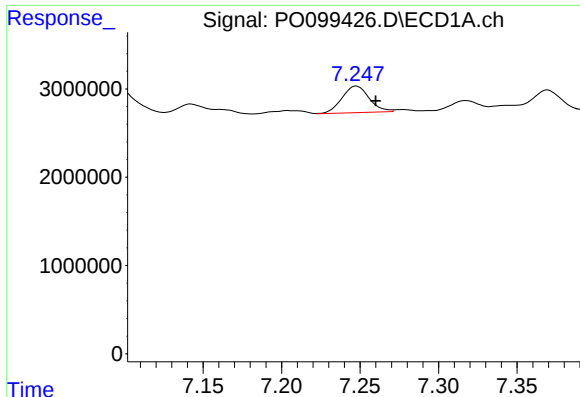


#31 AR-1260-1

R.T.: 7.248 min
Delta R.T.: -0.012 min
Response: 3651405
Conc: 50.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
11A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

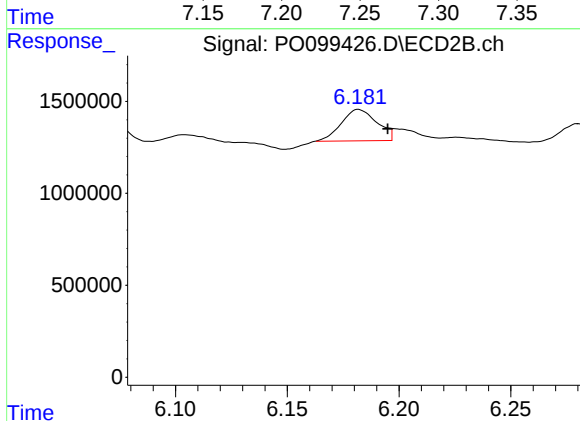


#31 AR-1260-1

R.T.: 6.181 min
Delta R.T.: -0.014 min
Response: 1894674
Conc: 53.71 ng/ml m

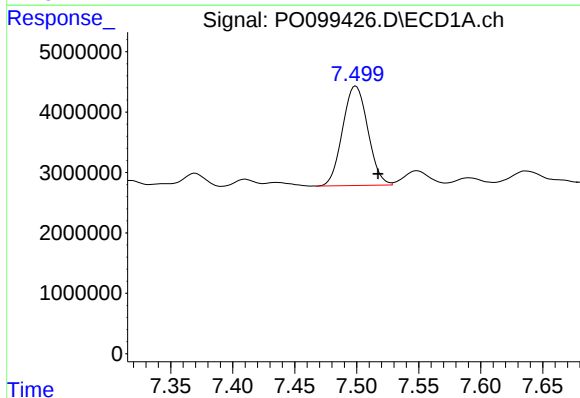


#32 AR-1260-2

R.T.: 7.499 min
Delta R.T.: -0.018 min
Response: 23347673
Conc: 295.93 ng/ml

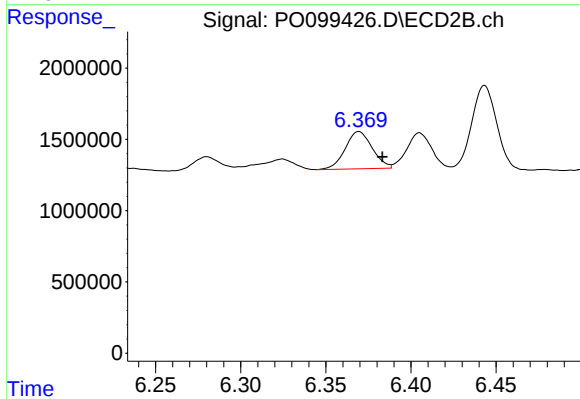

#32 AR-1260-2

R.T.: 6.369 min
Delta R.T.: -0.014 min
Response: 2890799
Conc: 72.11 ng/ml

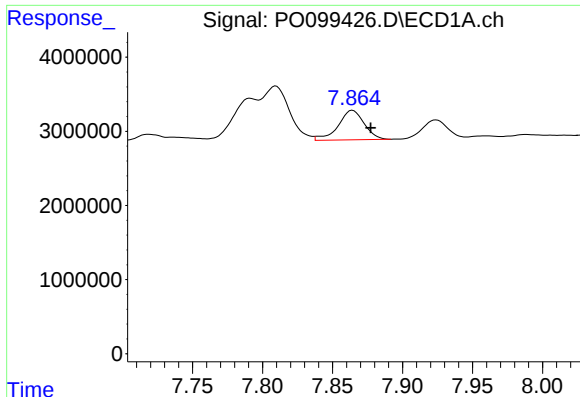


#33 AR-1260-3

R.T.: 7.864 min
Delta R.T.: -0.013 min
Response: 5165071
Conc: 94.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
11A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

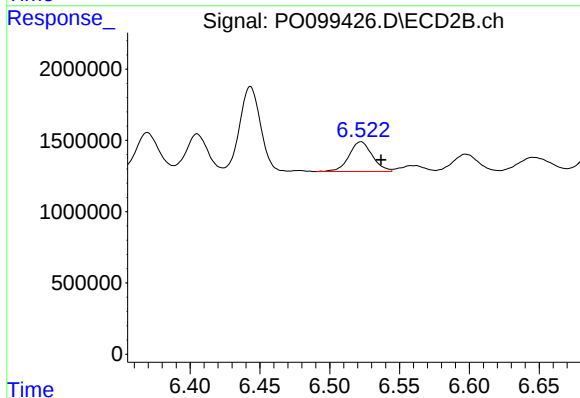


#33 AR-1260-3

R.T.: 6.522 min
Delta R.T.: -0.014 min
Response: 2421050
Conc: 64.03 ng/ml

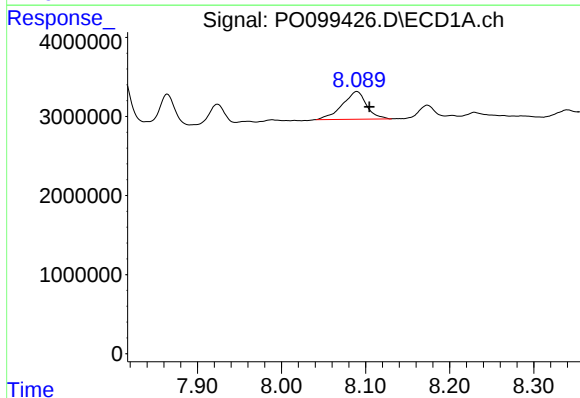


#34 AR-1260-4

R.T.: 8.090 min
Delta R.T.: -0.015 min
Response: 7010270
Conc: 111.88 ng/ml

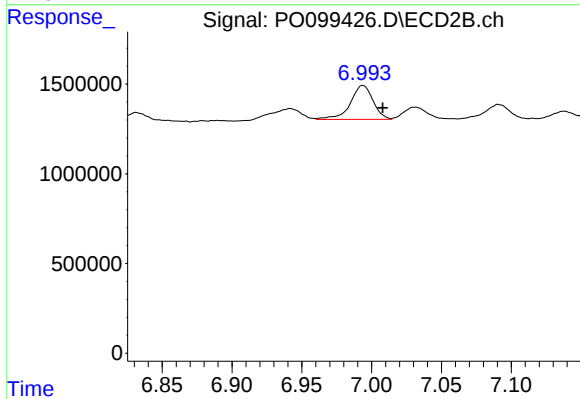

#34 AR-1260-4

R.T.: 6.994 min
Delta R.T.: -0.014 min
Response: 2153797
Conc: 74.53 ng/ml

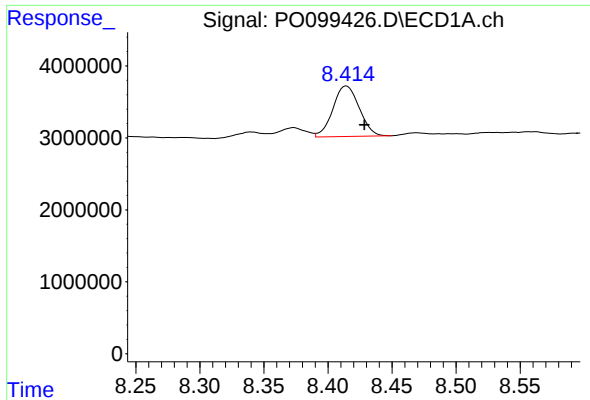


#35 AR-1260-5

R.T.: 8.414 min
Delta R.T.: -0.014 min
Response: 10047288
Conc: 93.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
11A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/07/2023
Supervised By :Ankita Jodhani 11/07/2023

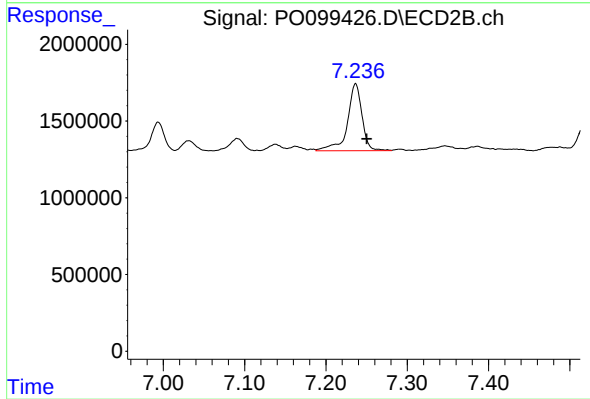

#35 AR-1260-5

R.T.: 7.237 min
Delta R.T.: -0.014 min
Response: 5433177
Conc: 90.28 ng/ml