

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110624\
 Data File : P0107754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 20:24
 Operator : YP/AJ
 Sample : P4704-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NWB-2108

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 00:46:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.372	3.643	194.4E6	74398685	21.327	23.116
2) SA Decachlor...	10.075	8.637	46747490	55387489	19.054	20.203

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110624\
Data File : PO107754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 20:24
Operator : YP/AJ
Sample : P4704-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NWB-2108

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 00:46:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

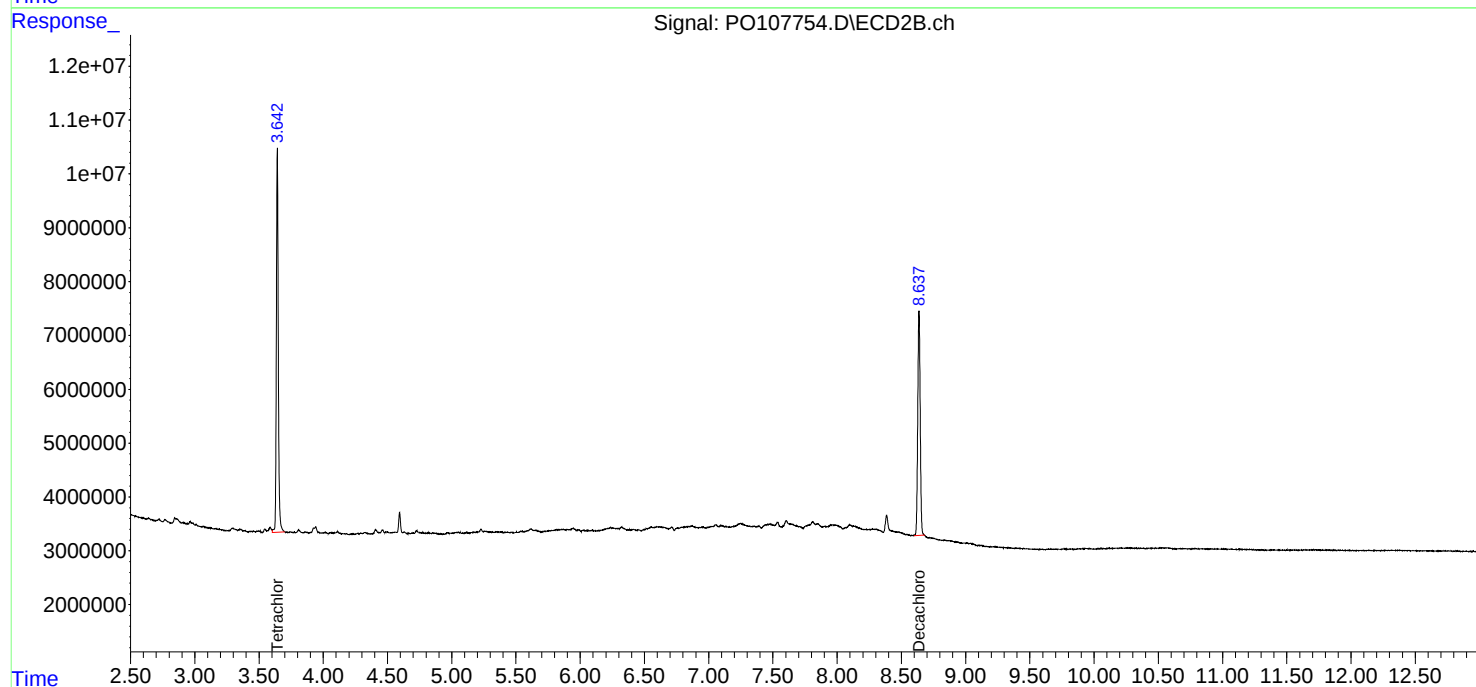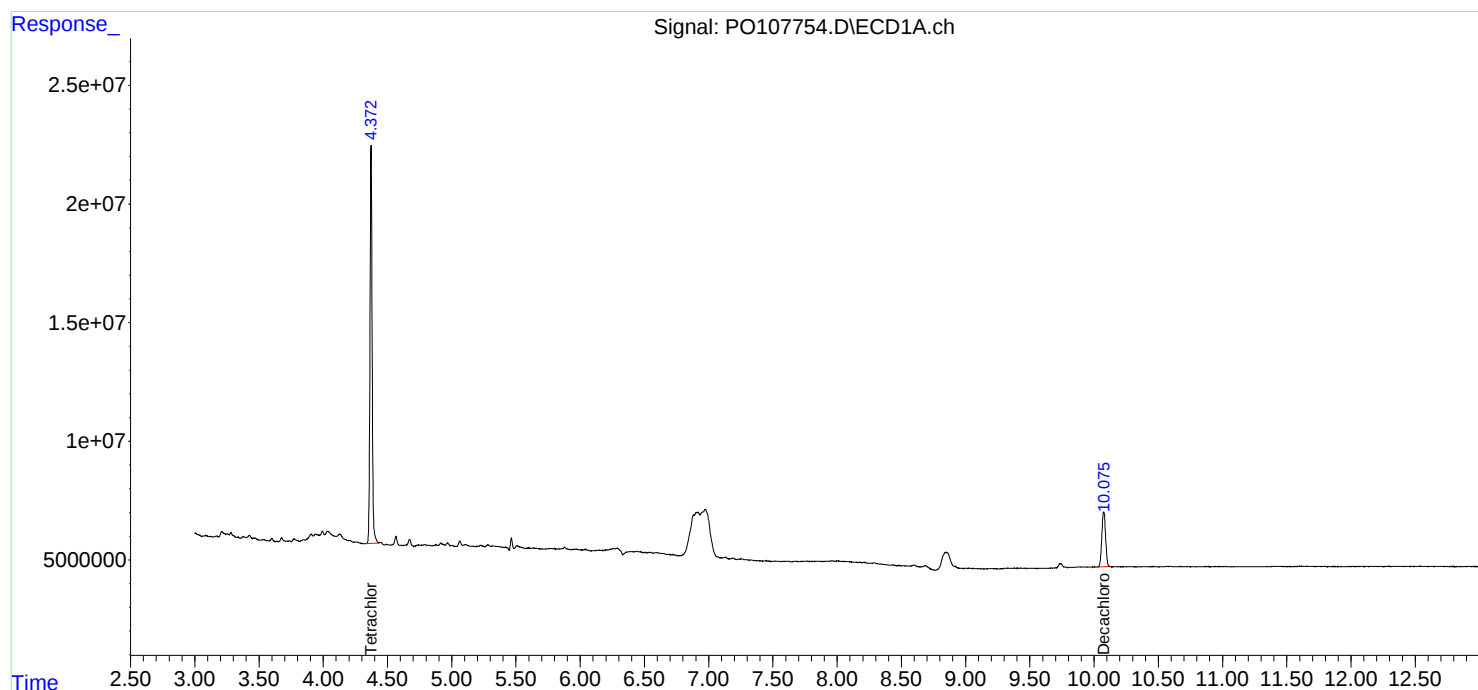


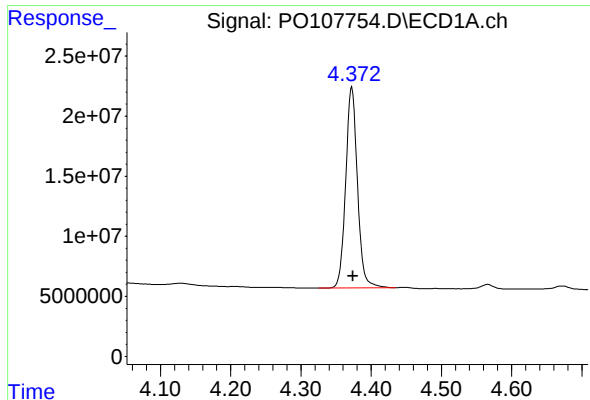

#1 Tetrachloro-m-xylene


R.T.: 4.372 min
Delta R.T.: -0.002 min
Response: 194369432
Conc: 21.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
NWB-2108

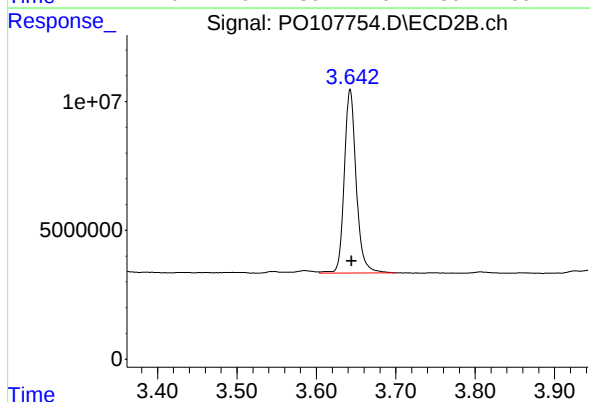


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.002 min
Response: 74398685
Conc: 23.12 ng/ml

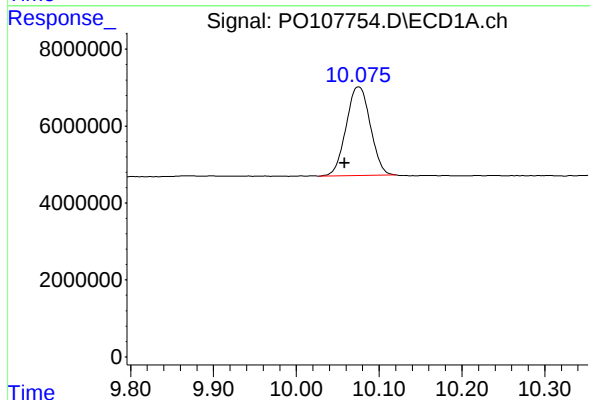

#2 Decachlorobiphenyl

R.T.: 10.075 min
Delta R.T.: 0.017 min
Response: 46747490
Conc: 19.05 ng/ml

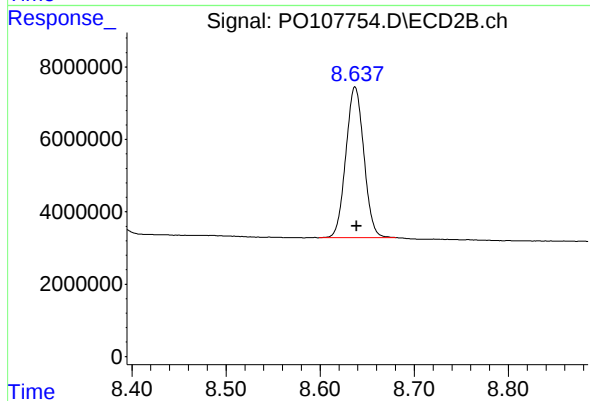

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: -0.002 min
Response: 55387489
Conc: 20.20 ng/ml