

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110723\
 Data File : PO099455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 10:28
 Operator : YP/AJ
 Sample : 05257-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2023
 Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 22:04:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.466	3.622	45059936	16971346	22.804	23.582m
2) SA Decachlor...	10.263	8.615	26015881	10601565	22.965	19.759

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO110723\
Data File : PO099455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 10:28
Operator : YP/AJ
Sample : 05257-09
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
WC-3


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/08/2023
Supervised By : Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 22:04:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

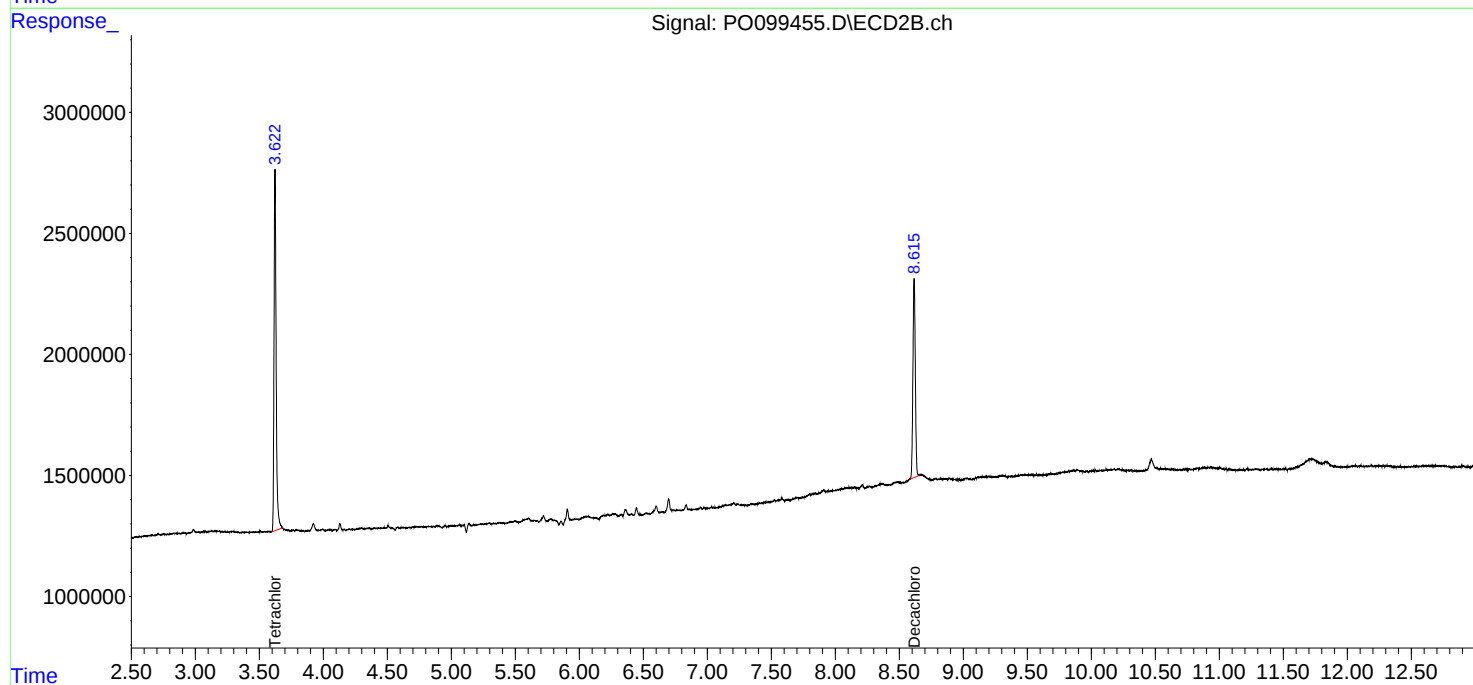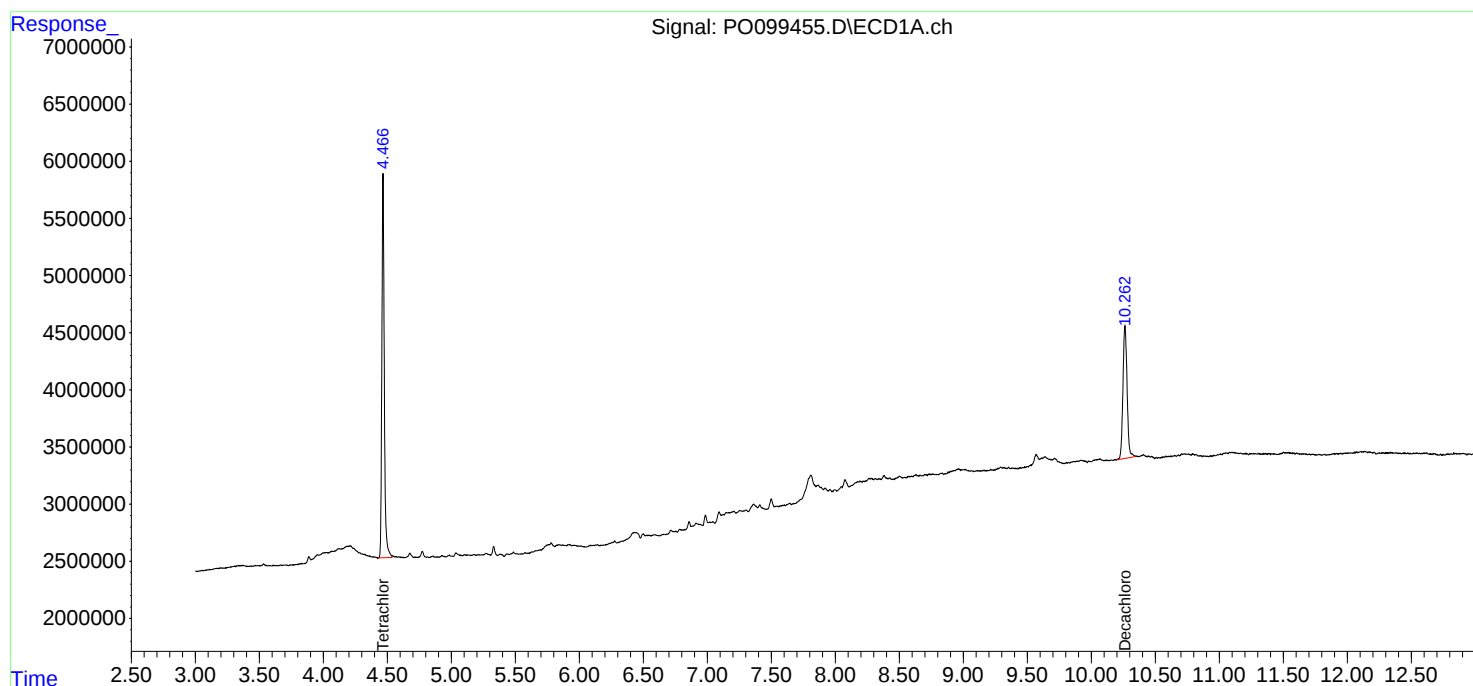

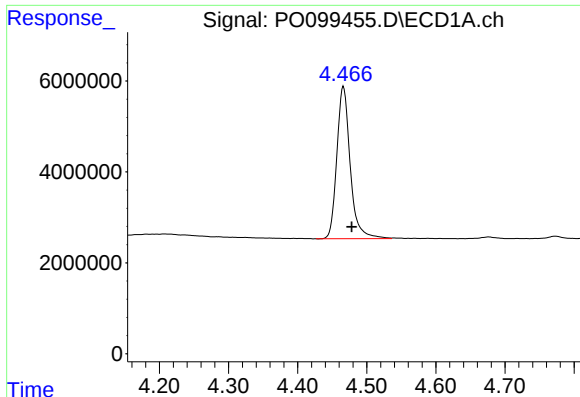


#1 Tetrachloro-m-xylene

R.T.: 4.466 min
Delta R.T.: -0.012 min
Response: 45059936
Conc: 22.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

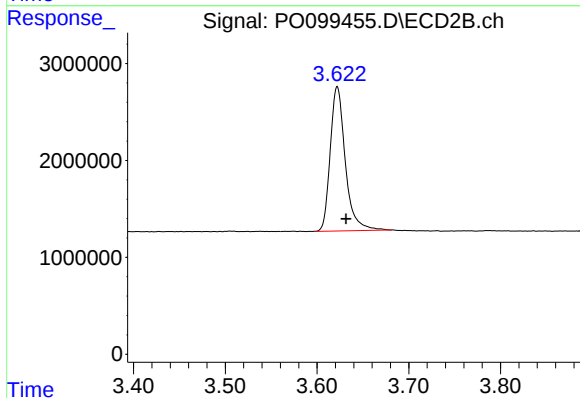


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.010 min
Response: 16971346
Conc: 23.58 ng/ml m

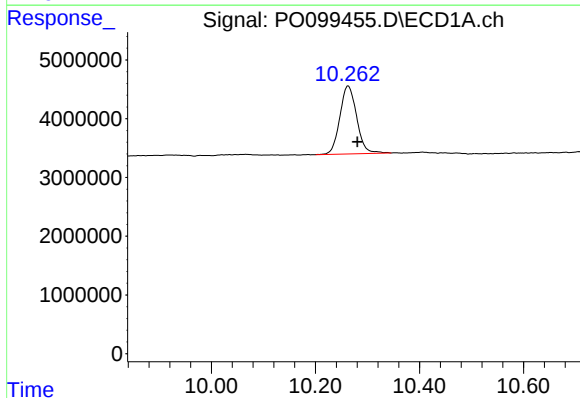

#2 Decachlorobiphenyl

R.T.: 10.263 min
Delta R.T.: -0.017 min
Response: 26015881
Conc: 22.96 ng/ml

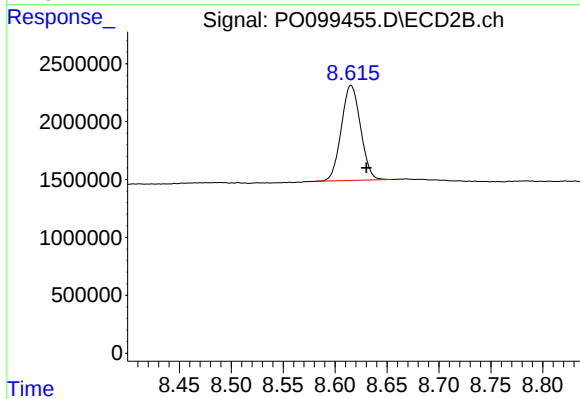

#2 Decachlorobiphenyl

R.T.: 8.615 min
Delta R.T.: -0.015 min
Response: 10601565
Conc: 19.76 ng/ml