

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110723\
 Data File : P0099469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 14:59
 Operator : YP/AJ
 Sample : 05258-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-A-03-B-03-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2023
 Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 22:08:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.468	3.624	45069142	17485948	22.809	24.297m
2) SA Decachlor...	10.264	8.615	26929141	11064514	23.771	20.622

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110723\
Data File : PO099469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 14:59
Operator : YP/AJ
Sample : 05258-03
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 22:08:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

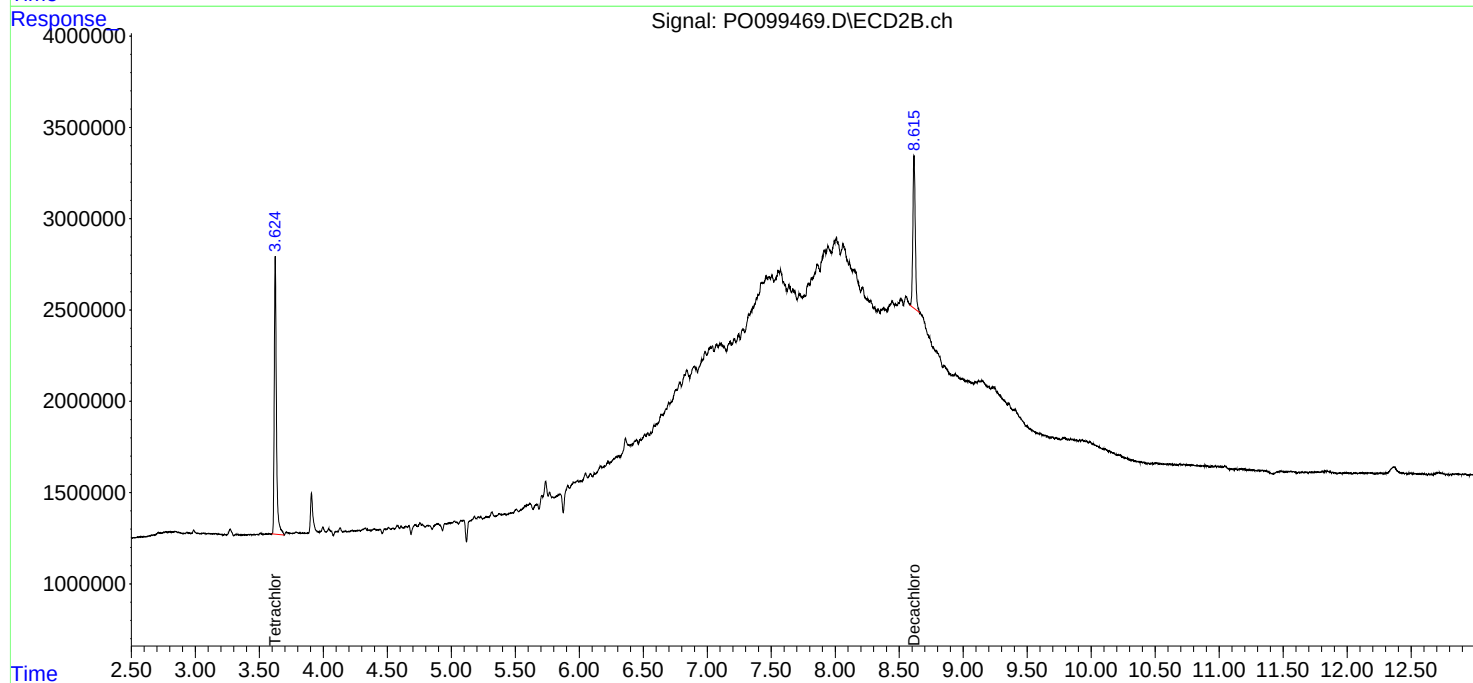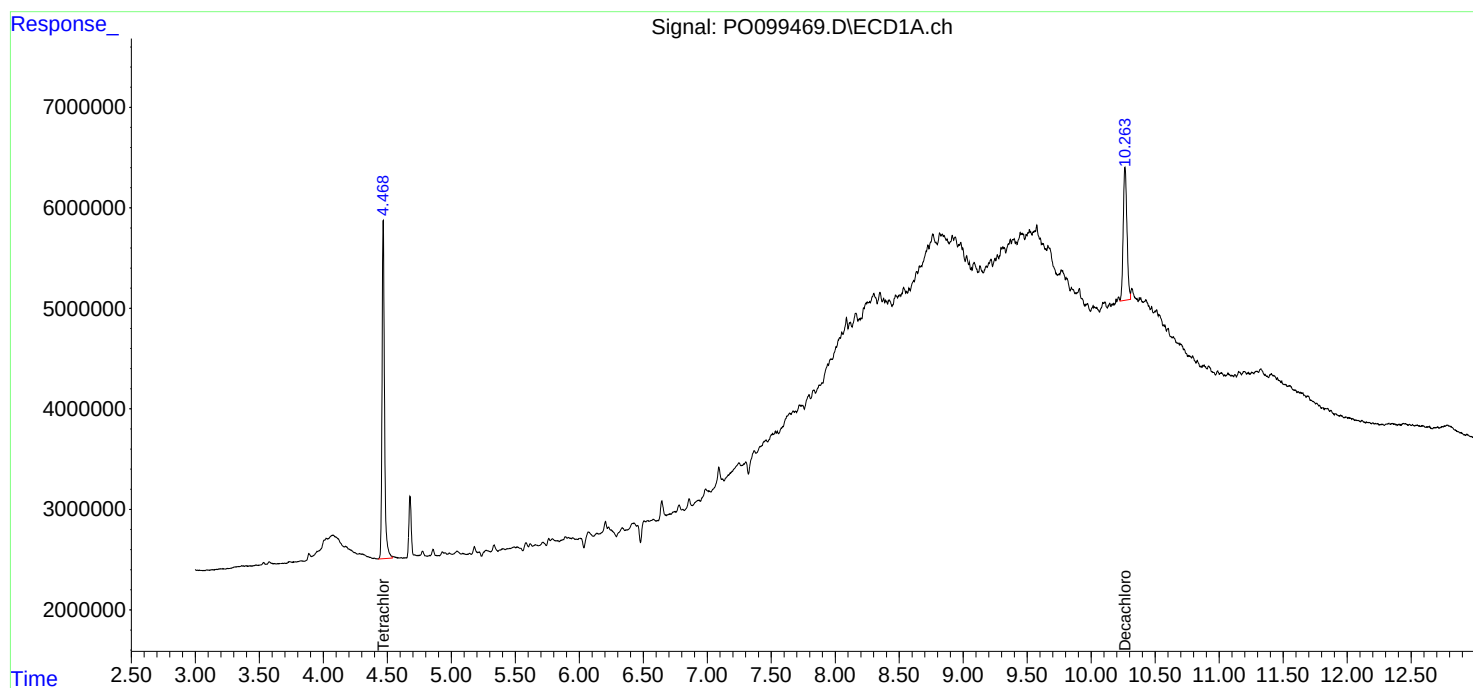

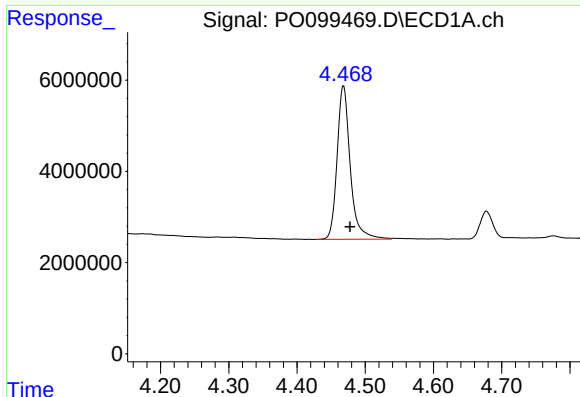


#1 Tetrachloro-m-xylene

R.T.: 4.468 min
Delta R.T.: -0.010 min
Response: 45069142
Conc: 22.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

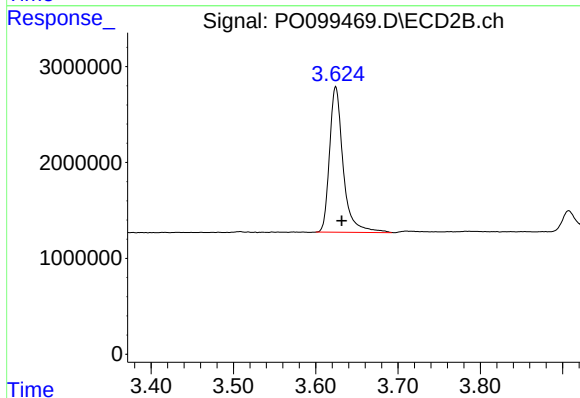


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.008 min
Response: 17485948
Conc: 24.30 ng/ml m

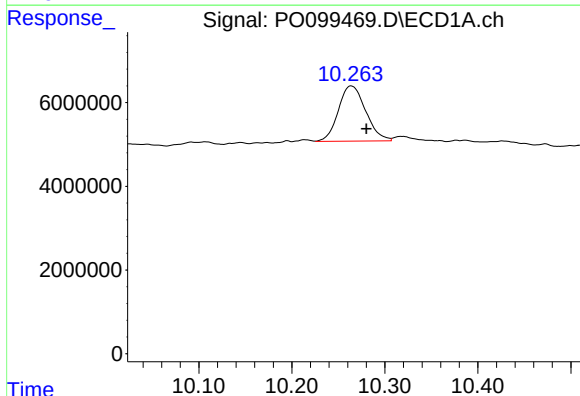

#2 Decachlorobiphenyl

R.T.: 10.264 min
Delta R.T.: -0.016 min
Response: 26929141
Conc: 23.77 ng/ml

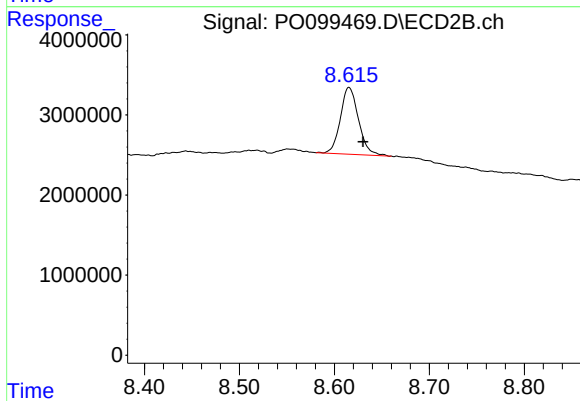

#2 Decachlorobiphenyl

R.T.: 8.615 min
Delta R.T.: -0.015 min
Response: 11064514
Conc: 20.62 ng/ml