

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110723\
 Data File : PO099472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 15:50
 Operator : YP/AJ
 Sample : 05258-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 06-A-06-B-06-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2023
 Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 22:09:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.468	3.623	46874890	17419399	23.723	24.204m
2) SA Decachlor...	10.261	8.614	26770583	10995346	23.631m	20.493

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110723\
Data File : PO099472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 15:50
Operator : YP/AJ
Sample : 05258-06
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
06-A-06-B-06-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 22:09:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

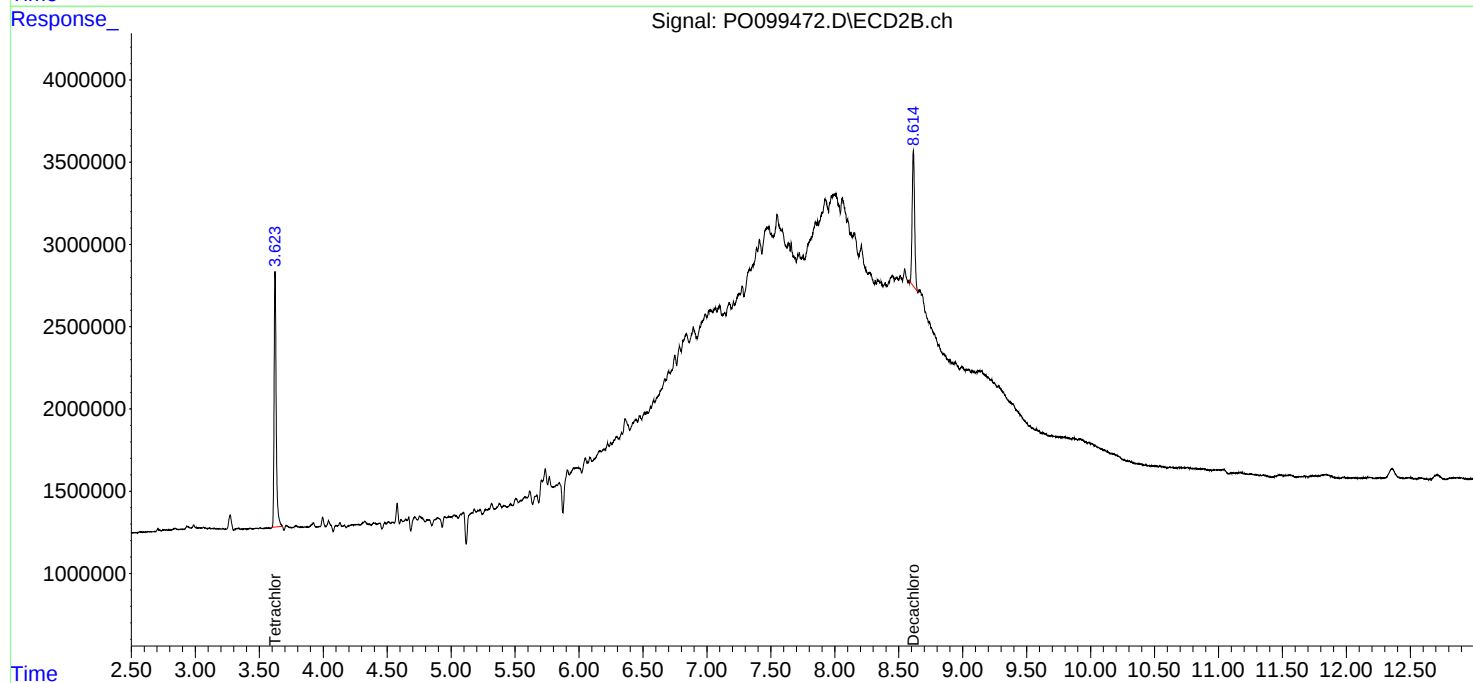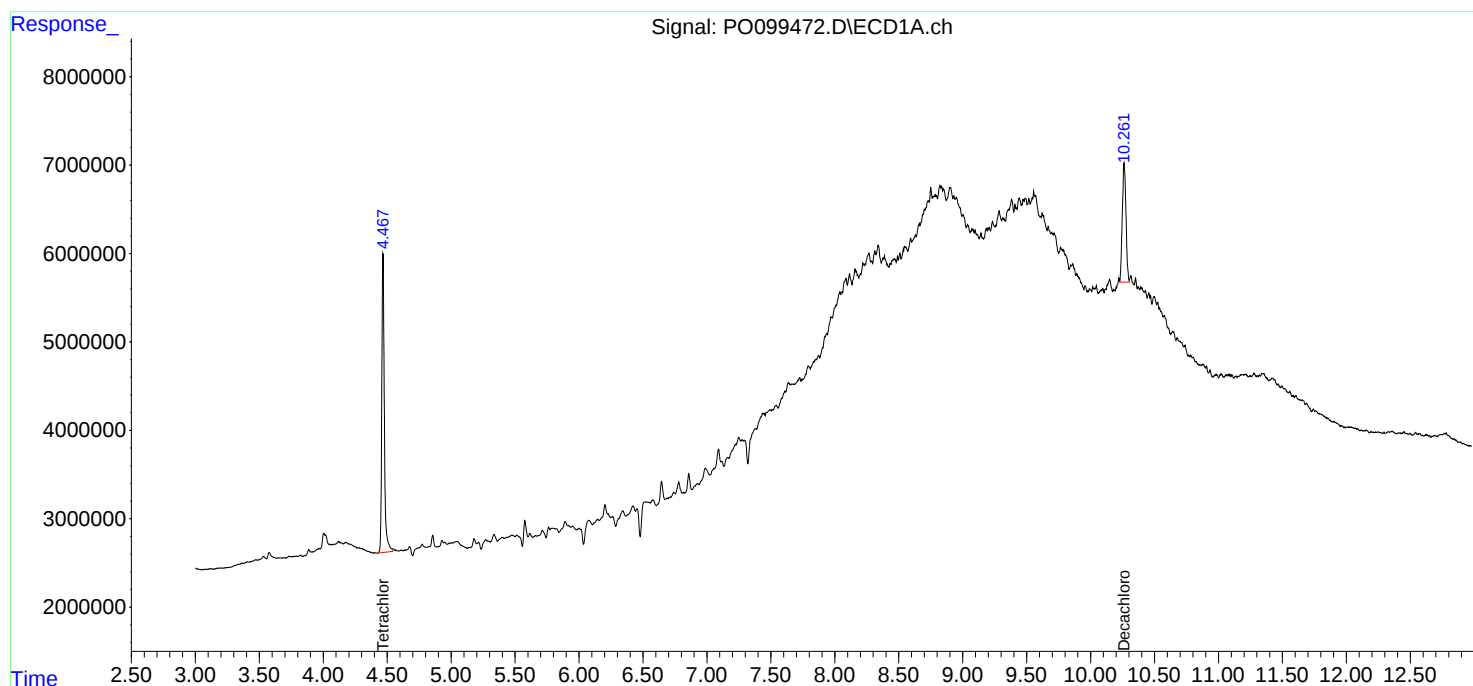

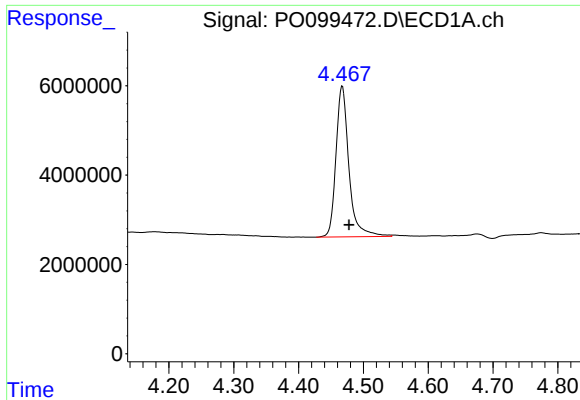


#1 Tetrachloro-m-xylene

R.T.: 4.468 min
Delta R.T.: -0.010 min
Response: 46874890
Conc: 23.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
06-A-06-B-06-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

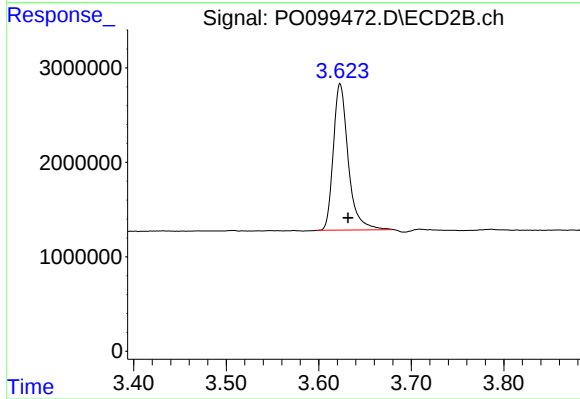


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.009 min
Response: 17419399
Conc: 24.20 ng/ml m

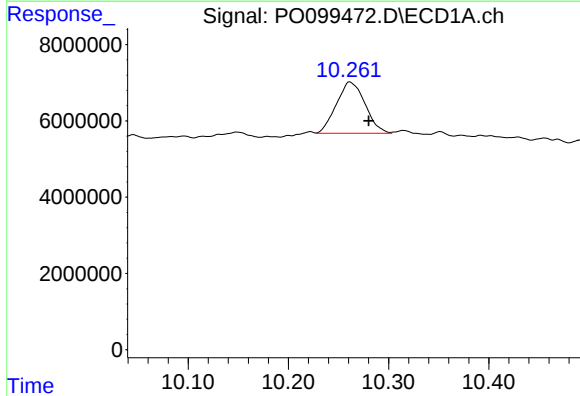

#2 Decachlorobiphenyl

R.T.: 10.261 min
Delta R.T.: -0.020 min
Response: 26770583
Conc: 23.63 ng/ml m

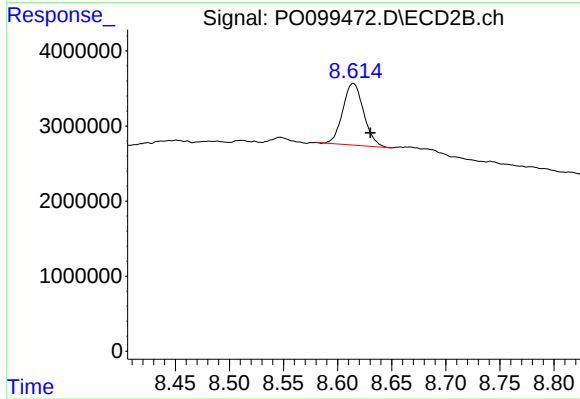

#2 Decachlorobiphenyl

R.T.: 8.614 min
Delta R.T.: -0.016 min
Response: 10995346
Conc: 20.49 ng/ml