

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110723\
 Data File : P0099483.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 18:56
 Operator : YP/AJ
 Sample : 05258-17
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 17-A-17-B-17-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2023
 Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 22:12:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.468	3.623	45412600	16812992	22.983	23.362m
2) SA Decachlor...	10.259	8.613	29403956	10260128	25.955	19.123 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110723\
Data File : P0099483.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 18:56
Operator : YP/AJ
Sample : 05258-17
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
17-A-17-B-17-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 22:12:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

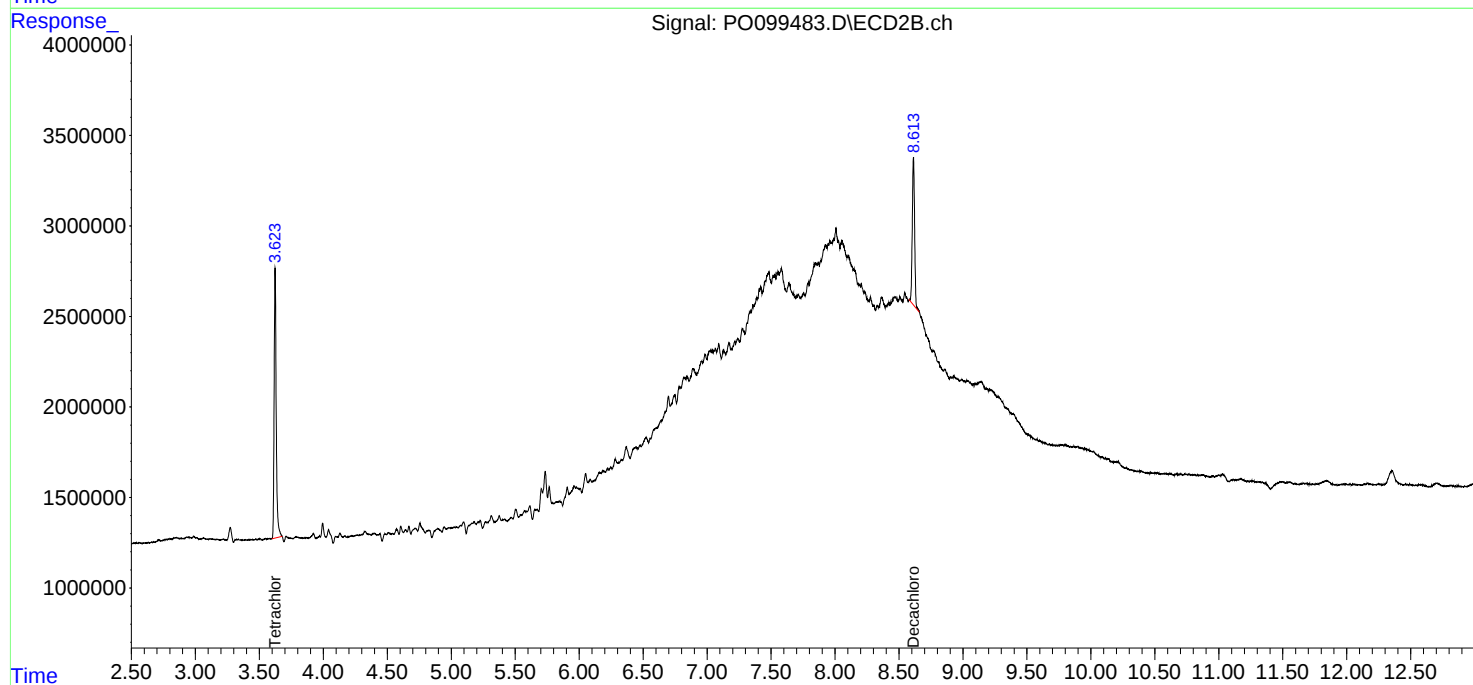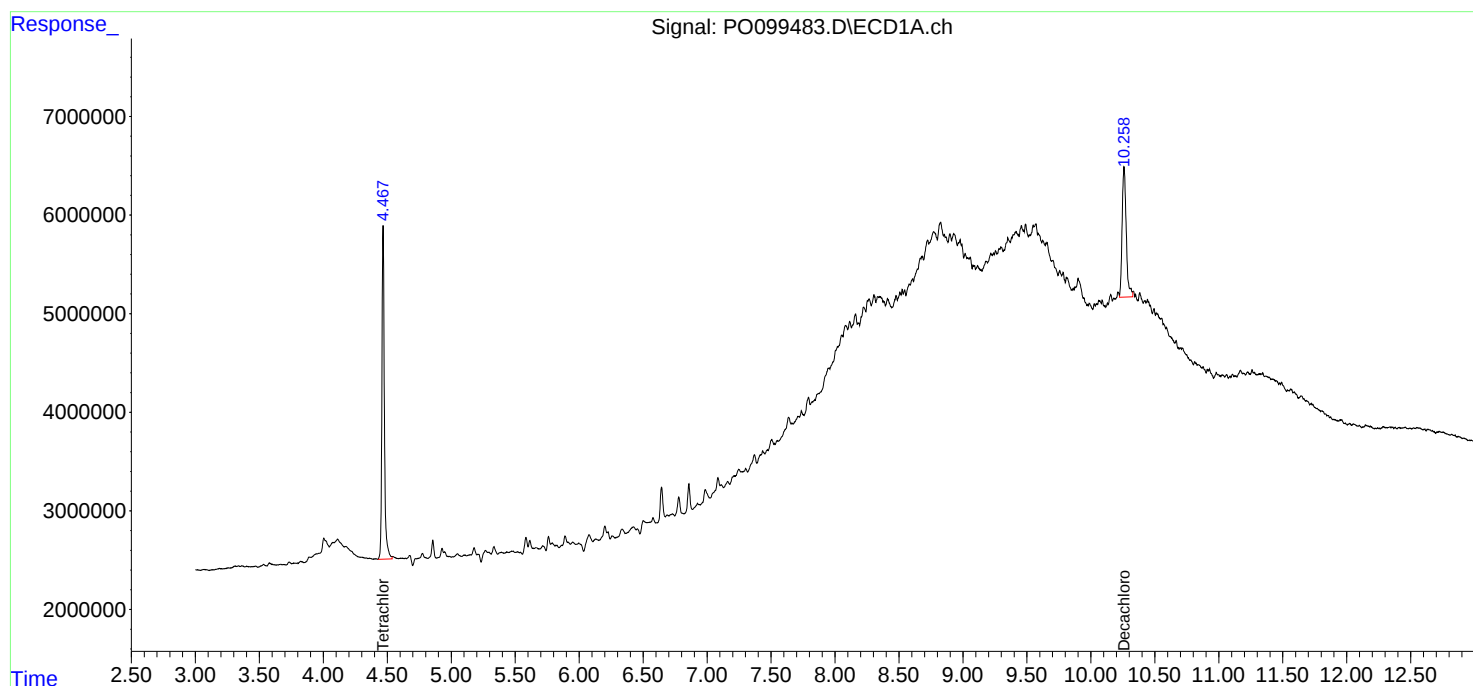

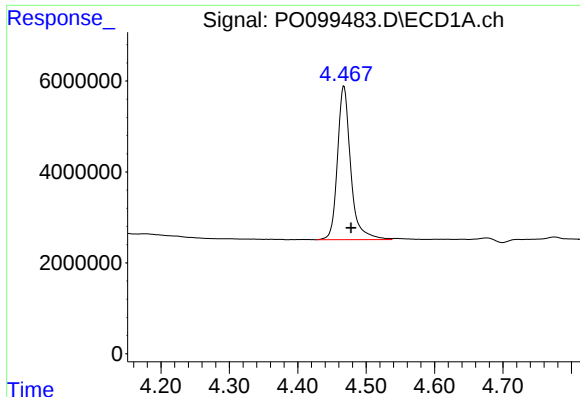


#1 Tetrachloro-m-xylene

R.T.: 4.468 min
Delta R.T.: -0.010 min
Response: 45412600
Conc: 22.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
17-A-17-B-17-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

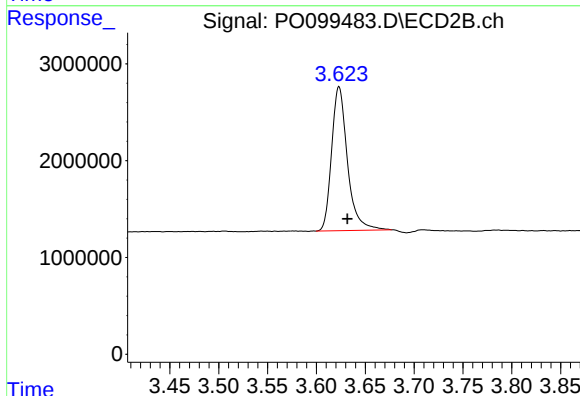


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: -0.009 min
Response: 16812992
Conc: 23.36 ng/ml m

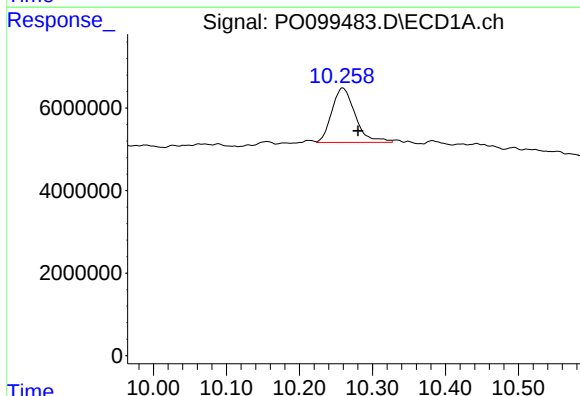

#2 Decachlorobiphenyl

R.T.: 10.259 min
Delta R.T.: -0.021 min
Response: 29403956
Conc: 25.96 ng/ml

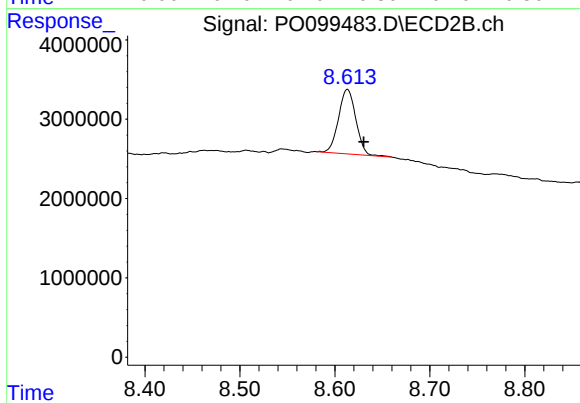

#2 Decachlorobiphenyl

R.T.: 8.613 min
Delta R.T.: -0.017 min
Response: 10260128
Conc: 19.12 ng/ml