

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO110723\  
 Data File : PO099494.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 07 Nov 2023 22:30  
 Operator : YP/AJ  
 Sample : 05258-24DL 400X  
 Misc :  
 ALS Vial : 44 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 24-A-24-B-24-CDL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 11/08/2023  
 Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 07 23:59:10 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO102523.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Oct 25 06:04:36 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| Target Compounds |    |           |       |       |          |          |          |          |
|------------------|----|-----------|-------|-------|----------|----------|----------|----------|
| 26)              | L6 | AR-1254-1 | 6.497 | 5.500 | 15753115 | 9711649  | 239.311  | 274.082  |
| 27)              | L6 | AR-1254-2 | 6.716 | 5.648 | 39677163 | 14992352 | 412.150  | 468.739  |
| 28)              | L6 | AR-1254-3 | 7.084 | 6.051 | 62638800 | 34493257 | 700.790  | 705.564  |
| 29)              | L6 | AR-1254-4 | 7.369 | 6.280 | 53299090 | 24728095 | 972.904m | 943.575  |
| 30)              | L6 | AR-1254-5 | 7.790 | 6.697 | 82082755 | 50846201 | 1219.024 | 1206.179 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO110723\  
Data File : PO099494.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 07 Nov 2023 22:30  
Operator : YP/AJ  
Sample : 05258-24DL 400X  
Misc :  
ALS Vial : 44 Sample Multiplier: 1



Instrument :  
ECD\_O  
ClientSampleId :  
24-A-24-B-24-CDL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/08/2023  
Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 07 23:59:10 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO102523.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Oct 25 06:04:36 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

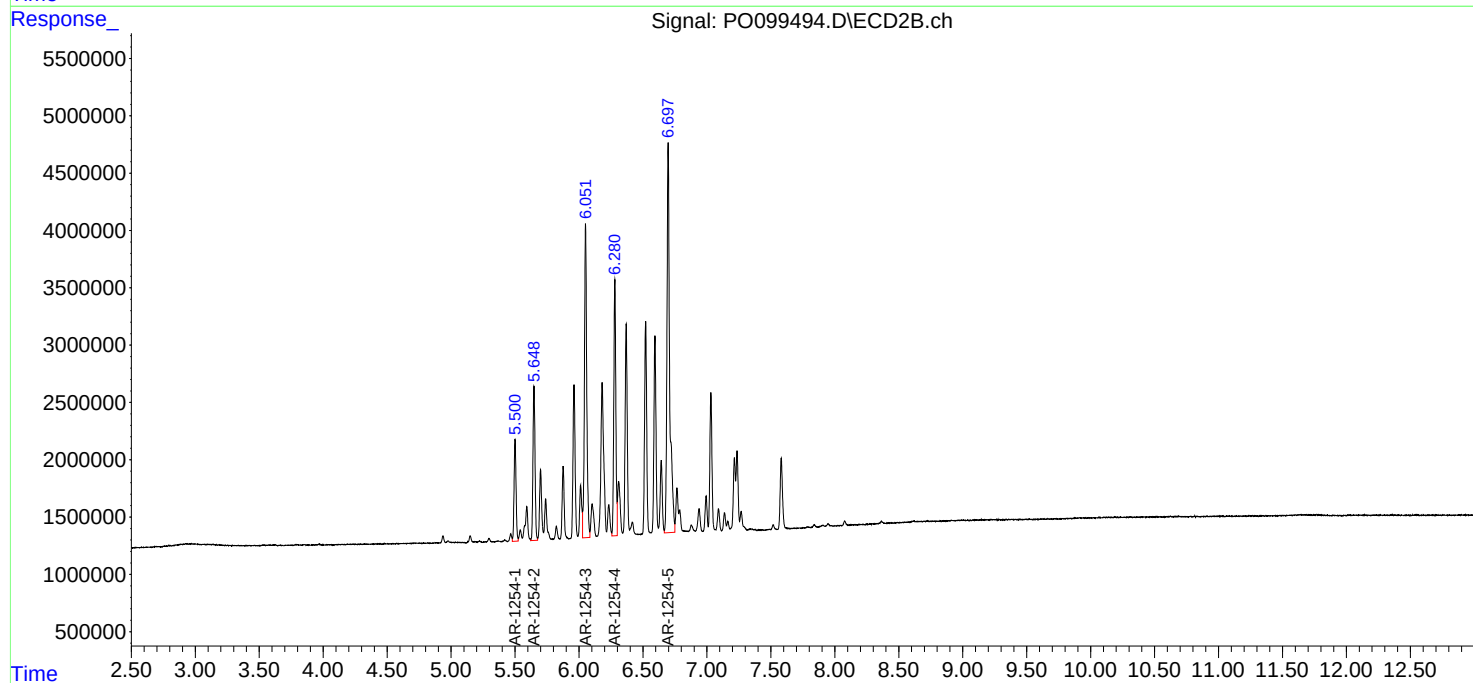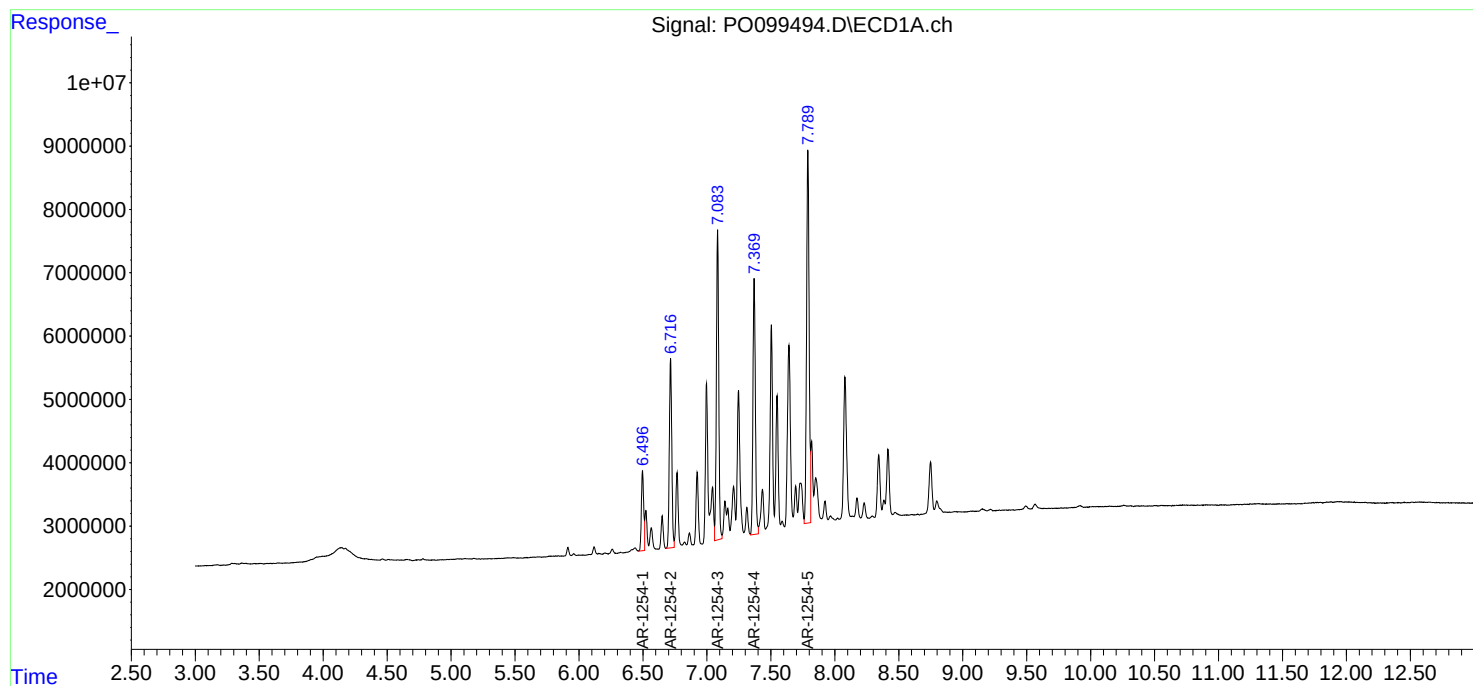

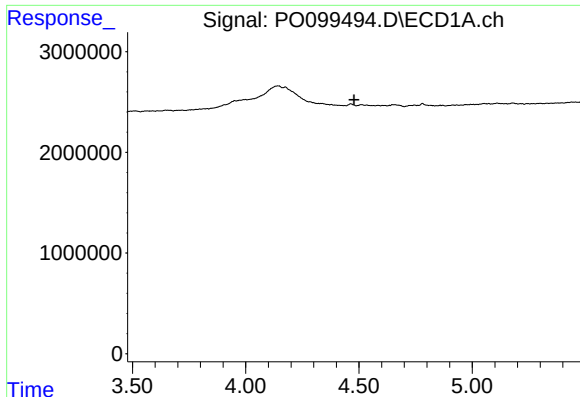

# #1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 4.478 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_O  
ClientSampleId :  
24-A-24-B-24-CDL

## Manual Integrations APPROVED

Reviewed By :Yogesh Patel 11/08/2023  
Supervised By :Ankita Jodhani 11/08/2023

# #1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 3.632 min  
Response: 0  
Conc: N.D.

# #2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 10.280 min  
Response: 0  
Conc: N.D.

# #2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.630 min  
Response: 0  
Conc: N.D.

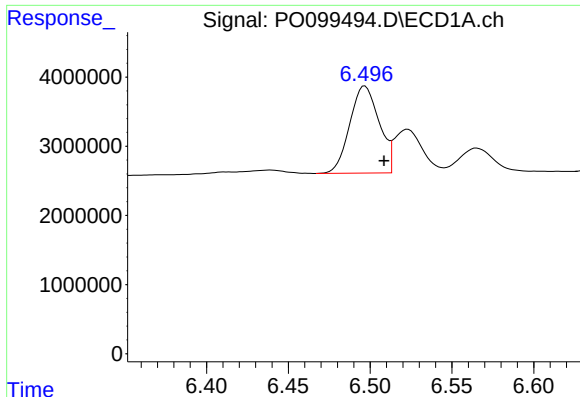


#26 AR-1254-1

R.T.: 6.497 min  
Delta R.T.: -0.012 min  
Response: 15753115  
Conc: 239.31 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
24-A-24-B-24-CDL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/08/2023  
Supervised By :Ankita Jodhani 11/08/2023

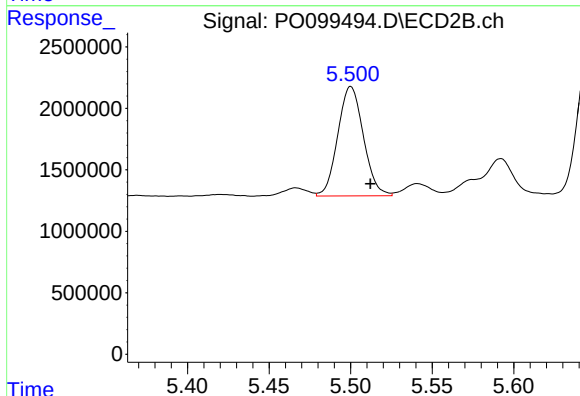


#26 AR-1254-1

R.T.: 5.500 min  
Delta R.T.: -0.012 min  
Response: 9711649  
Conc: 274.08 ng/ml

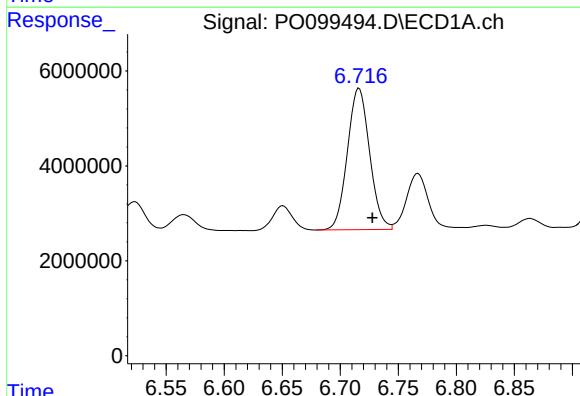


#27 AR-1254-2

R.T.: 6.716 min  
Delta R.T.: -0.011 min  
Response: 39677163  
Conc: 412.15 ng/ml

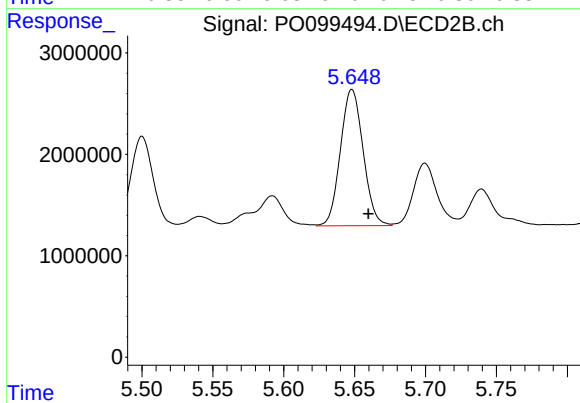

#27 AR-1254-2

R.T.: 5.648 min  
Delta R.T.: -0.011 min  
Response: 14992352  
Conc: 468.74 ng/ml

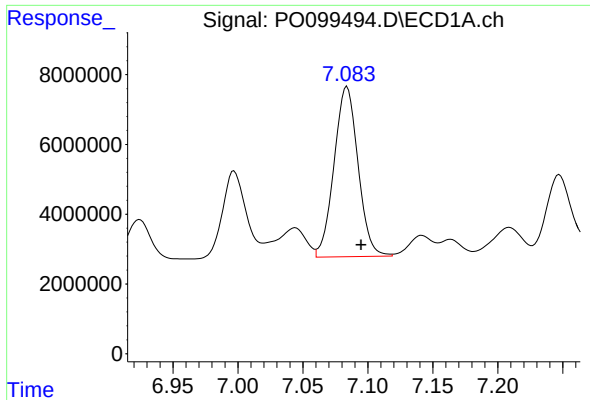


#28 AR-1254-3

R.T.: 7.084 min  
Delta R.T.: -0.011 min  
Response: 62638800  
Conc: 700.79 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
24-A-24-B-24-CDL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/08/2023  
Supervised By :Ankita Jodhani 11/08/2023

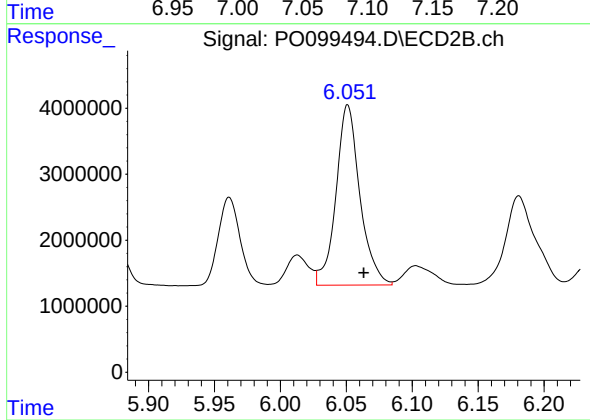


#28 AR-1254-3

R.T.: 6.051 min  
Delta R.T.: -0.012 min  
Response: 34493257  
Conc: 705.56 ng/ml

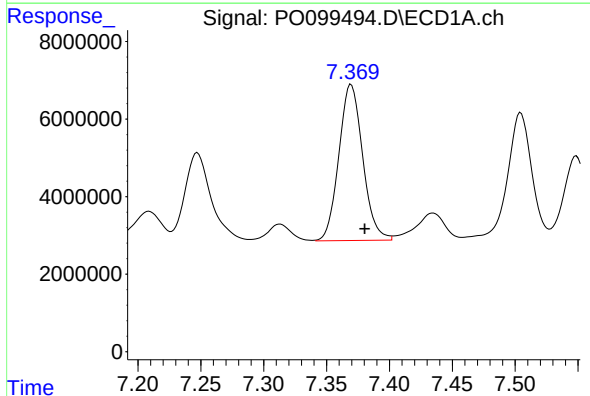


#29 AR-1254-4

R.T.: 7.369 min  
Delta R.T.: -0.011 min  
Response: 53299090  
Conc: 972.90 ng/ml m

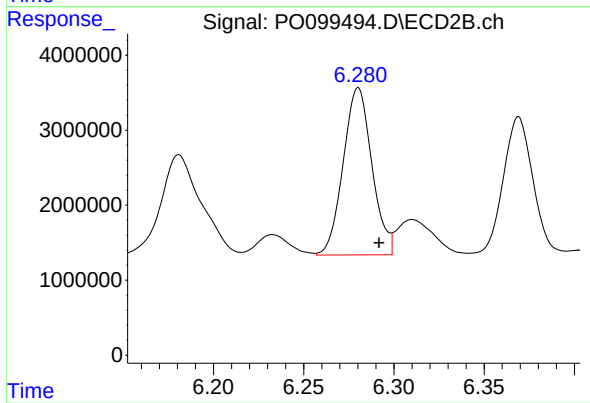

#29 AR-1254-4

R.T.: 6.280 min  
Delta R.T.: -0.012 min  
Response: 24728095  
Conc: 943.57 ng/ml

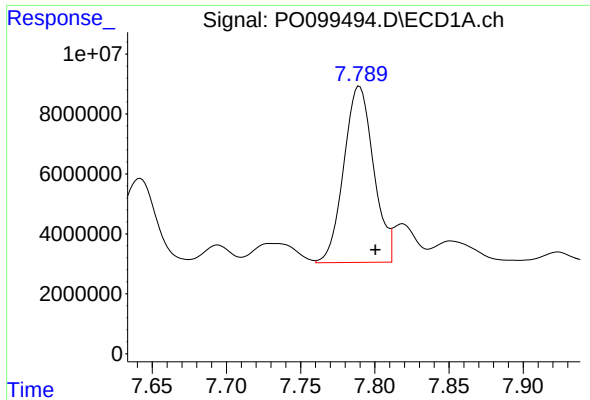


#30 AR-1254-5

R.T.: 7.790 min  
Delta R.T.: -0.011 min  
Response: 82082755  
Conc: 1219.02 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
24-A-24-B-24-CDL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/08/2023  
Supervised By :Ankita Jodhani 11/08/2023

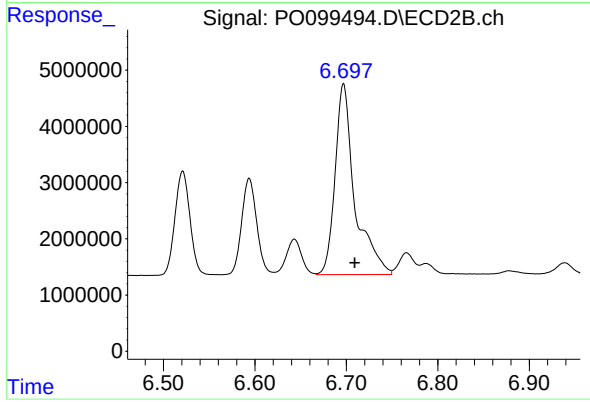

#30 AR-1254-5

R.T.: 6.697 min  
Delta R.T.: -0.012 min  
Response: 50846201  
Conc: 1206.18 ng/ml