

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO110723\
 Data File : PO099496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2023 23:04
 Operator : YP/AJ
 Sample : 05258-26DL 200X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 26-A-26-B-26-CDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2023
 Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 23:59:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
2) SA Decachlor...	10.259	8.611	5439256	2328684	4.801m	4.340
Target Compounds						
26) L6 AR-1254-1	6.497	5.501	21015205	12637681	319.249	356.661
27) L6 AR-1254-2	6.716	5.649	49770804	18531591	516.999	579.395
28) L6 AR-1254-3	7.083	6.052	74917773	41718415	838.165	853.356
29) L6 AR-1254-4	7.369	6.280	61333300	28609394	1119.558m	1091.677
30) L6 AR-1254-5	7.790	6.697	95208975	59709789	1413.963	1416.441

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110723\
Data File : PO099496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2023 23:04
Operator : YP/AJ
Sample : 05258-26DL 200X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
26-A-26-B-26-CDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 23:59:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

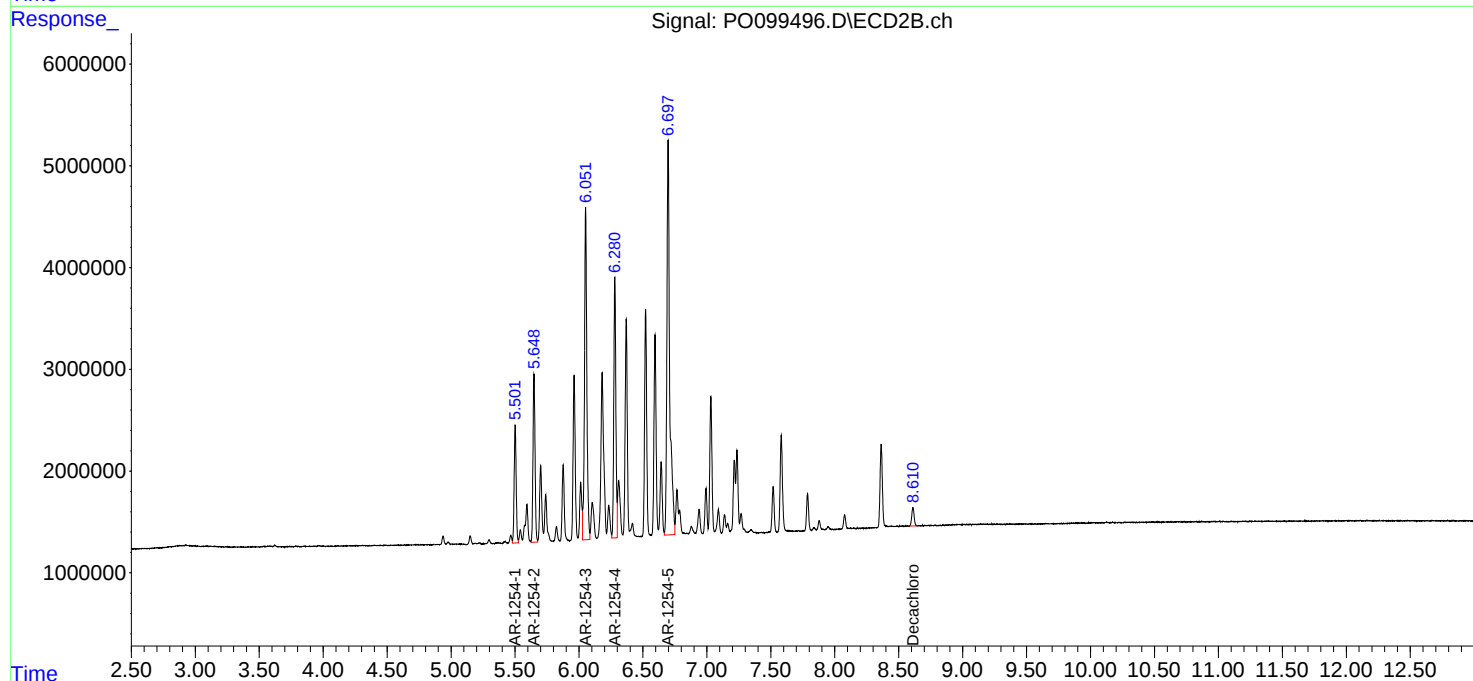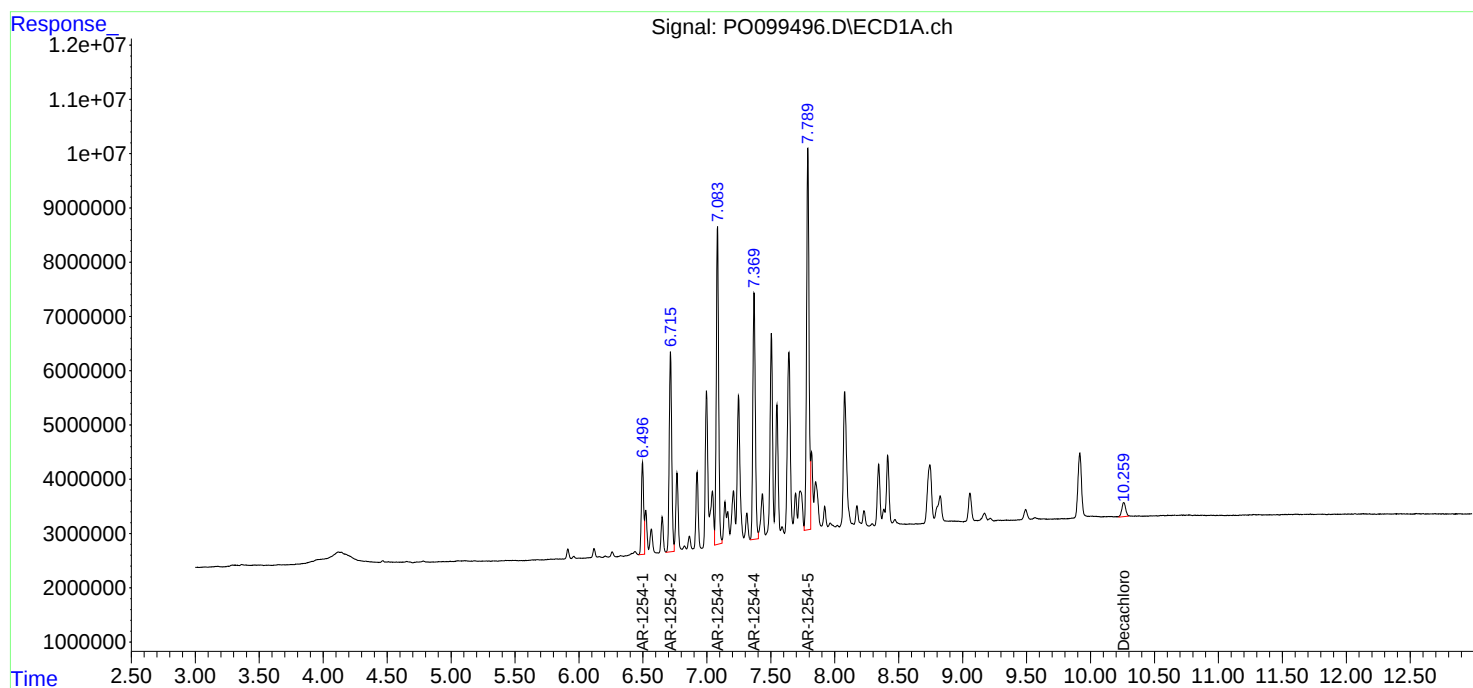

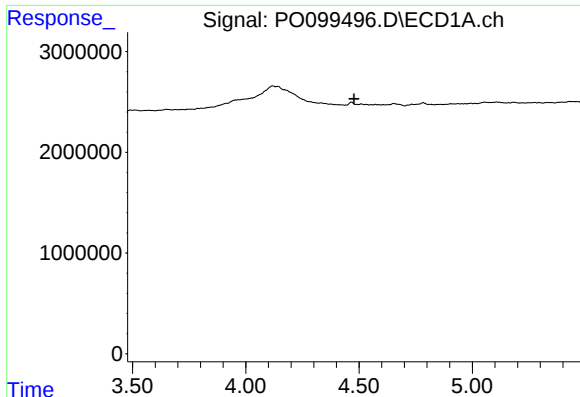

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.478 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
26-A-26-B-26-CDL

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.632 min
Response: 0
Conc: N.D.

#2 Decachlorobiphenyl

R.T.: 10.259 min
Delta R.T.: -0.022 min
Response: 5439256
Conc: 4.80 ng/ml m

#2 Decachlorobiphenyl

R.T.: 8.611 min
Delta R.T.: -0.019 min
Response: 2328684
Conc: 4.34 ng/ml

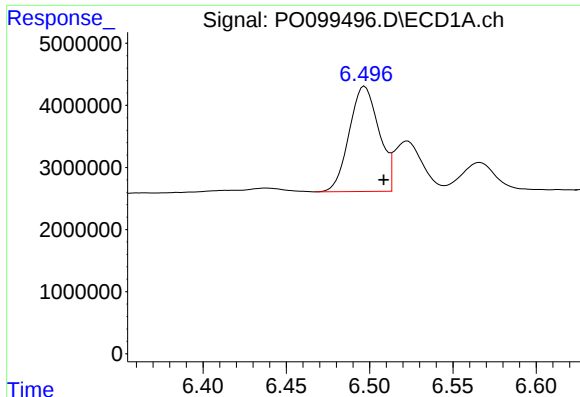


#26 AR-1254-1

R.T.: 6.497 min
Delta R.T.: -0.011 min
Response: 21015205
Conc: 319.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
26-A-26-B-26-CDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

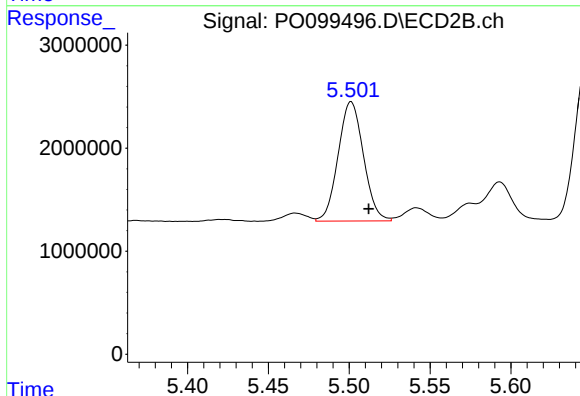


#26 AR-1254-1

R.T.: 5.501 min
Delta R.T.: -0.011 min
Response: 12637681
Conc: 356.66 ng/ml

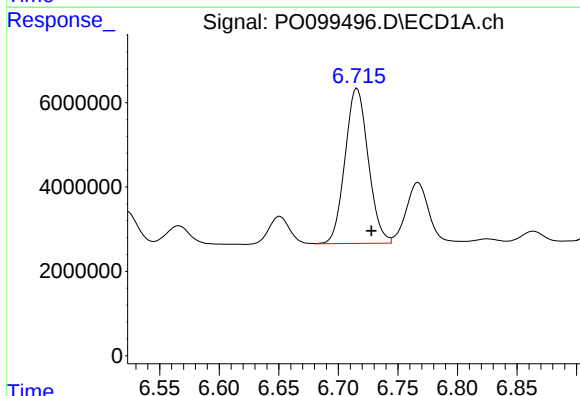


#27 AR-1254-2

R.T.: 6.716 min
Delta R.T.: -0.012 min
Response: 49770804
Conc: 517.00 ng/ml

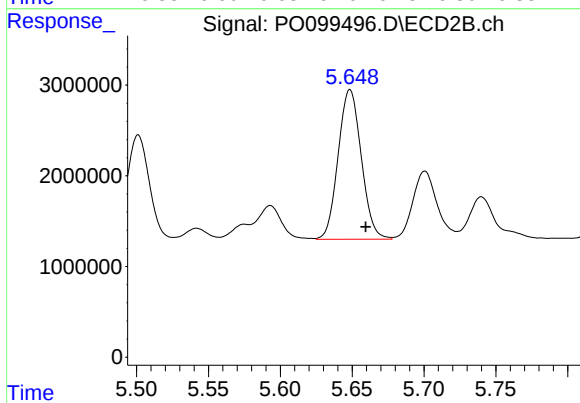

#27 AR-1254-2

R.T.: 5.649 min
Delta R.T.: -0.011 min
Response: 18531591
Conc: 579.39 ng/ml

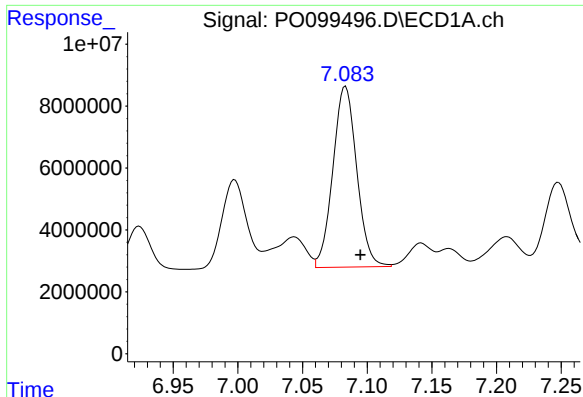


#28 AR-1254-3

R.T.: 7.083 min
Delta R.T.: -0.011 min
Response: 74917773
Conc: 838.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
26-A-26-B-26-CDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

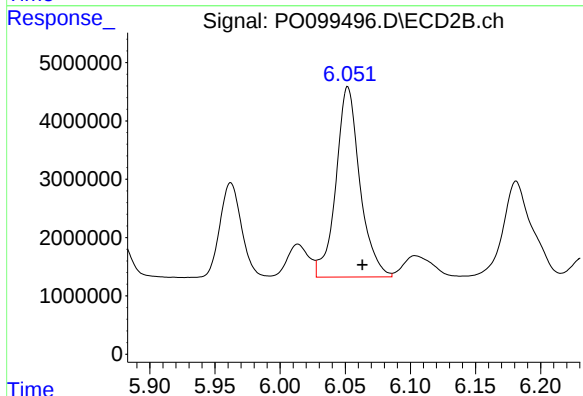


#28 AR-1254-3

R.T.: 6.052 min
Delta R.T.: -0.011 min
Response: 41718415
Conc: 853.36 ng/ml

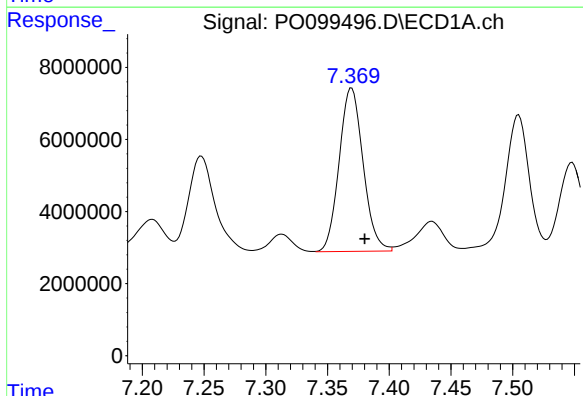


#29 AR-1254-4

R.T.: 7.369 min
Delta R.T.: -0.011 min
Response: 61333300
Conc: 1119.56 ng/ml m

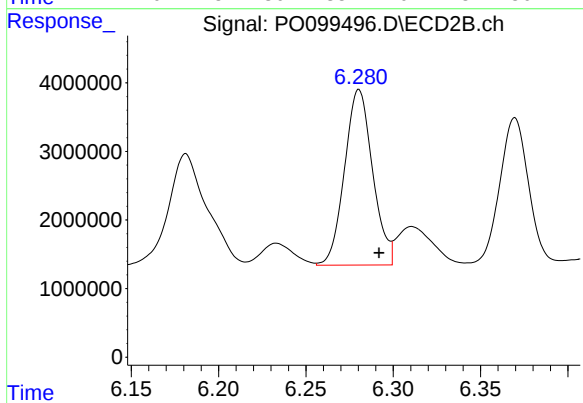

#29 AR-1254-4

R.T.: 6.280 min
Delta R.T.: -0.011 min
Response: 28609394
Conc: 1091.68 ng/ml

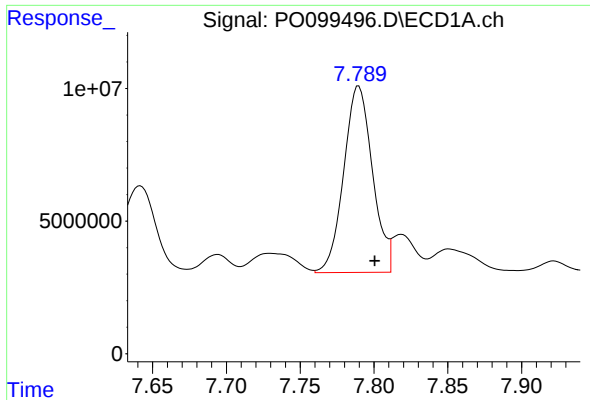


#30 AR-1254-5

R.T.: 7.790 min
Delta R.T.: -0.011 min
Response: 95208975
Conc: 1413.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
26-A-26-B-26-CDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

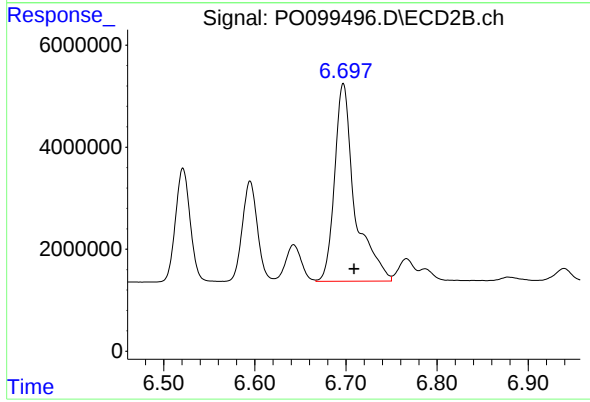

#30 AR-1254-5

R.T.: 6.697 min
Delta R.T.: -0.012 min
Response: 59709789
Conc: 1416.44 ng/ml