

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110723\
 Data File : PO099513.D
 Signal(s) : ECD2B.ch
 Acq On : 08 Nov 23 04:20 am
 Operator : YP/AJ
 Sample : 05247-19
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 27A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2023
 Supervised By :Ankita Jodhani 11/08/2023

Integration File: autoint1.e
 Quant Time: Nov 08 04:55:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.465	3.621	37048904	13878897	18.750	19.285m
2) SA Decachlor...	10.260	8.610	18489016	7966726	16.321	14.849

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110723\
Data File : PO099513.D
Signal(s) : ECD2B.ch
Acq On : 08 Nov 23 04:20 am
Operator : YP/AJ
Sample : 05247-19
Misc :
ALS Vial : 63 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
27A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

Integration File: autoint1.e
Quant Time: Nov 08 04:55:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

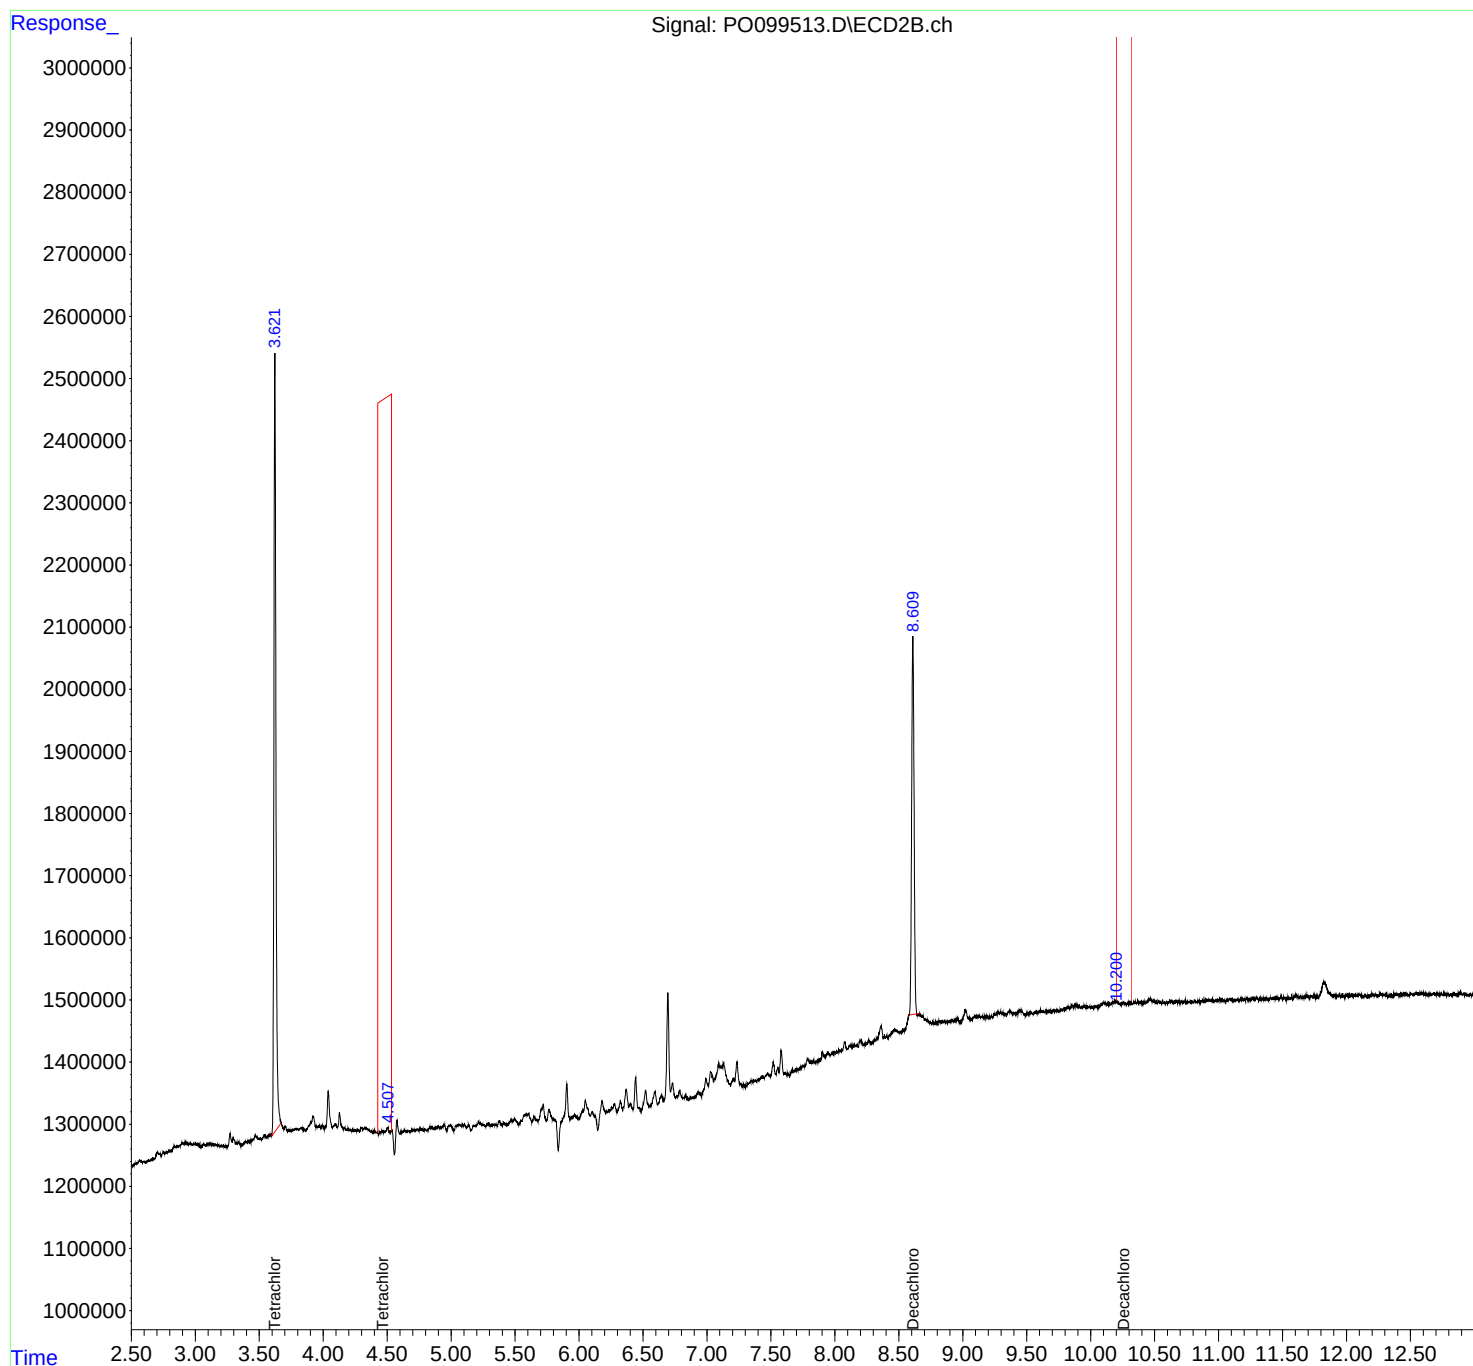

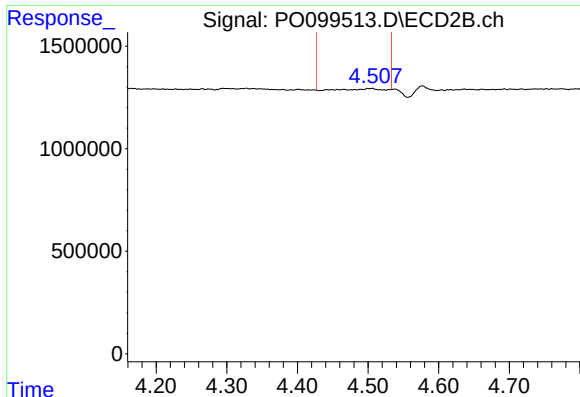


#1 Tetrachloro-m-xylene

R.T.: 4.465 min
Delta R.T.: -0.013 min
Response: 37048904
Conc: 18.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
27A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :Ankita Jodhani 11/08/2023

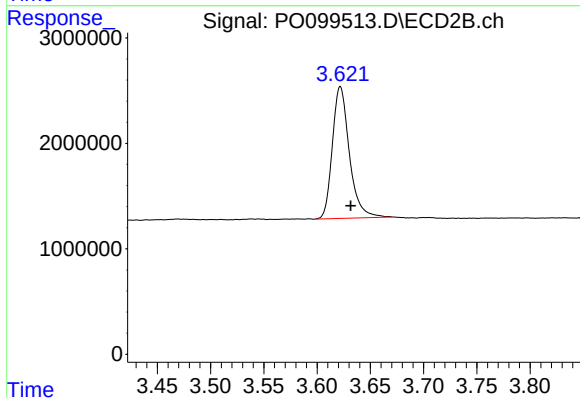


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.010 min
Response: 13878897
Conc: 19.28 ng/ml m

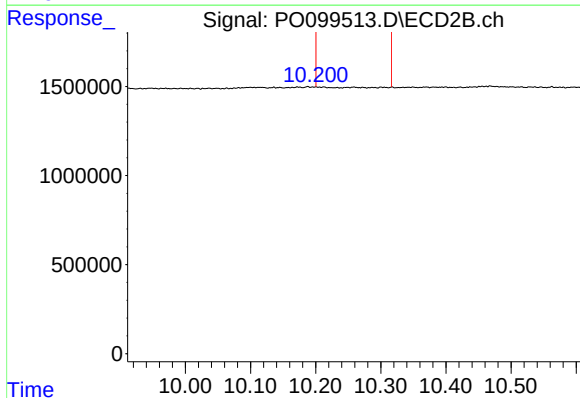

#2 Decachlorobiphenyl

R.T.: 10.260 min
Delta R.T.: -0.021 min
Response: 18489016
Conc: 16.32 ng/ml

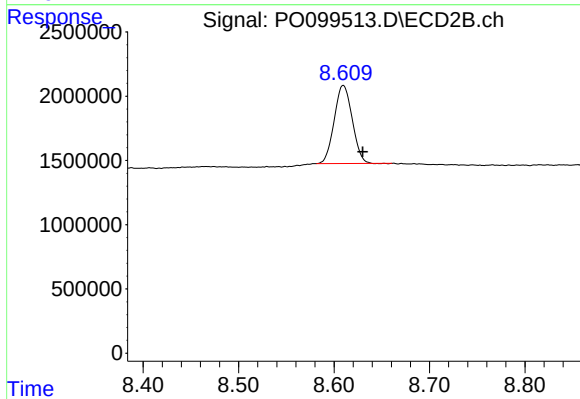

#2 Decachlorobiphenyl

R.T.: 8.610 min
Delta R.T.: -0.020 min
Response: 7966726
Conc: 14.85 ng/ml