

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110724\
 Data File : P0107795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 19:49
 Operator : YP/AJ
 Sample : P4739-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BP-B2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2024
 Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 00:58:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.642	170.0E6	51277913	18.657m	15.932m
2) SA Decachlor...	10.076	8.636	36499345	39437859	14.877	14.385m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110724\
Data File : PO107795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 19:49
Operator : YP/AJ
Sample : P4739-09
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BP-B2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 00:58:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

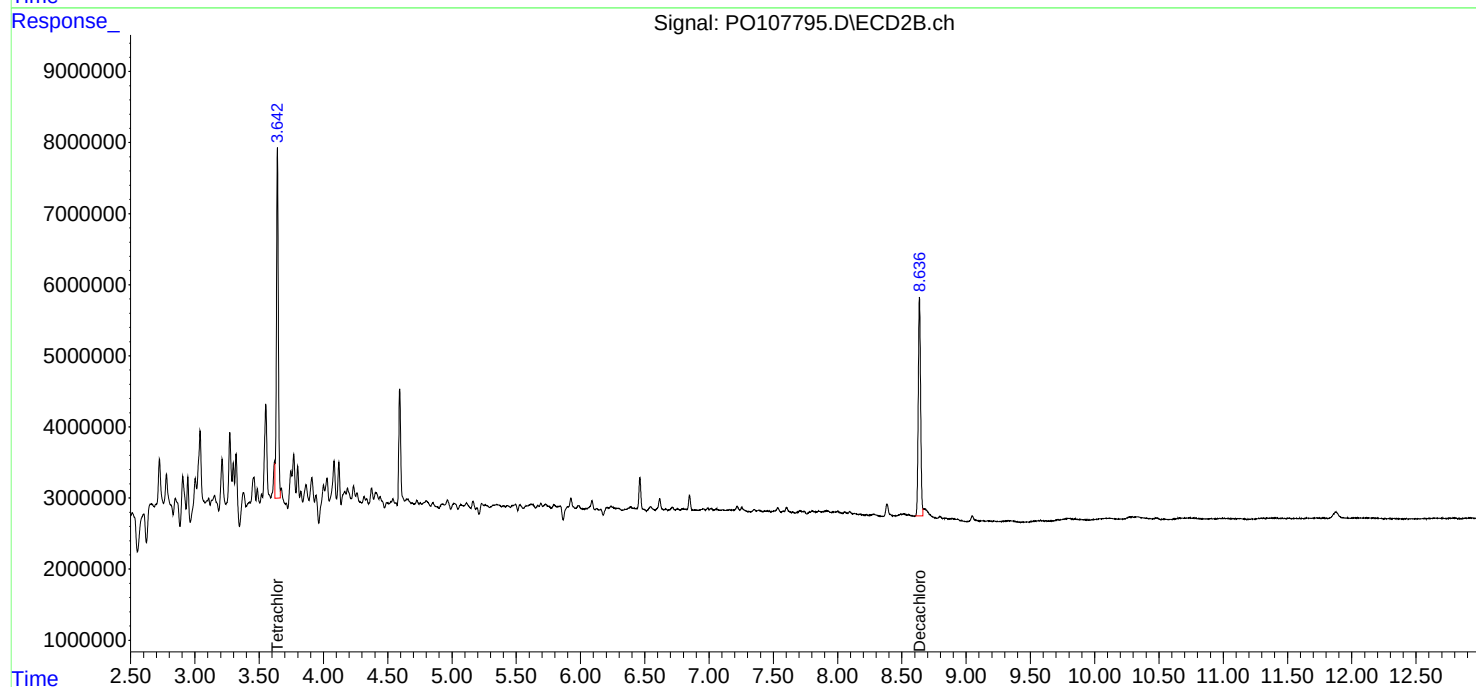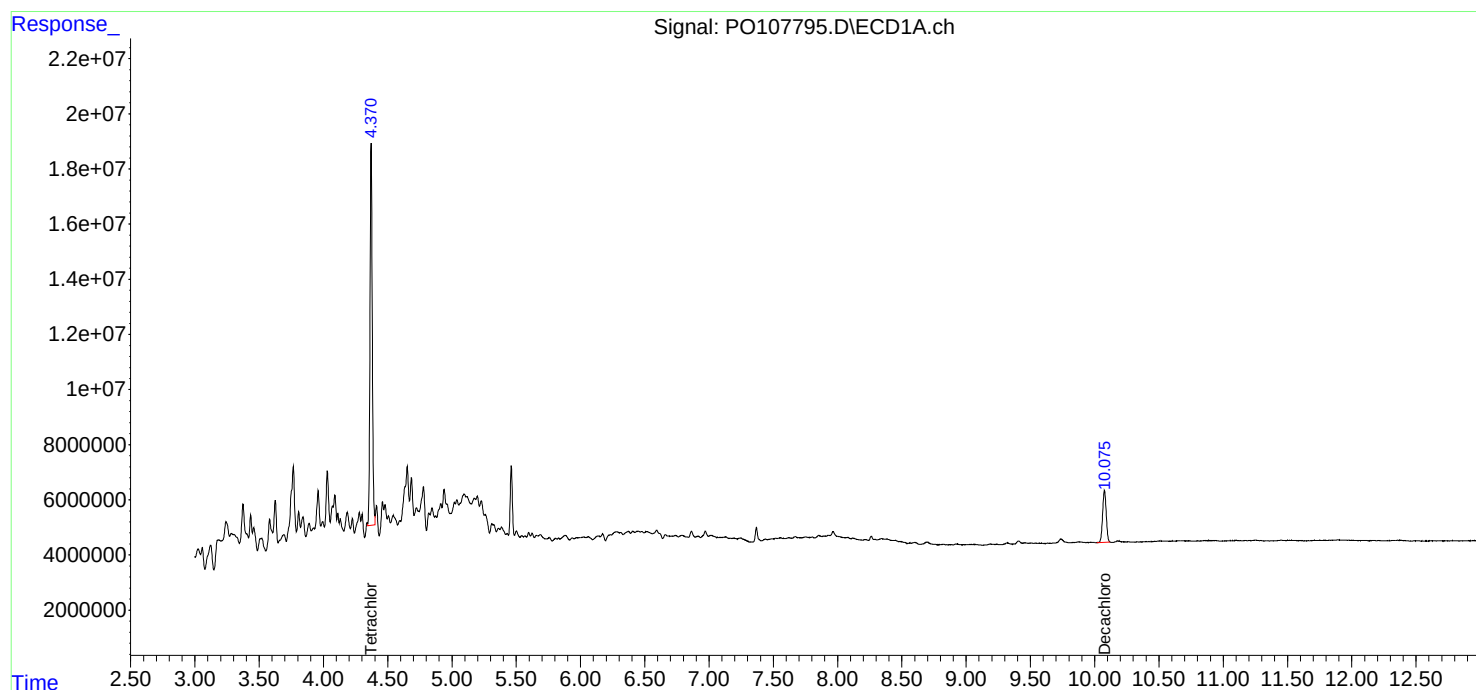

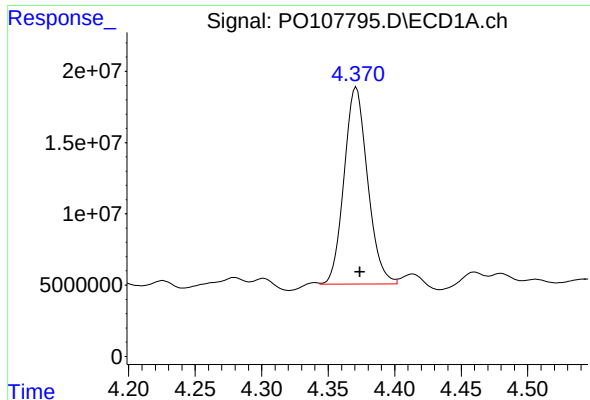


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: -0.004 min
Response: 170042313
Conc: 18.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
BP-B2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :Ankita Jodhani 11/08/2024

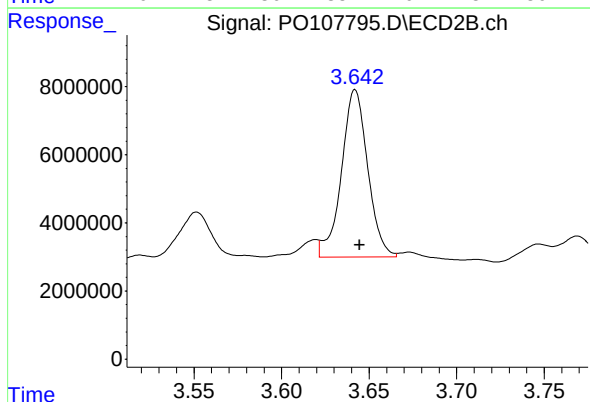


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.003 min
Response: 51277913
Conc: 15.93 ng/ml

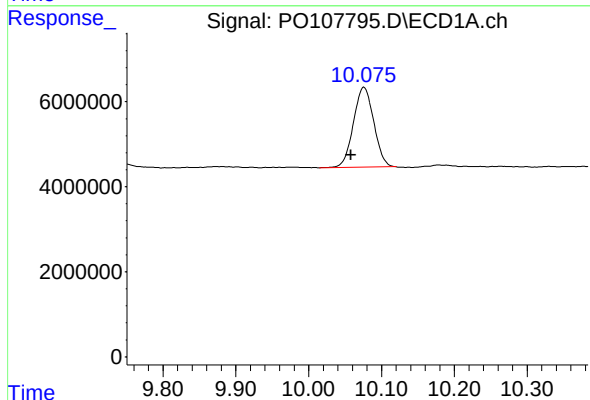

#2 Decachlorobiphenyl

R.T.: 10.076 min
Delta R.T.: 0.018 min
Response: 36499345
Conc: 14.88 ng/ml

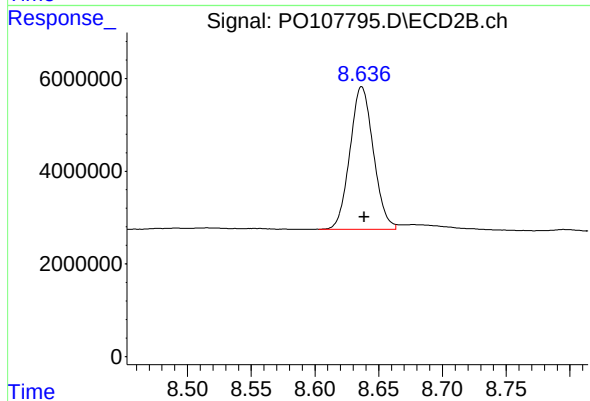

#2 Decachlorobiphenyl

R.T.: 8.636 min
Delta R.T.: -0.002 min
Response: 39437859
Conc: 14.38 ng/ml