

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110724\
 Data File : P0107796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2024 20:05
 Operator : YP/AJ
 Sample : P4739-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-11

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2024
 Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 00:59:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.642	148.4E6	55444121	16.287m	17.227
2) SA Decachlor...	10.079	8.637	35319431	35170984	14.396	12.829

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110724\
Data File : PO107796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2024 20:05
Operator : YP/AJ
Sample : P4739-13
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :Ankita Jodhani 11/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 00:59:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

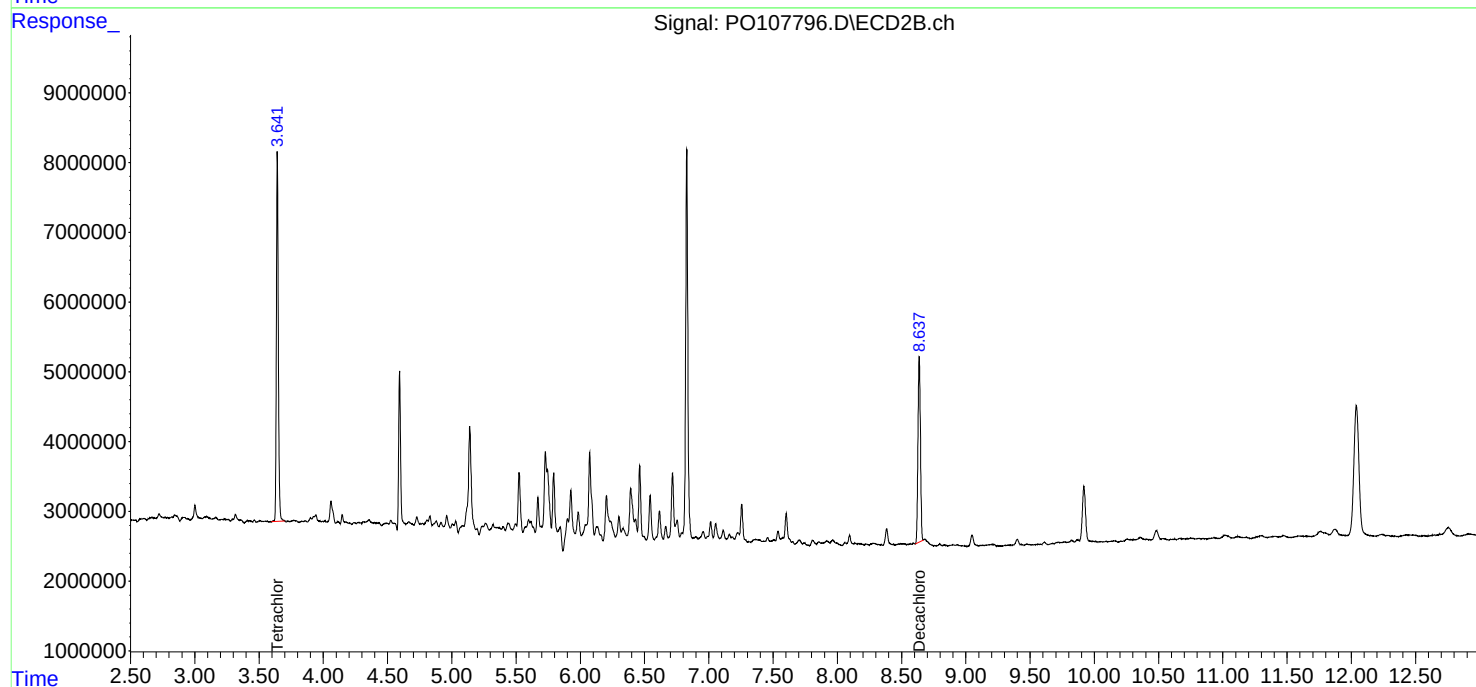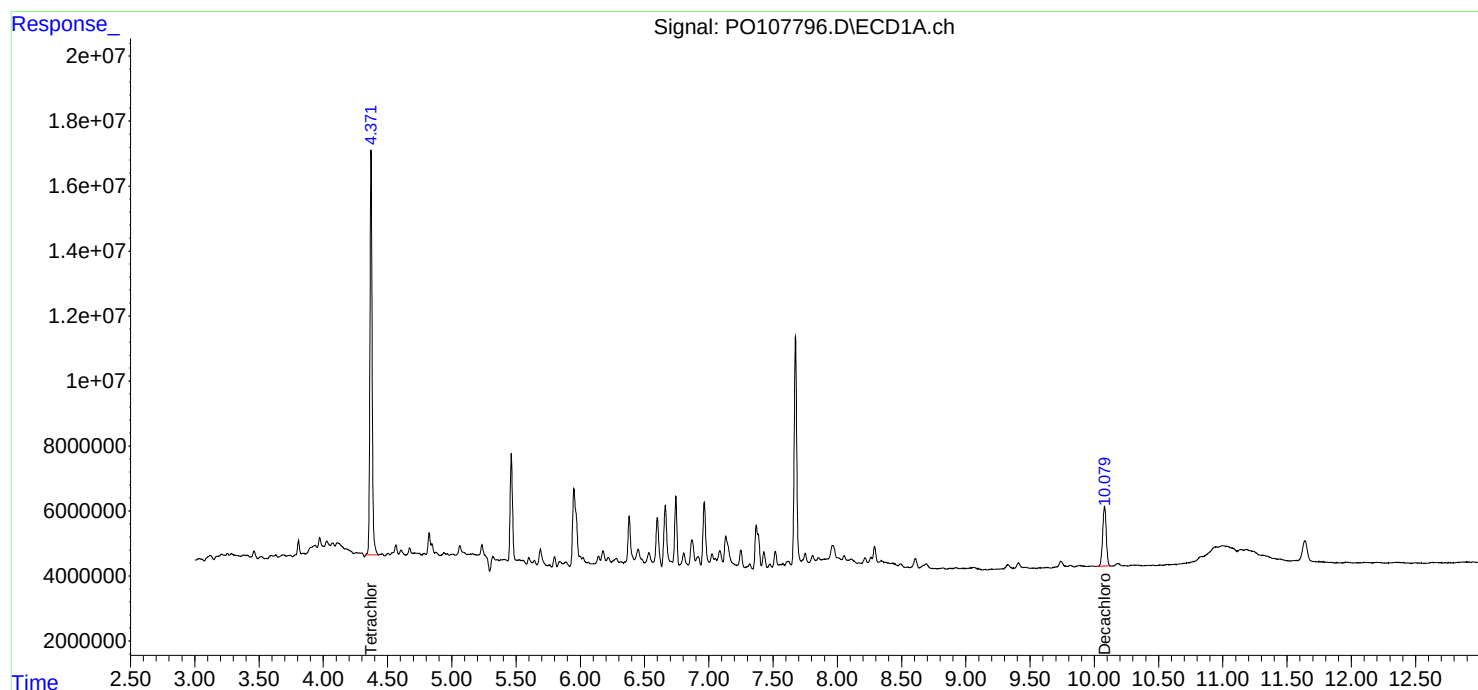

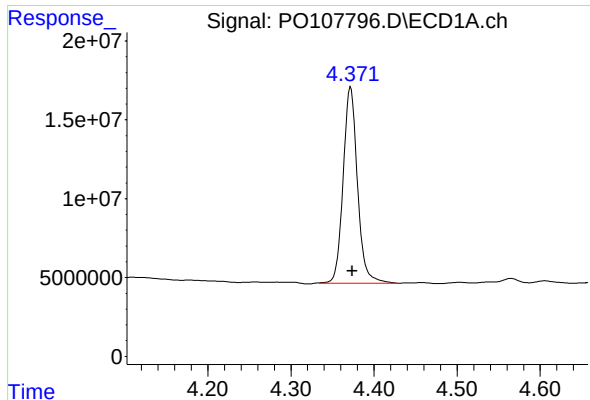


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 148433852
Conc: 16.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :Ankita Jodhani 11/08/2024

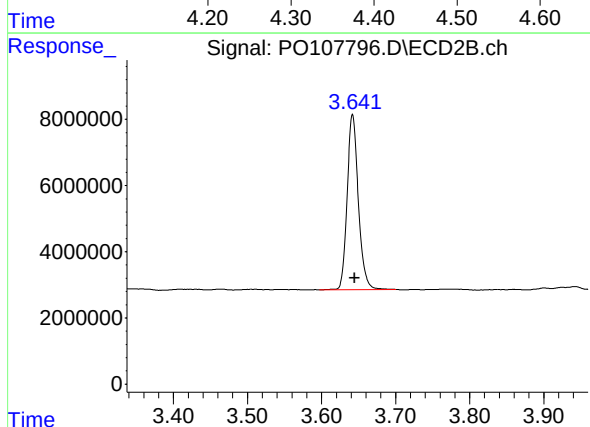


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.003 min
Response: 55444121
Conc: 17.23 ng/ml

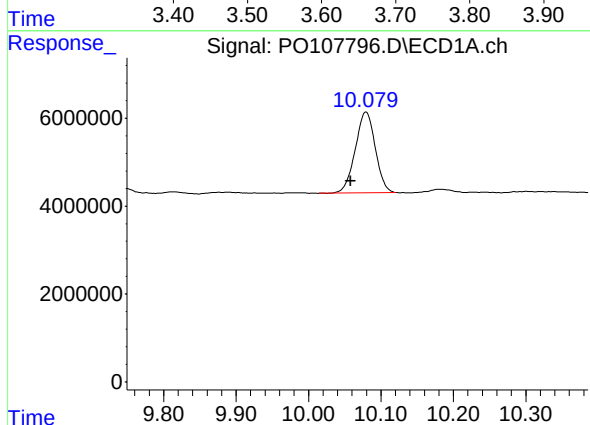

#2 Decachlorobiphenyl

R.T.: 10.079 min
Delta R.T.: 0.021 min
Response: 35319431
Conc: 14.40 ng/ml

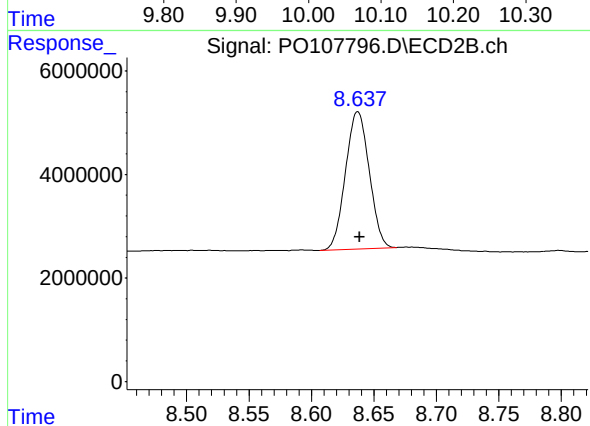

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: -0.002 min
Response: 35170984
Conc: 12.83 ng/ml