

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110725\
 Data File : PO114982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2025 20:13
 Operator : YP/AJ
 Sample : Q3579-02 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2404-0073-B

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/10/2025
 Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 01:41:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.346	3.647	3742566	3409058	0.532m	0.763m#
2) SA Decachlor...	9.936	8.643	4928700	3950570	1.115	1.012

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110725\
Data File : PO114982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2025 20:13
Operator : YP/AJ
Sample : Q3579-02 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2404-0073-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 01:41:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

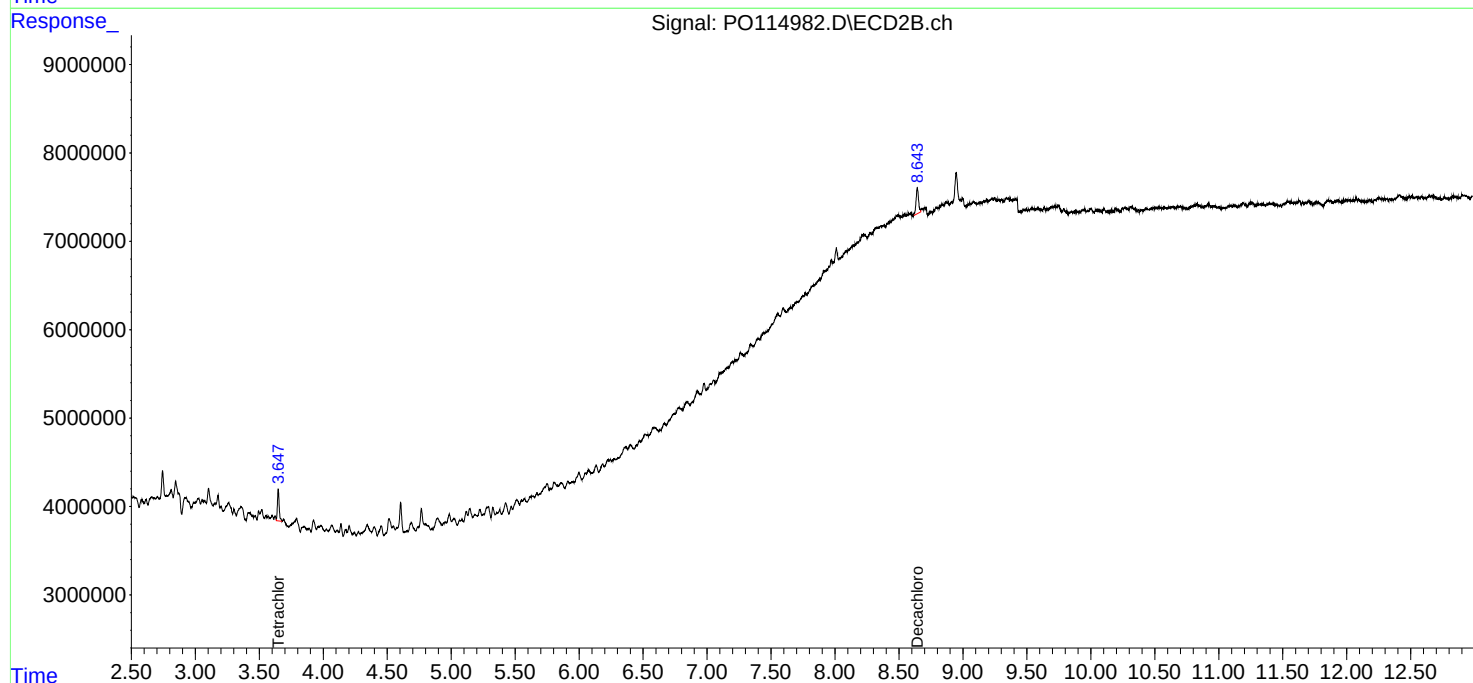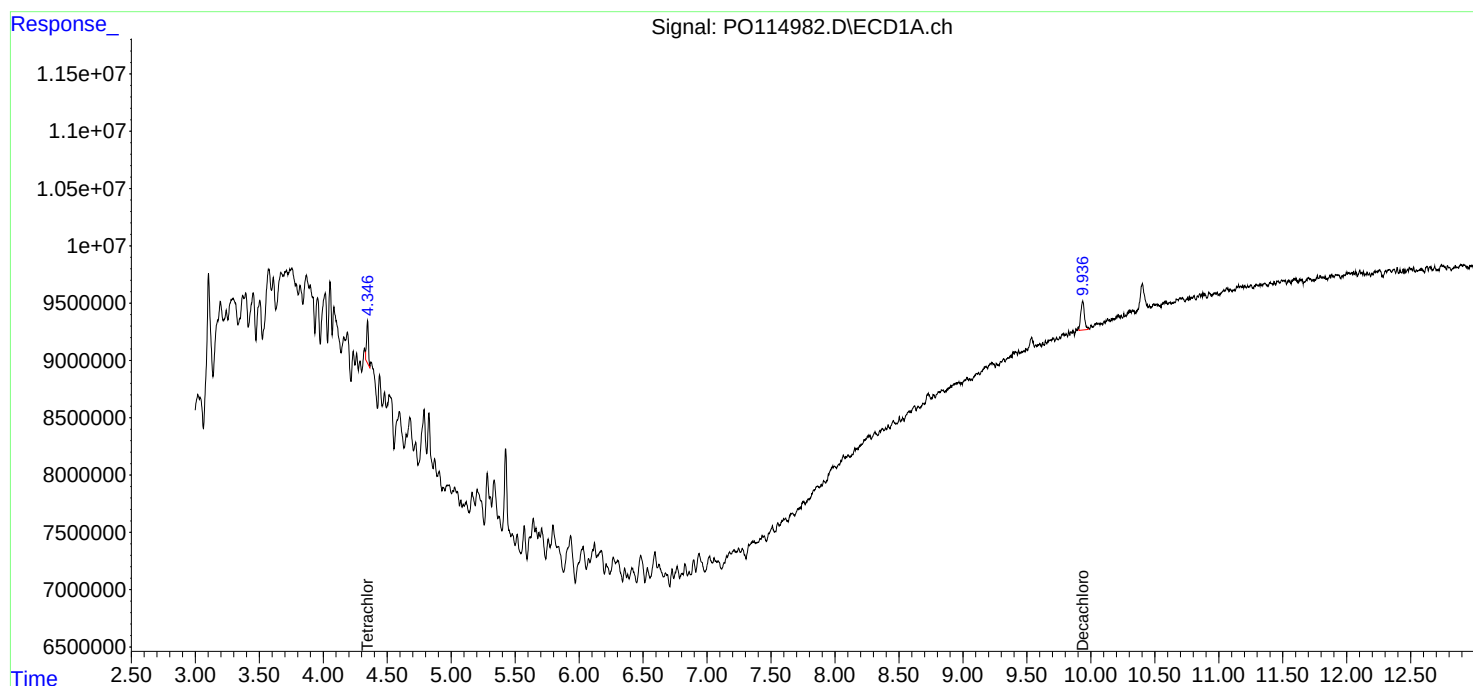

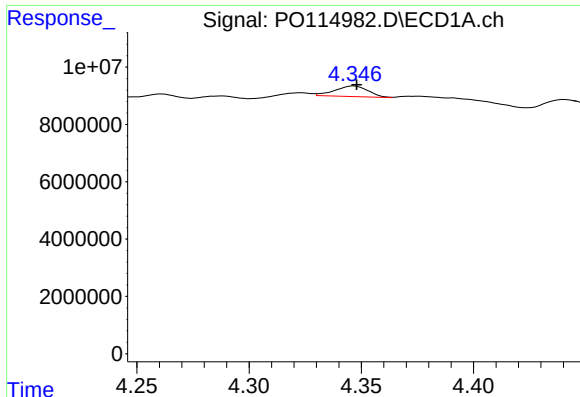


#1 Tetrachloro-m-xylene

R.T.: 4.346 min
Delta R.T.: -0.002 min
Response: 3742566
Conc: 0.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2404-0073-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

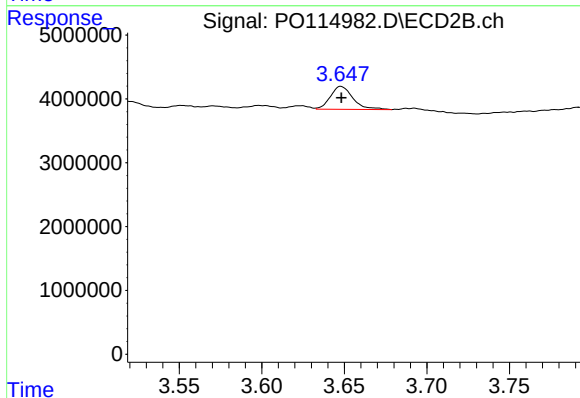


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 3409058
Conc: 0.76 ng/ml m

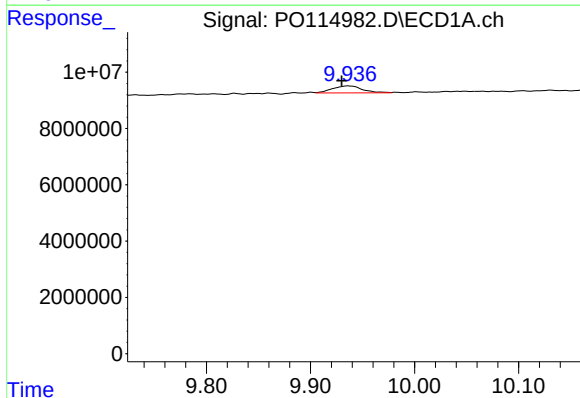

#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: 0.006 min
Response: 4928700
Conc: 1.12 ng/ml

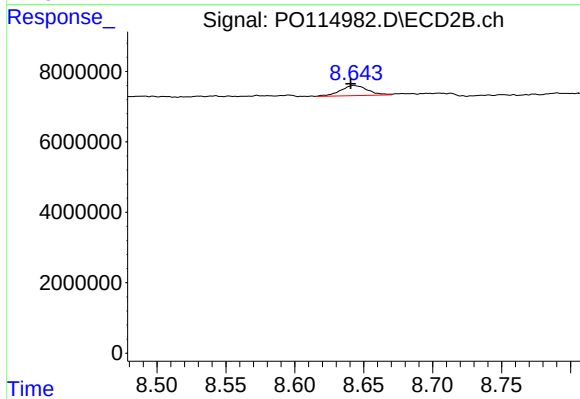

#2 Decachlorobiphenyl

R.T.: 8.643 min
Delta R.T.: 0.002 min
Response: 3950570
Conc: 1.01 ng/ml