

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110725\
 Data File : PO114983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Nov 2025 20:30
 Operator : YP/AJ
 Sample : Q3579-03 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FCA-340K-A

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/10/2025
 Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 01:42:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.346	3.647	6278582	4522460	0.892	1.012
2) SA Decachlor...	9.930	8.641	7904554	6562848	1.788m	1.681m
Target Compounds						
26) L6 AR-1254-1	6.329	5.525	12007246	14137616	47.379	47.097
27) L6 AR-1254-2	6.545	5.673	19507579	12151570	52.660m	45.071
28) L6 AR-1254-3	6.906	6.075	19336906	17240977	50.243	40.832
29) L6 AR-1254-4	7.186	6.303	16321839	13055102	49.653	43.898
30) L6 AR-1254-5	7.603	6.719	13807374	15085340	45.742	37.948

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110725\
Data File : PO114983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Nov 2025 20:30
Operator : YP/AJ
Sample : Q3579-03 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FCA-340K-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 01:42:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

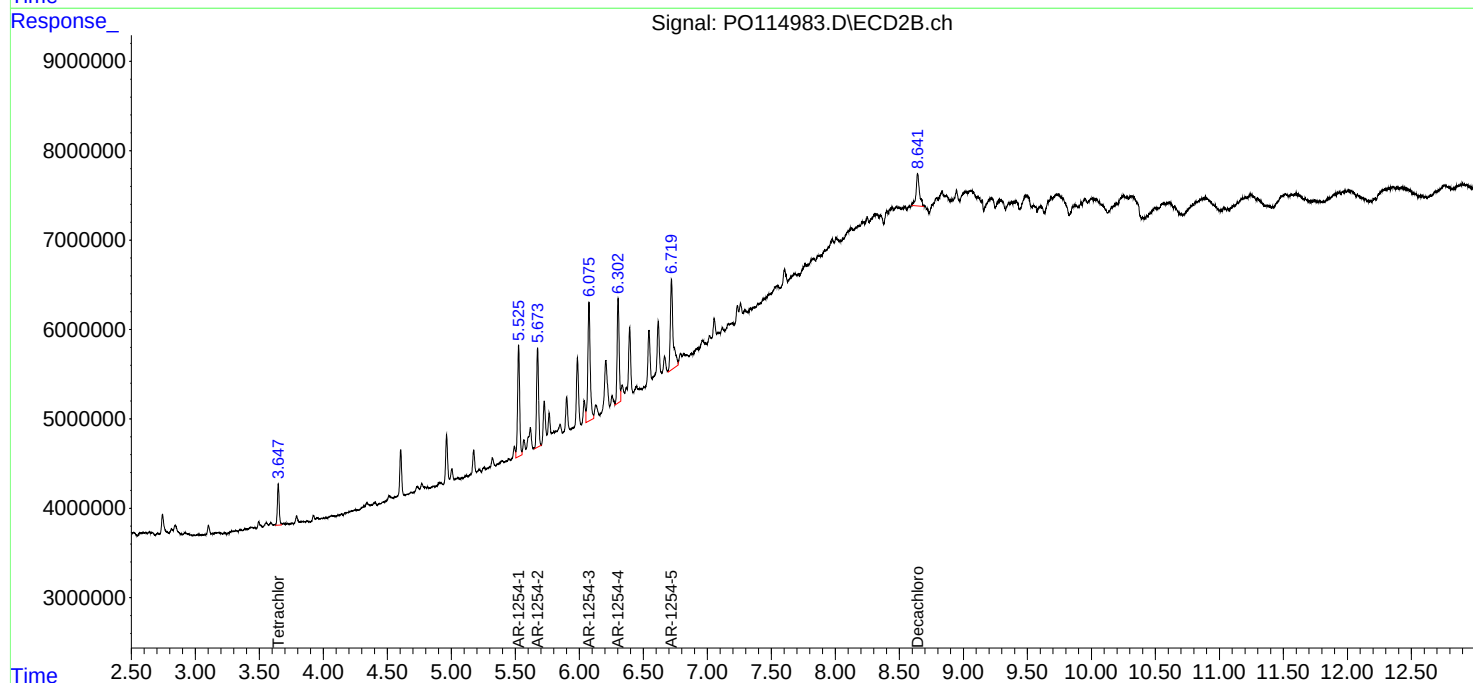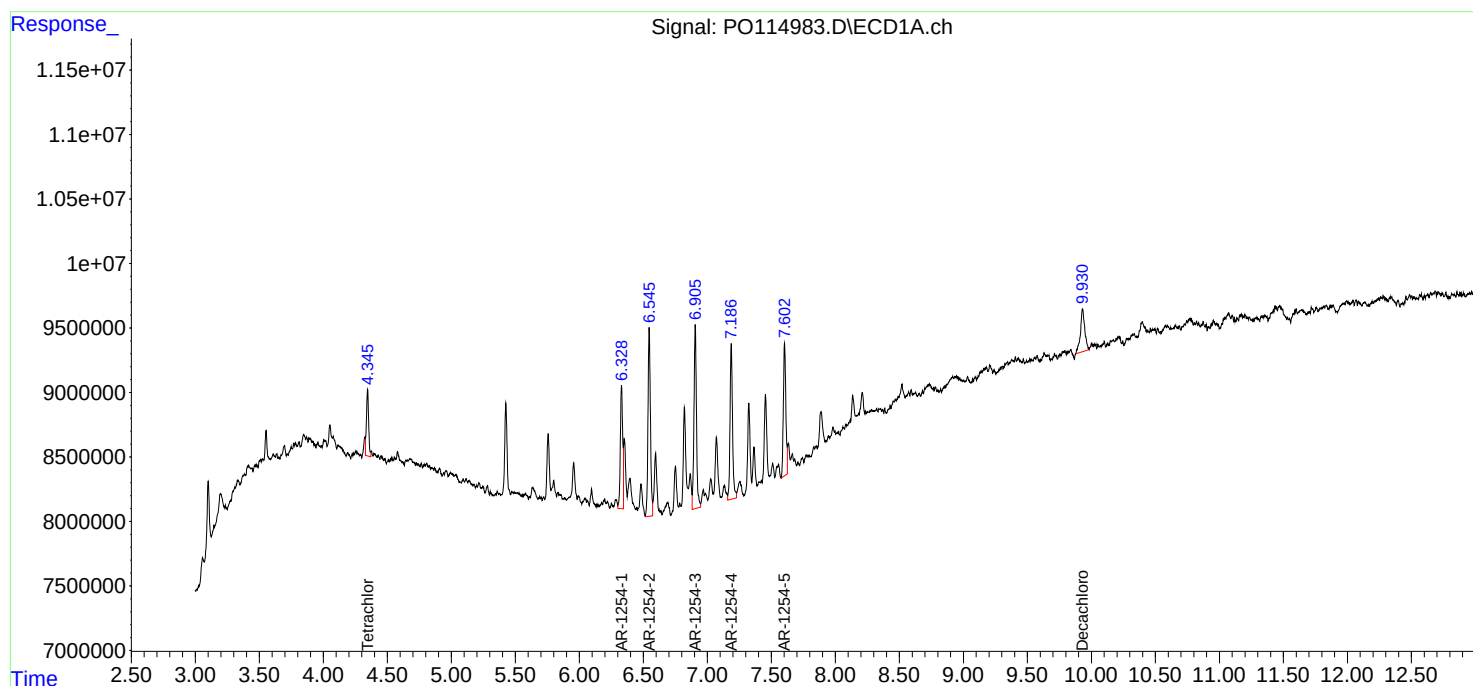

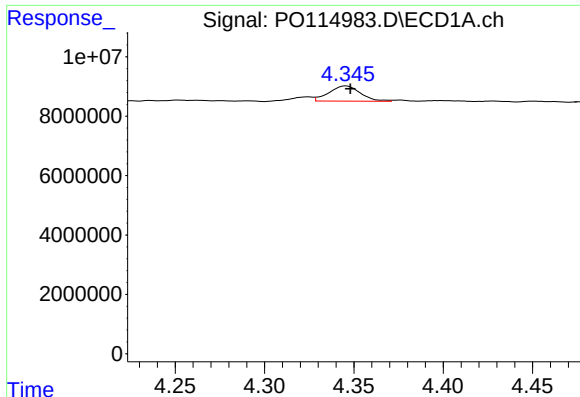


#1 Tetrachloro-m-xylene

R.T.: 4.346 min
Delta R.T.: -0.002 min
Response: 6278582
Conc: 0.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
FCA-340K-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

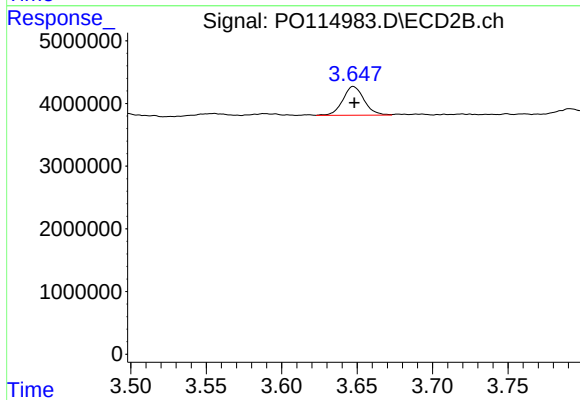


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 4522460
Conc: 1.01 ng/ml

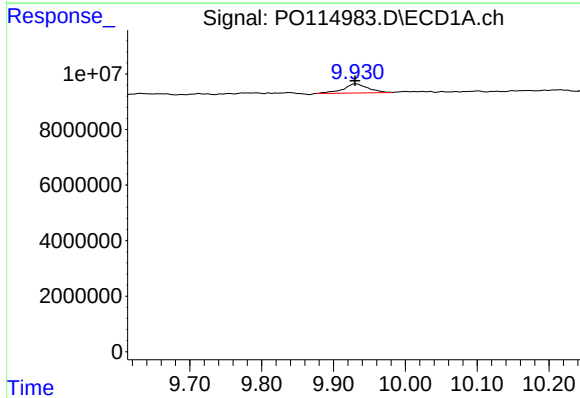


#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: 0.000 min
Response: 7904554
Conc: 1.79 ng/ml m

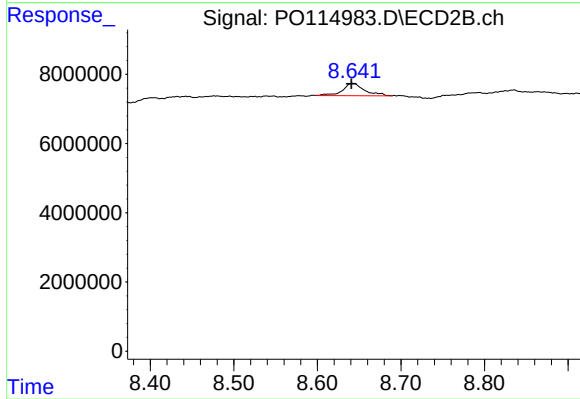

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 6562848
Conc: 1.68 ng/ml m

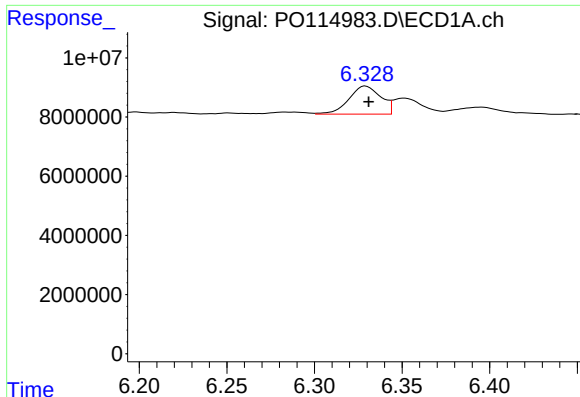


#26 AR-1254-1

R.T.: 6.329 min
Delta R.T.: -0.002 min
Response: 12007246
Conc: 47.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
FCA-340K-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

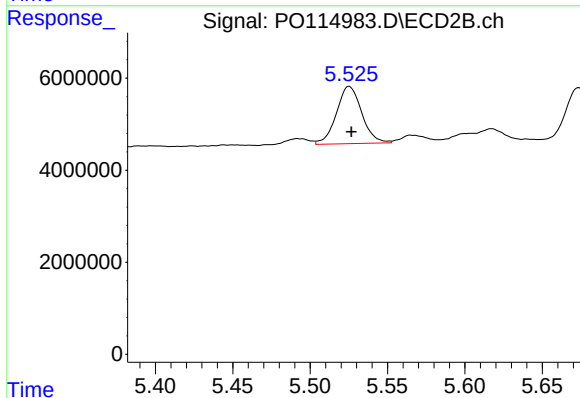


#26 AR-1254-1

R.T.: 5.525 min
Delta R.T.: -0.002 min
Response: 14137616
Conc: 47.10 ng/ml

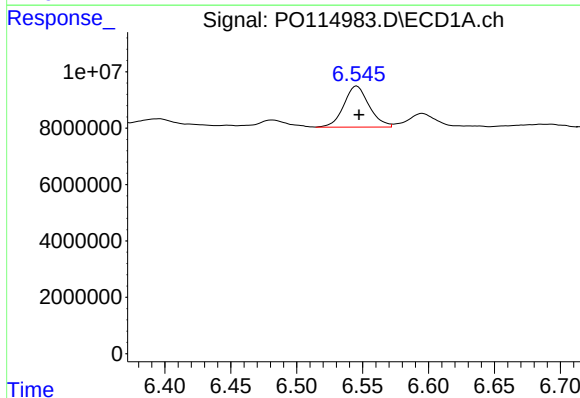


#27 AR-1254-2

R.T.: 6.545 min
Delta R.T.: -0.002 min
Response: 19507579
Conc: 52.66 ng/ml m

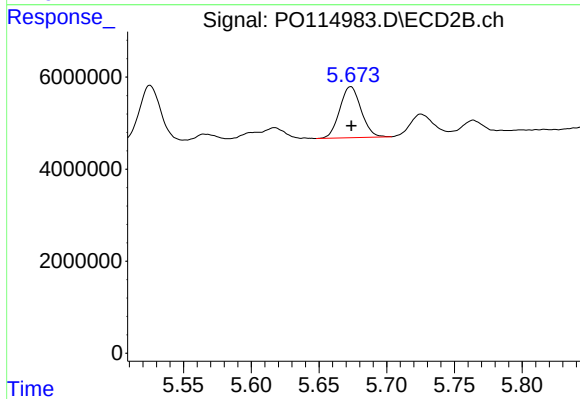

#27 AR-1254-2

R.T.: 5.673 min
Delta R.T.: 0.000 min
Response: 12151570
Conc: 45.07 ng/ml

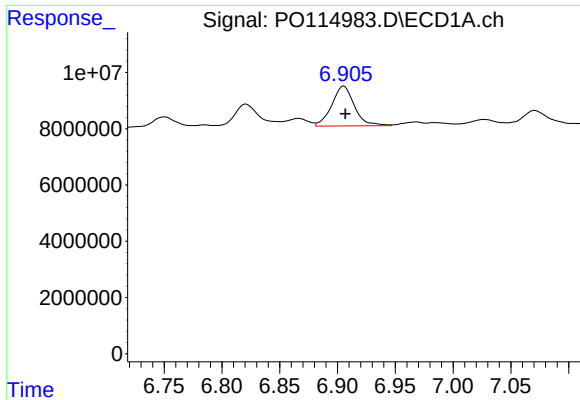


#28 AR-1254-3

R.T.: 6.906 min
Delta R.T.: -0.001 min
Response: 19336906
Conc: 50.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
FCA-340K-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

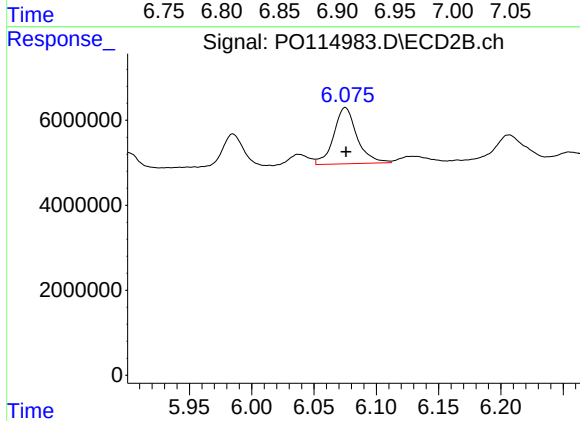


#28 AR-1254-3

R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 17240977
Conc: 40.83 ng/ml

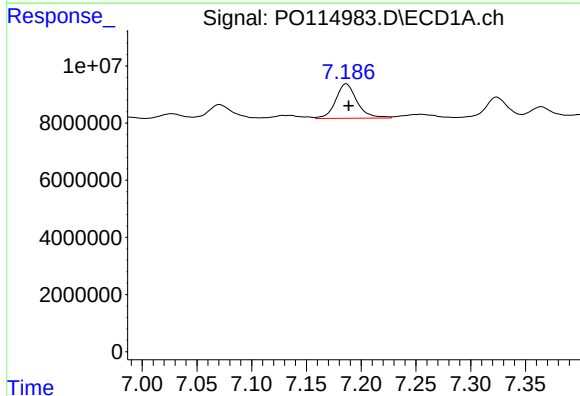


#29 AR-1254-4

R.T.: 7.186 min
Delta R.T.: -0.002 min
Response: 16321839
Conc: 49.65 ng/ml

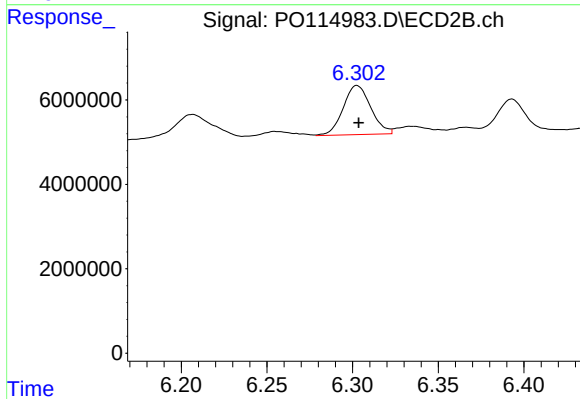

#29 AR-1254-4

R.T.: 6.303 min
Delta R.T.: -0.001 min
Response: 13055102
Conc: 43.90 ng/ml

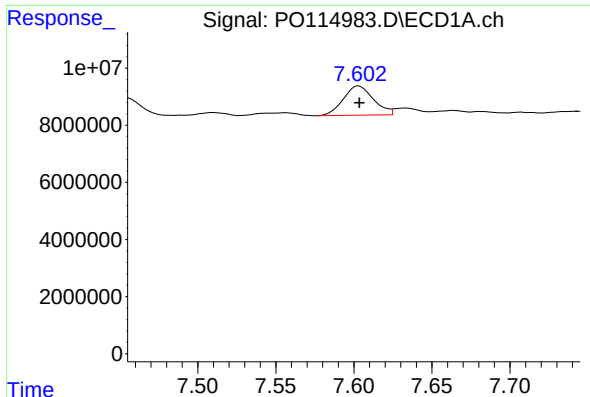


#30 AR-1254-5

R.T.: 7.603 min
Delta R.T.: 0.000 min
Response: 13807374
Conc: 45.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
FCA-340K-A

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/10/2025
Supervised By :Yogesh Patel 11/10/2025

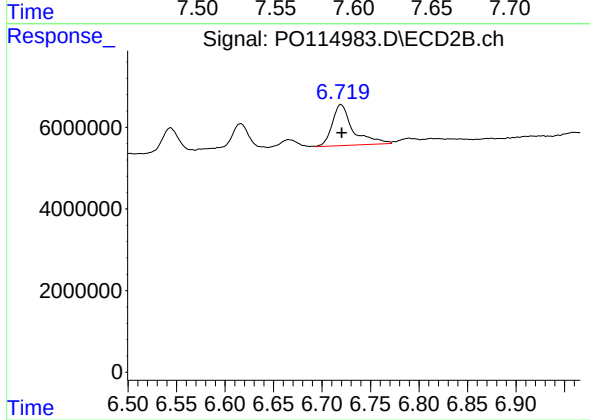

#30 AR-1254-5

R.T.: 6.719 min
Delta R.T.: 0.000 min
Response: 15085340
Conc: 37.95 ng/ml