

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110818\
 Data File : PO051190.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Nov 2018 10:54
 Operator : SM/SJ
 Sample : J5816-07RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4A-SRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 07 11:18:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 06 00:37:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.337	5639899	2493530	15.117	12.086
2) SA Decachlor...	9.982	8.073	2687465	1722370	9.100	8.113

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110818\
Data File : PO051190.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Nov 2018 10:54
Operator : SM/SJ
Sample : J5816-07RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-4A-SRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 11:18:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 06 00:37:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

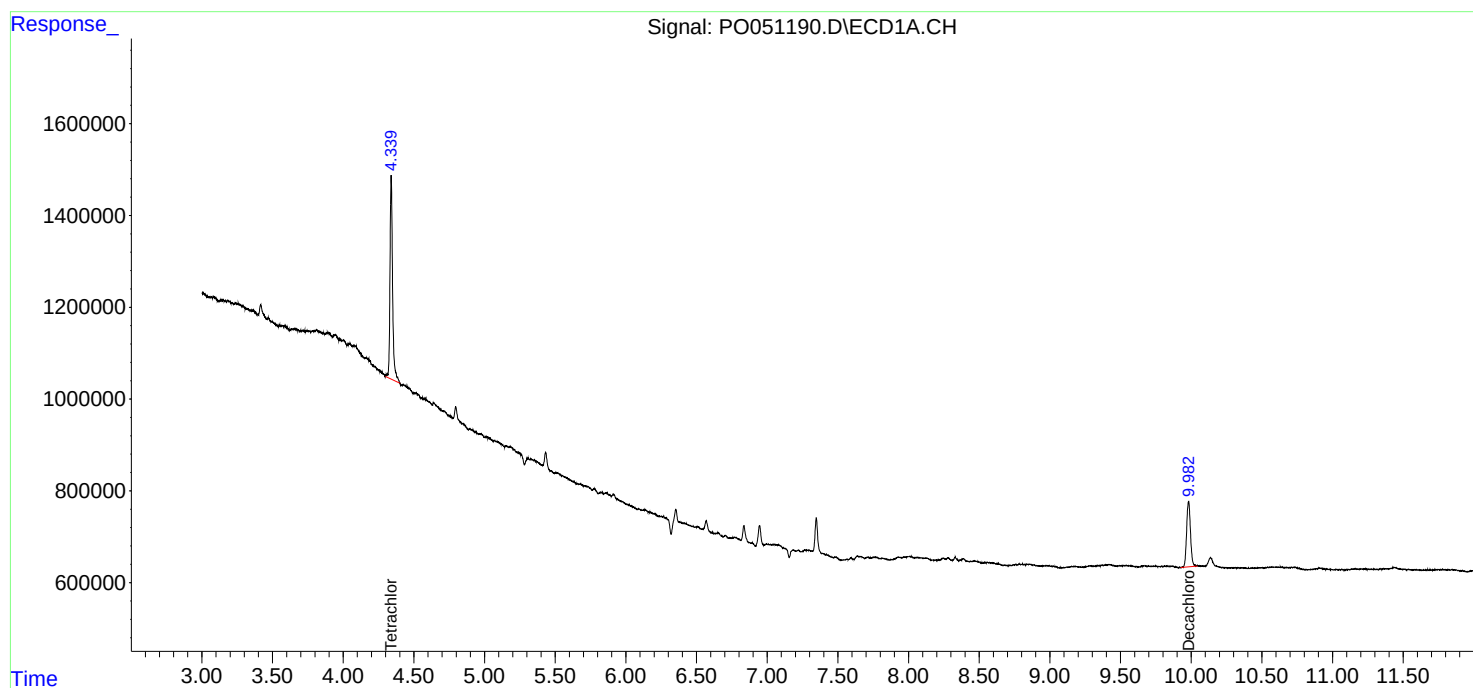


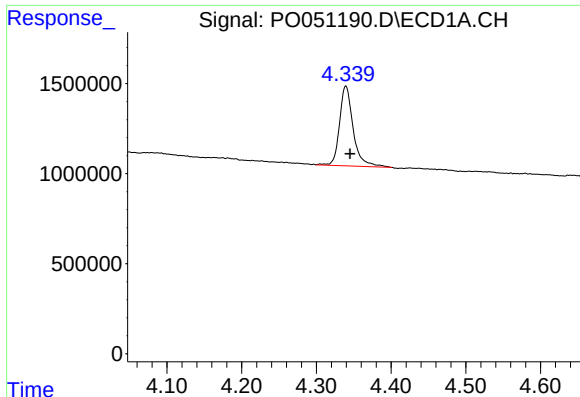

#1 Tetrachloro-m-xylene


R.T.: 4.339 min
Delta R.T.: -0.006 min
Response: 5639899
Conc: 15.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4A-SRE

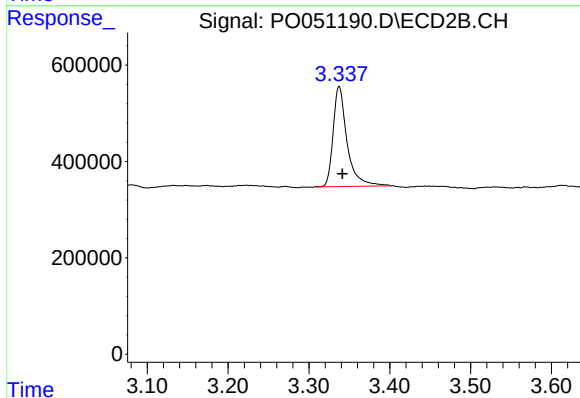


#1 Tetrachloro-m-xylene

R.T.: 3.337 min
Delta R.T.: -0.004 min
Response: 2493530
Conc: 12.09 ng/ml

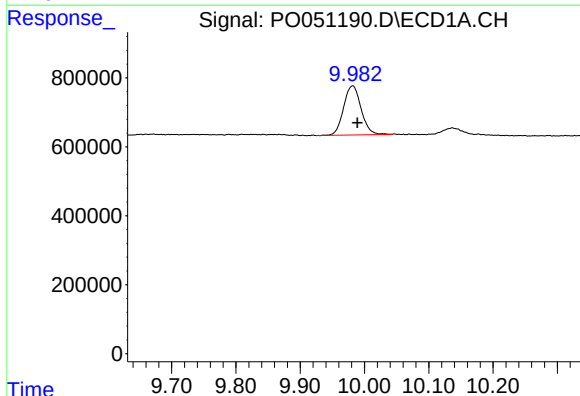

#2 Decachlorobiphenyl

R.T.: 9.982 min
Delta R.T.: -0.007 min
Response: 2687465
Conc: 9.10 ng/ml

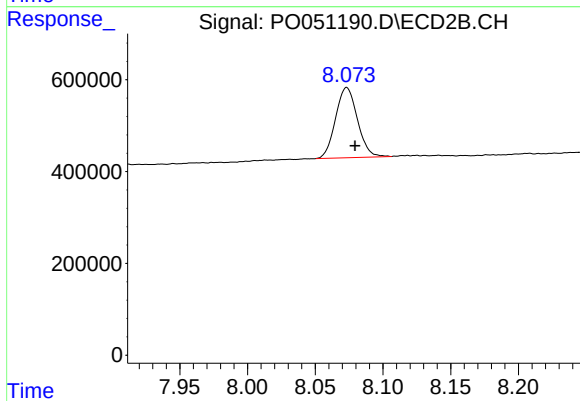

#2 Decachlorobiphenyl

R.T.: 8.073 min
Delta R.T.: -0.006 min
Response: 1722370
Conc: 8.11 ng/ml