

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110819\
 Data File : PO063588.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2019 11:14
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 12:37:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 04:54:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.322	3.576	779038	530582	23.543	25.164
2) SA Decachlor...	9.947	8.551	1080224	615683	19.686	20.771

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110819\
Data File : PO063588.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2019 11:14
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 12:37:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 04:54:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

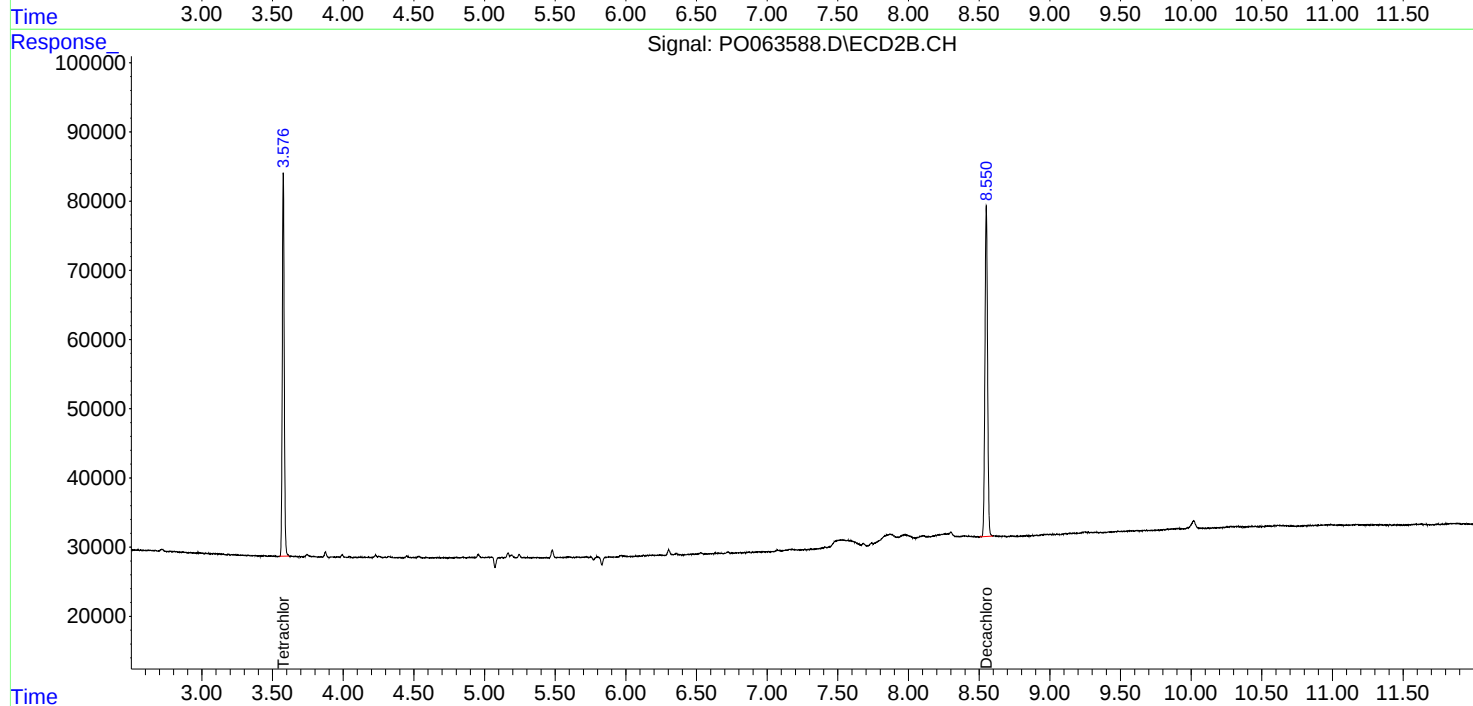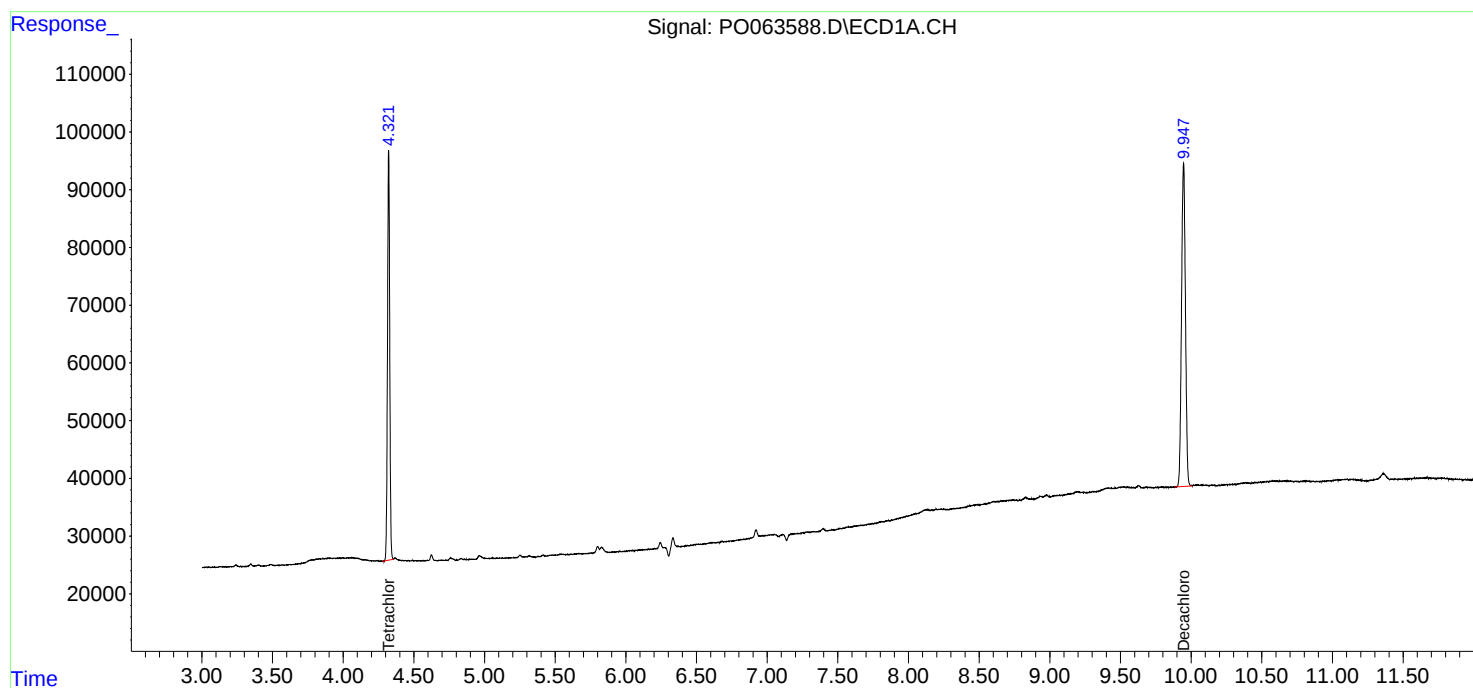


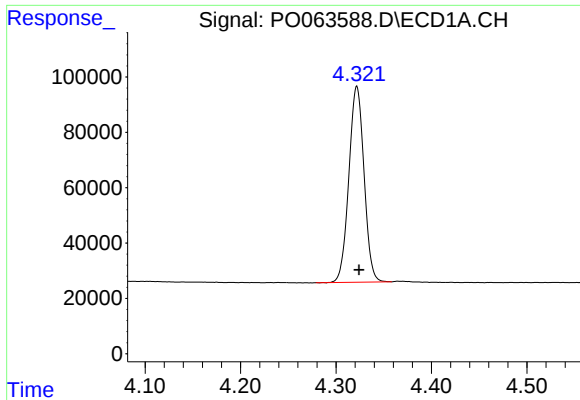

#1 Tetrachloro-m-xylene


R.T.: 4.322 min
Delta R.T.: -0.002 min
Response: 779038
Conc: 23.54 ng/ml

Instrument :
ECD_O
ClientSampleId :

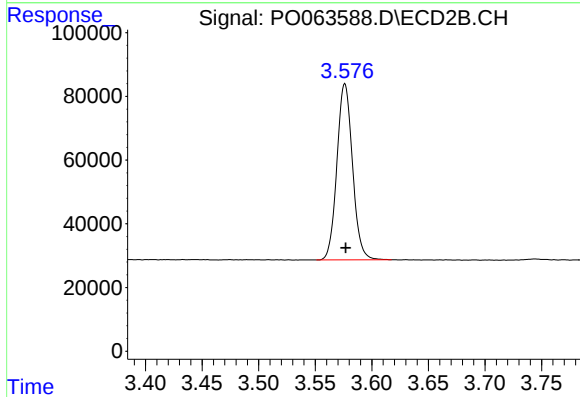


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: 0.000 min
Response: 530582
Conc: 25.16 ng/ml

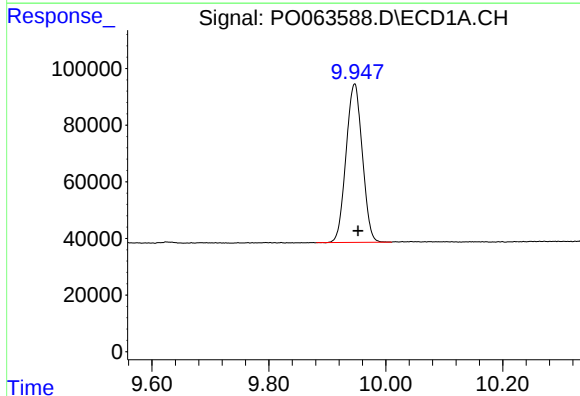

#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.006 min
Response: 1080224
Conc: 19.69 ng/ml

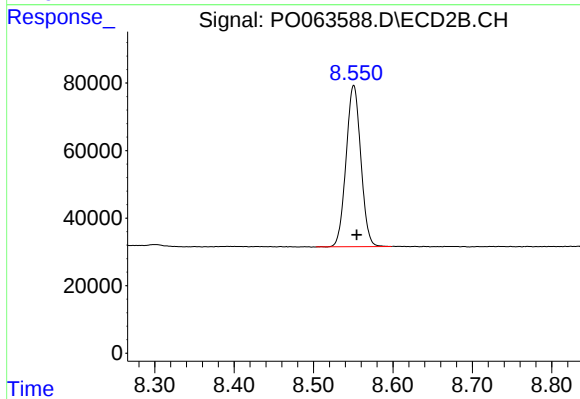

#2 Decachlorobiphenyl

R.T.: 8.551 min
Delta R.T.: -0.004 min
Response: 615683
Conc: 20.77 ng/ml