

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110819\
 Data File : P0063584.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2019 10:07
 Operator : SM/AJ
 Sample : K5733-02 20X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 02-A-02-B-02-C

Manual Integrations
 APPROVED

Ankita
 11/11/2019 8:58:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 12:36:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 04:54:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.319	3.576	37340	21847	1.128m	1.036m
2)	SA Decachlor...	9.946	8.550	44797	26612	0.816m	0.898m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110819\
Data File : PO063584.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2019 10:07
Operator : SM/AJ
Sample : K5733-02 20X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
11/11/2019 8:58:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 12:36:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 04:54:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

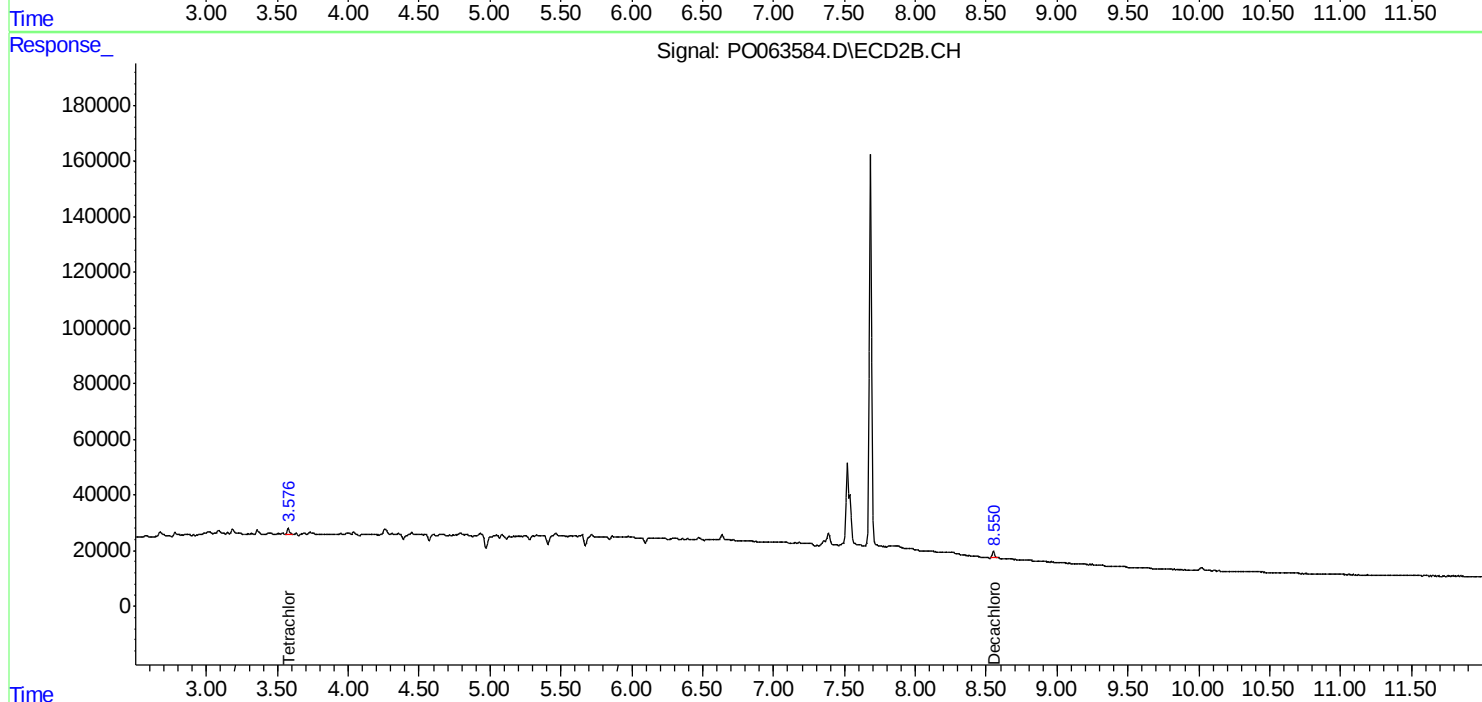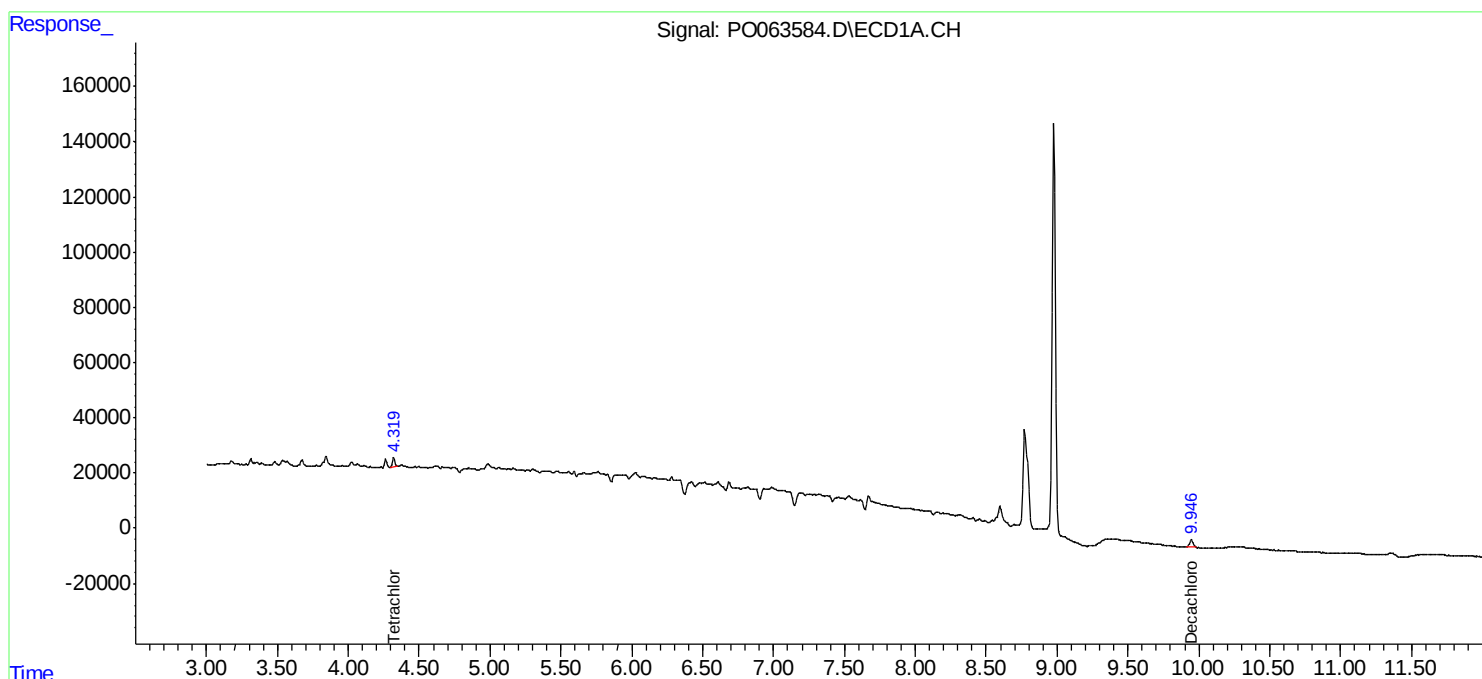

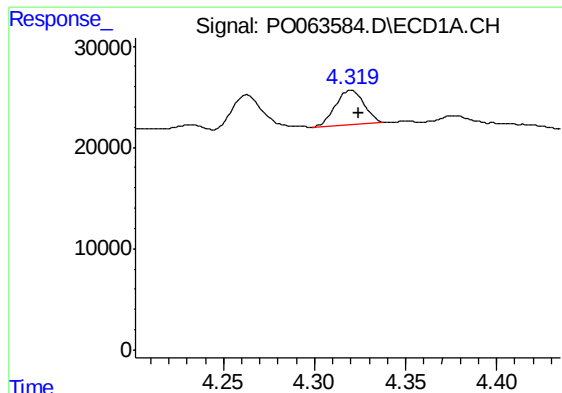


#1 Tetrachloro-m-xylene

R.T.: 4.319 min
Delta R.T.: -0.005 min
Response: 37340
Conc: 1.13 ng/ml m

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
11/11/2019 8:58:43 AM

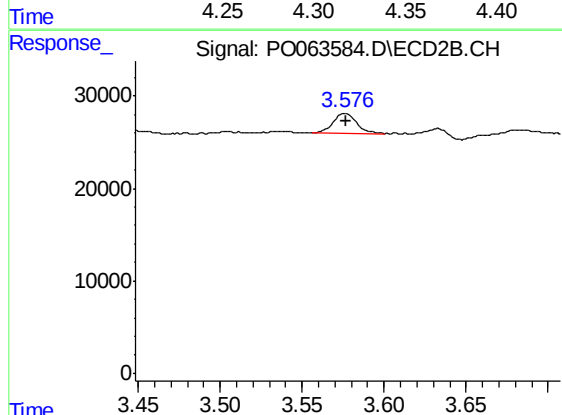


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: -0.001 min
Response: 21847
Conc: 1.04 ng/ml m

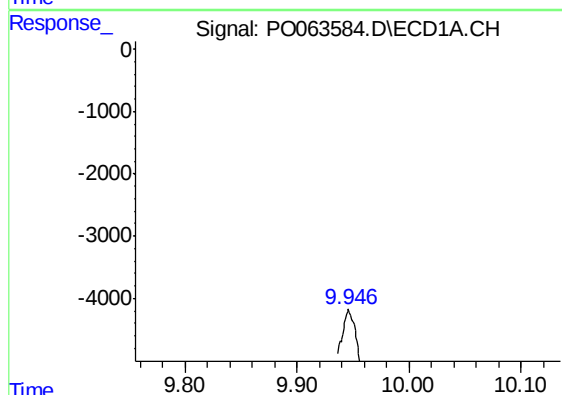

#2 Decachlorobiphenyl

R.T.: 9.946 min
Delta R.T.: -0.007 min
Response: 44797
Conc: 0.82 ng/ml m

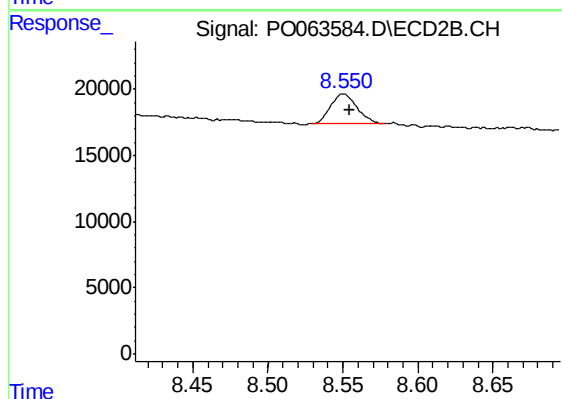

#2 Decachlorobiphenyl

R.T.: 8.550 min
Delta R.T.: -0.004 min
Response: 26612
Conc: 0.90 ng/ml m