

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110819\
Data File : P0063599.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2019 14:28
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 15:52:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 04:54:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.321	3.576	884596	597947	26.733	28.359
2)	SA Decachlor...	9.947	8.551	952237	544736	17.354	18.378

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110819\
Data File : P0063599.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2019 14:28
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 15:52:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 04:54:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

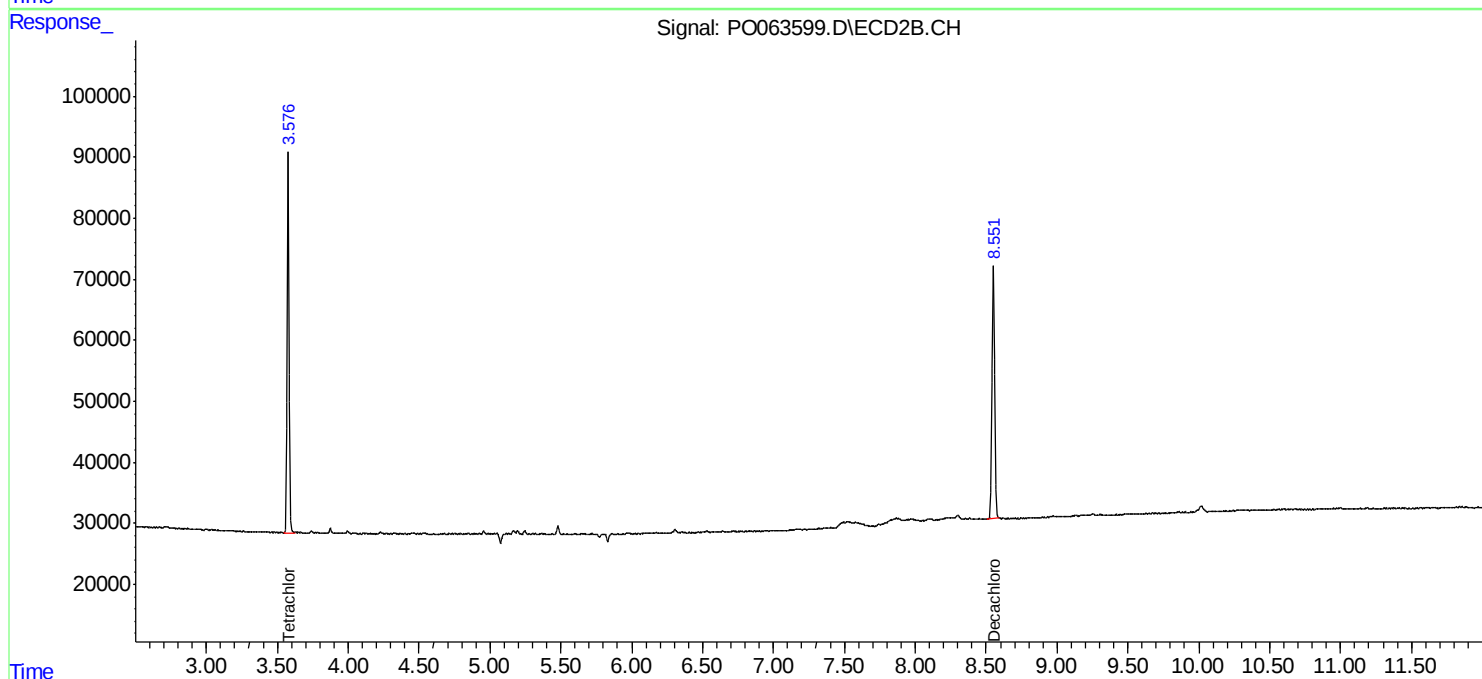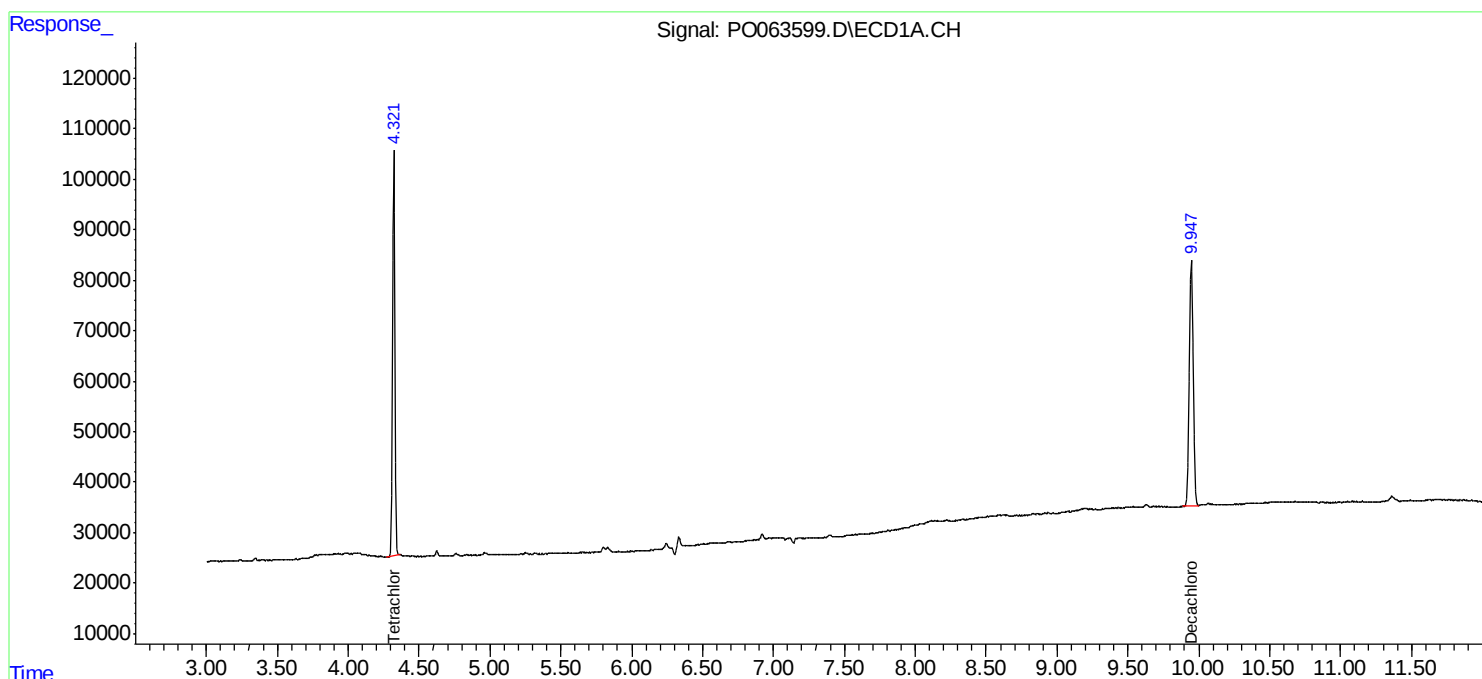


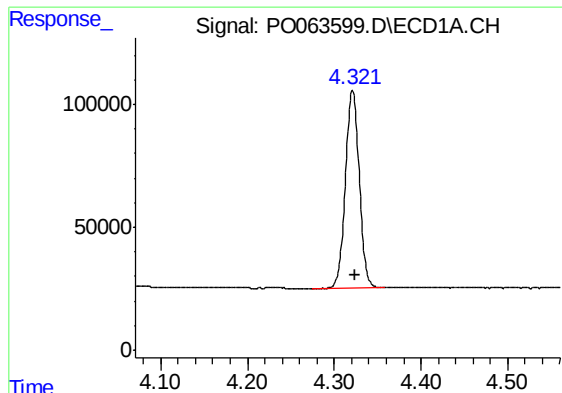

#1 Tetrachloro-m-xylene


R.T.: 4.321 min
Delta R.T.: -0.003 min
Response: 884596
Conc: 26.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

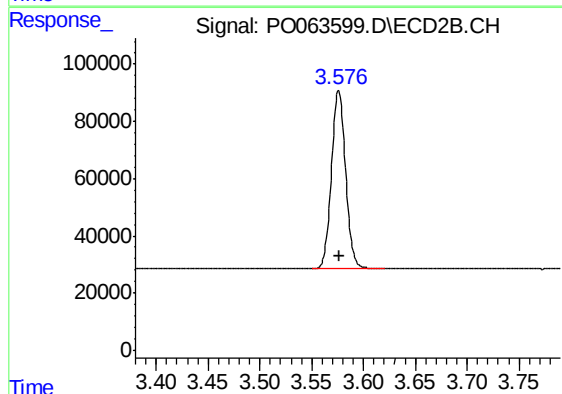


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: -0.001 min
Response: 597947
Conc: 28.36 ng/ml

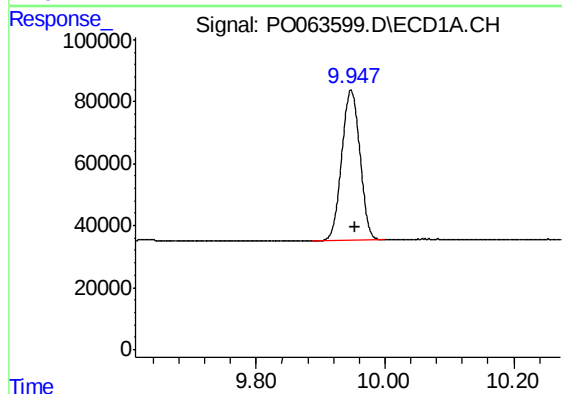

#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.006 min
Response: 952237
Conc: 17.35 ng/ml

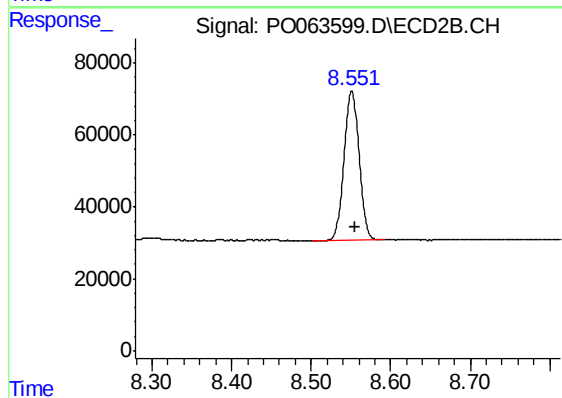

#2 Decachlorobiphenyl

R.T.: 8.551 min
Delta R.T.: -0.003 min
Response: 544736
Conc: 18.38 ng/ml