

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
 Data File : PO082596.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2021 12:35
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 08:24:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.962	1688462	617343	19.290	19.948
2)	SA Decachlor...	11.067	9.276	1245741	614523	19.726	21.343
Target Compounds							
8)	L2 AR-1221-1	5.205f	0.000	36453	0	38.654	N.D. #
9)	L2 AR-1221-2	5.323	4.313	22737	8089	35.078	27.865
10)	L2 AR-1221-3	0.000	4.407	0	26310	N.D.	28.433 #
11)	L3 AR-1232-1	0.000	4.407	0	26310	N.D.	33.327 #
28)	L6 AR-1254-3	7.850	0.000	36201	0	8.464	N.D. #
33)	L7 AR-1260-3	8.643	7.164	5625	9022	1.986	4.242 #
34)	L7 AR-1260-4	8.881	0.000	13259	0	3.978	N.D. #
36)	L8 AR-1262-1	8.643	0.000	5625	0	1.516	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
Data File : PO082596.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 12:35
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:24:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

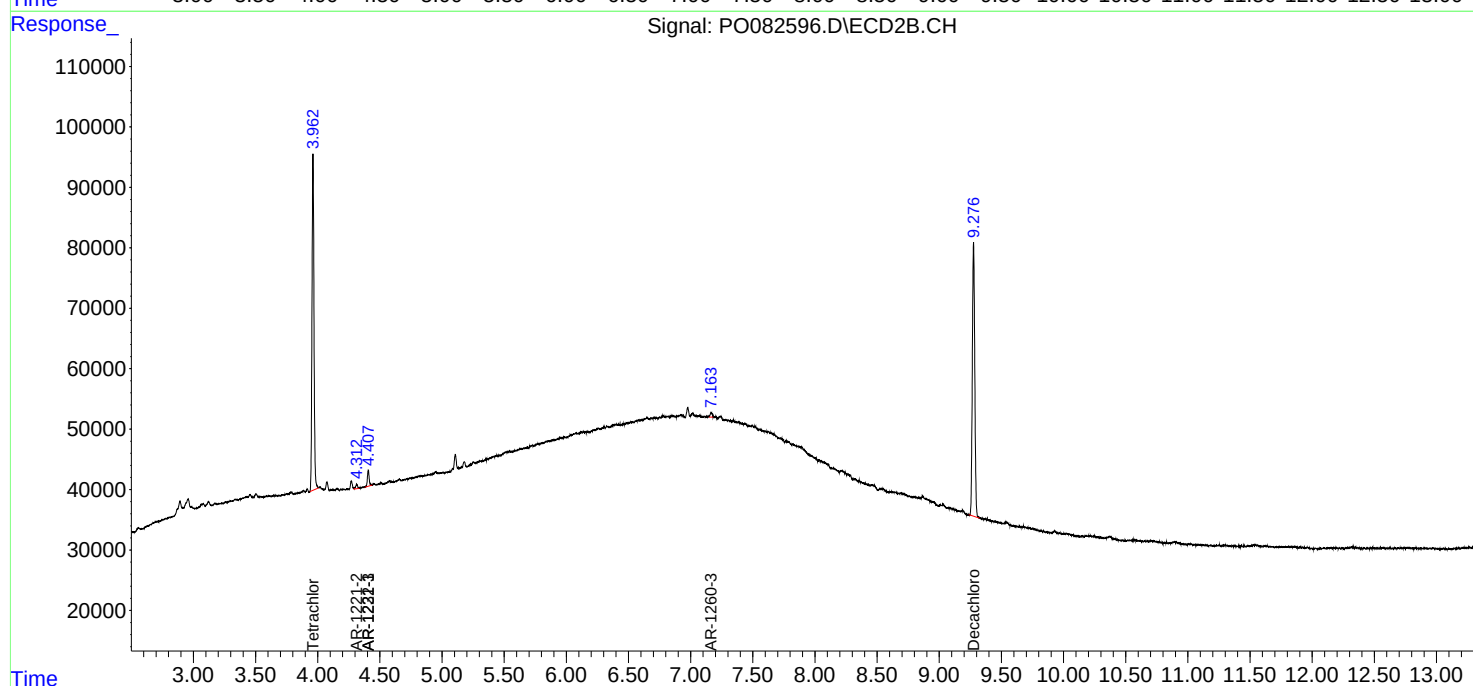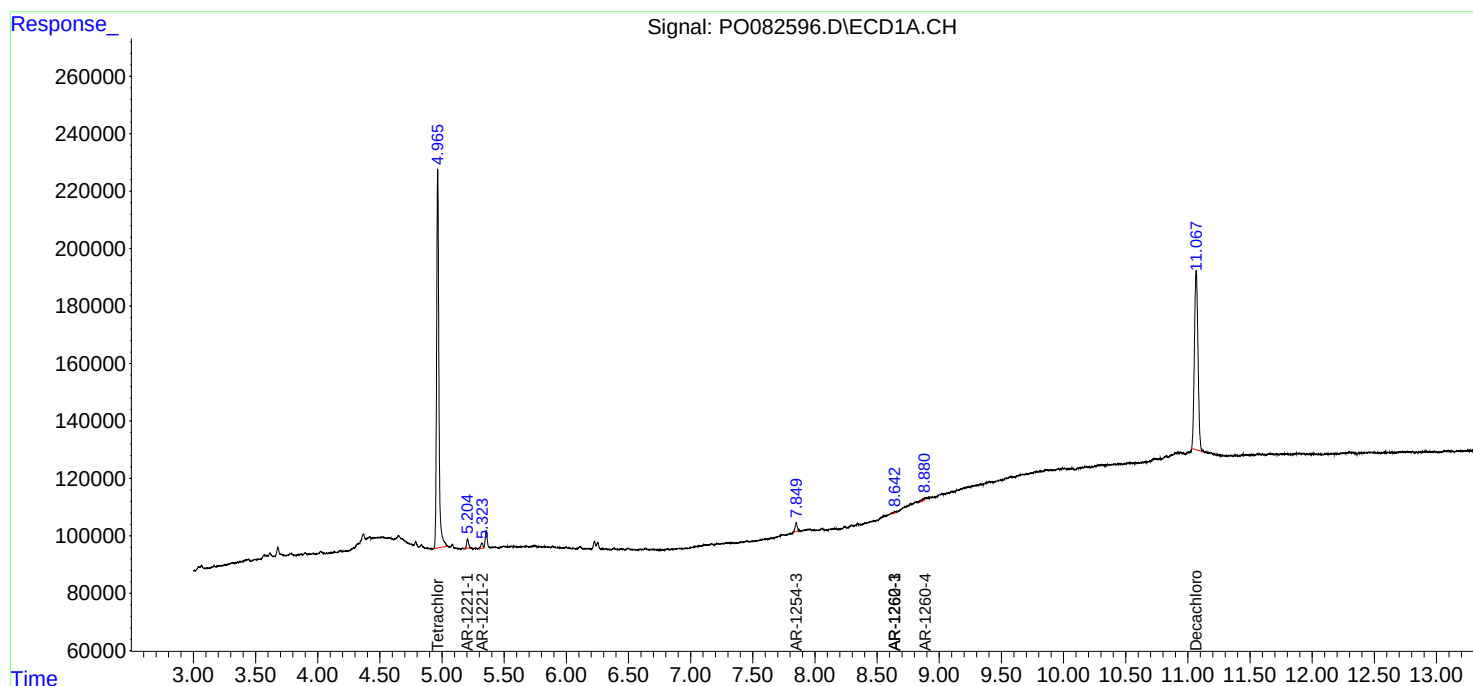


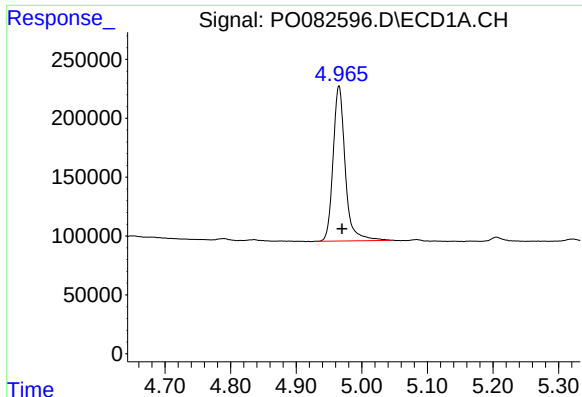

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: -0.005 min
Response: 1688462
Conc: 19.29 ng/ml

Instrument :
ECD_O
ClientSampleId :

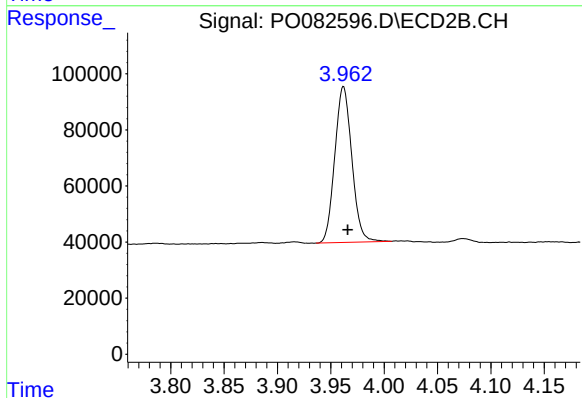


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.004 min
Response: 617343
Conc: 19.95 ng/ml

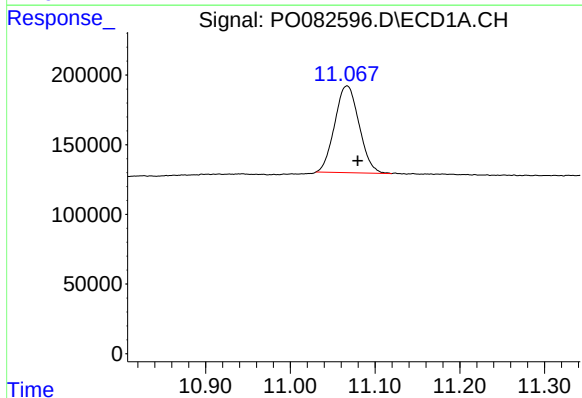


#2 Decachlorobiphenyl

R.T.: 11.067 min
Delta R.T.: -0.013 min
Response: 1245741
Conc: 19.73 ng/ml

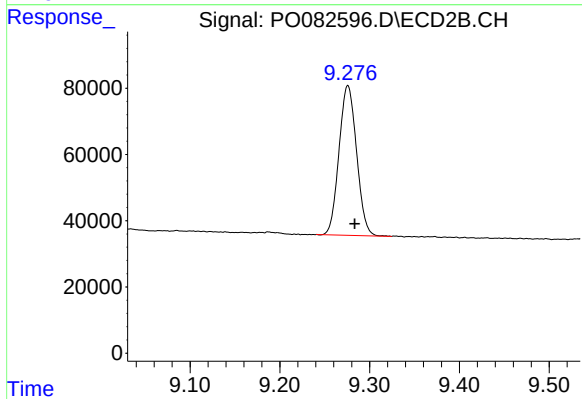

#2 Decachlorobiphenyl


R.T.: 9.276 min
Delta R.T.: -0.008 min
Response: 614523
Conc: 21.34 ng/ml

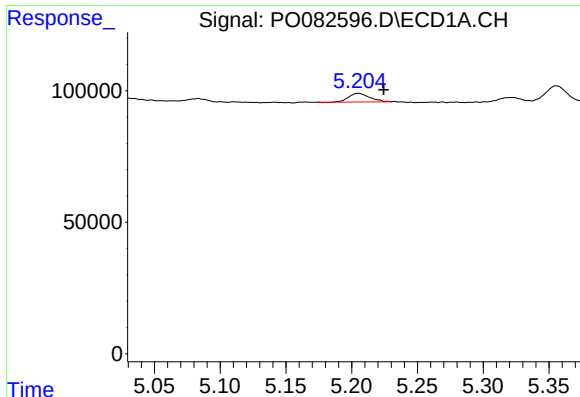

#8 AR-1221-1


R.T.: 5.205 min
Delta R.T.: -0.019 min
Response: 36453
Conc: 38.65 ng/ml

Instrument :
ECD_O
ClientSampleId :

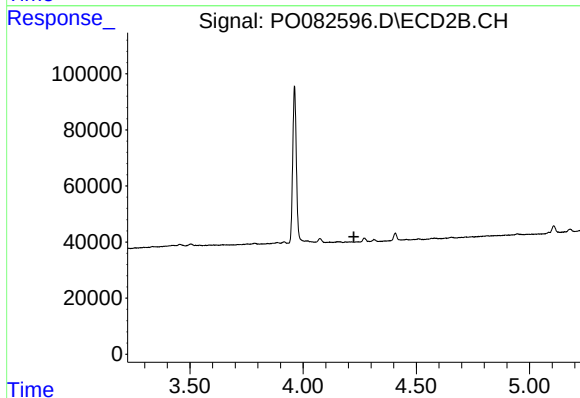


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.224 min
Response: 0
Conc: N.D.

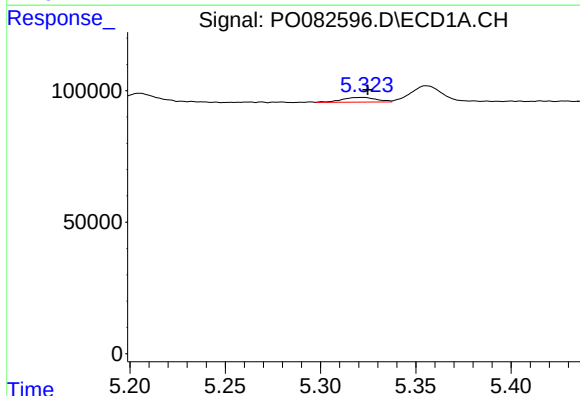


#9 AR-1221-2

R.T.: 5.323 min
Delta R.T.: -0.002 min
Response: 22737
Conc: 35.08 ng/ml

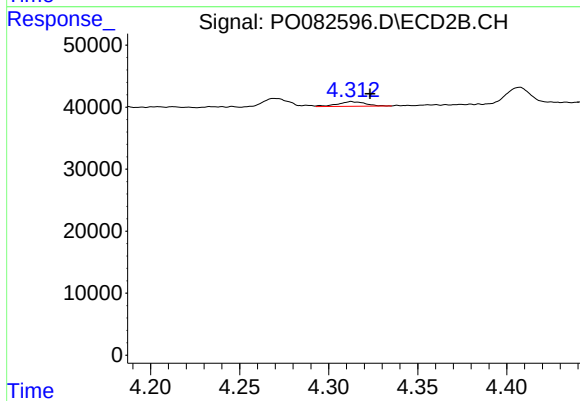

#9 AR-1221-2


R.T.: 4.313 min
Delta R.T.: -0.011 min
Response: 8089
Conc: 27.86 ng/ml

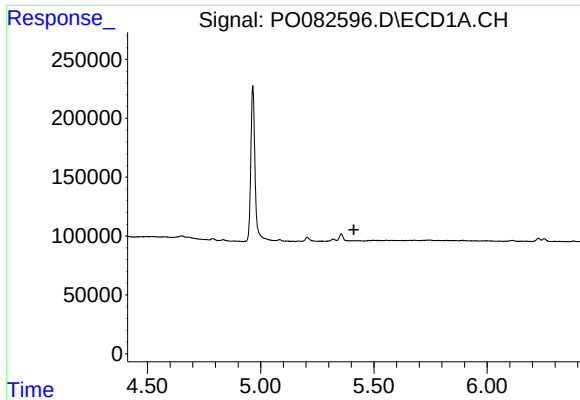

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

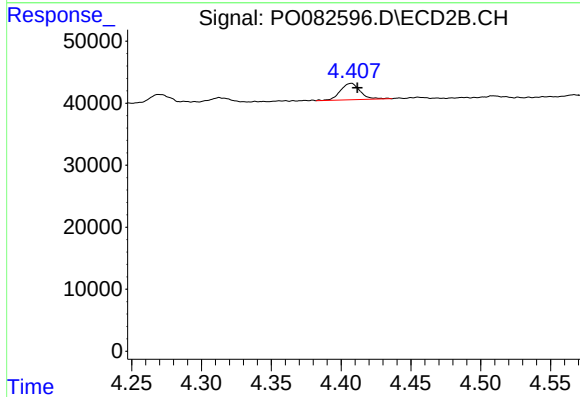


#10 AR-1221-3

R.T.: 4.407 min
Delta R.T.: -0.004 min
Response: 26310
Conc: 28.43 ng/ml

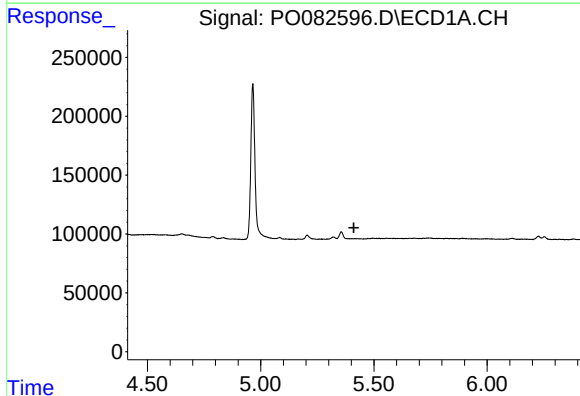


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.

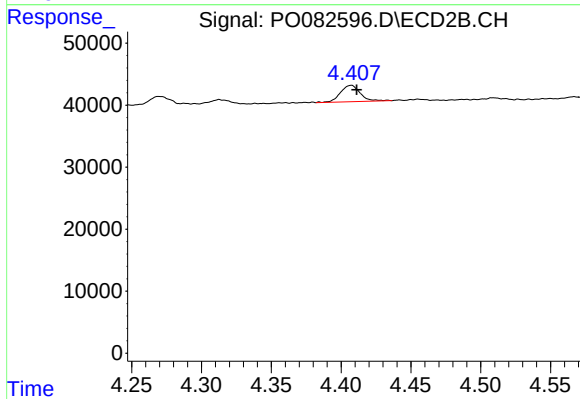

#11 AR-1232-1


R.T.: 4.407 min
Delta R.T.: -0.004 min
Response: 26310
Conc: 33.33 ng/ml

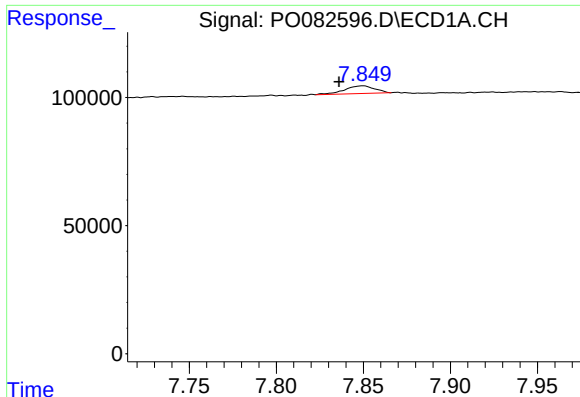

#28 AR-1254-3


R.T.: 7.850 min
Delta R.T.: 0.014 min
Response: 36201
Conc: 8.46 ng/ml

Instrument :
ECD_O
ClientSampleId :

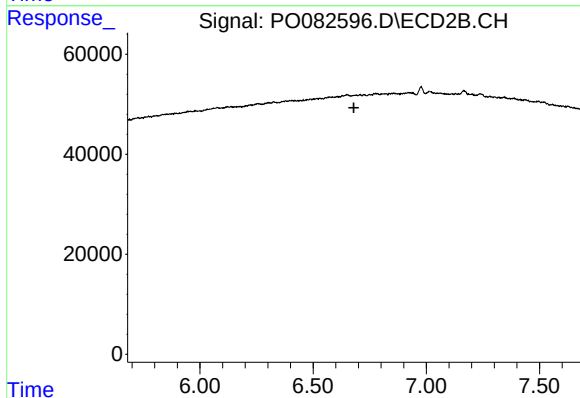


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

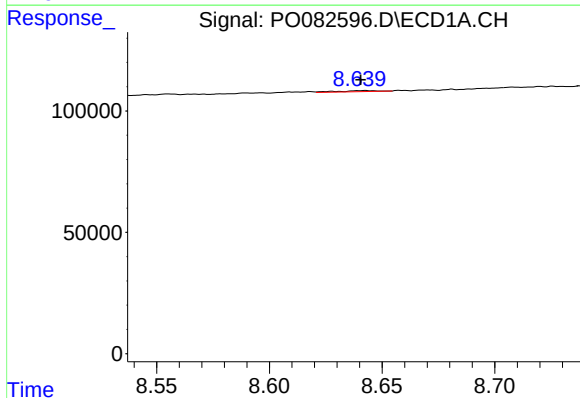


#33 AR-1260-3

R.T.: 8.643 min
Delta R.T.: 0.002 min
Response: 5625
Conc: 1.99 ng/ml

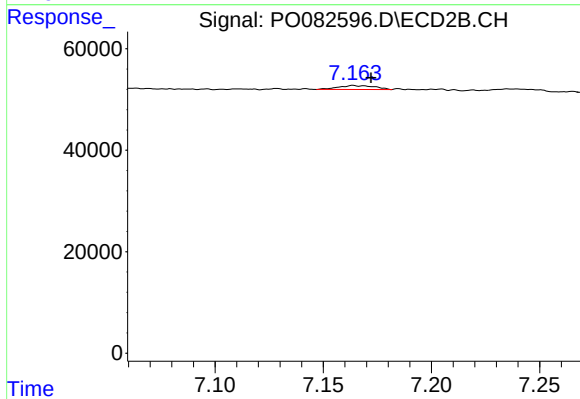

#33 AR-1260-3


R.T.: 7.164 min
Delta R.T.: -0.008 min
Response: 9022
Conc: 4.24 ng/ml

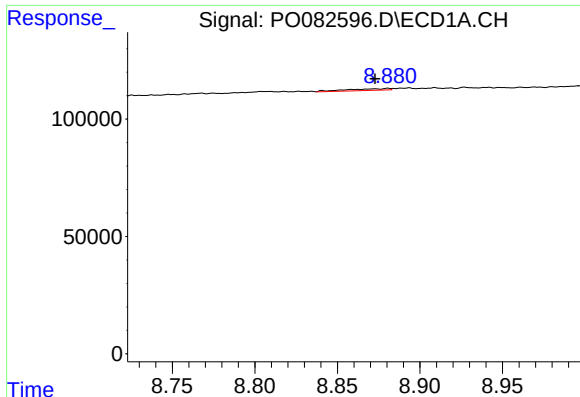

#34 AR-1260-4


R.T.: 8.881 min
Delta R.T.: 0.008 min
Response: 13259
Conc: 3.98 ng/ml

Instrument :
ECD_O
ClientSampleId :

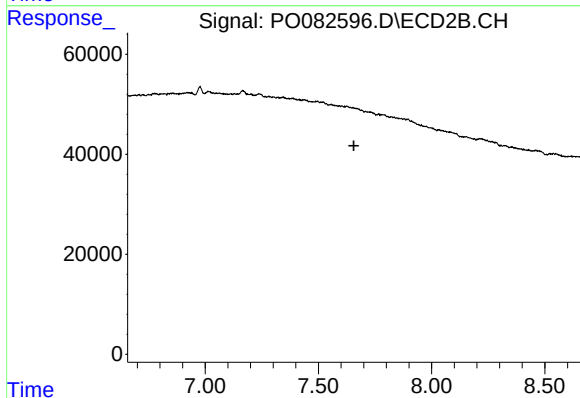


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.657 min
Response: 0
Conc: N.D.

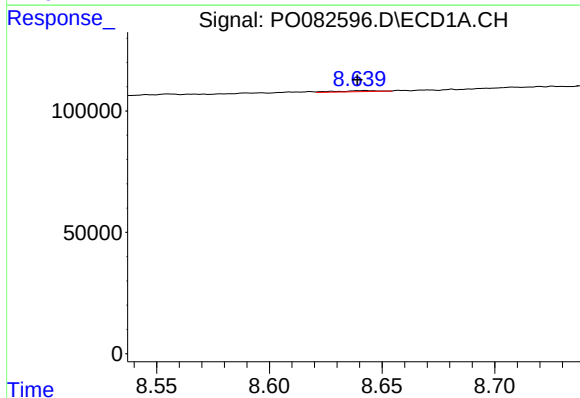

#36 AR-1262-1

R.T.: 8.643 min
Delta R.T.: 0.004 min
Response: 5625
Conc: 1.52 ng/ml

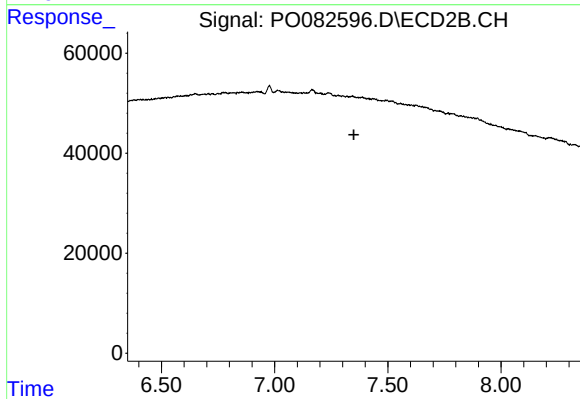

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.