

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
 Data File : PO082609.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2021 16:55
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 08:25:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.963	1728367	631967	19.746	20.421
2)	SA Decachlor...	11.070	9.277	1281806	629783	20.297	21.873
Target Compounds							
8)	L2 AR-1221-1	5.207f	0.000	46307	0	49.103	N.D. #
9)	L2 AR-1221-2	5.325	4.316	25658	7340	39.585	25.284 #
10)	L2 AR-1221-3	0.000	4.407	0	23641	N.D.	25.549 #
11)	L3 AR-1232-1	0.000	4.407	0	23641	N.D.	29.947 #
28)	L6 AR-1254-3	7.850	0.000	25711	0	6.011	N.D. #
30)	L6 AR-1254-5	8.565	0.000	10337	0	3.214	N.D. #
32)	L7 AR-1260-2	8.296f	0.000	13634	0	3.627	N.D. #
34)	L7 AR-1260-4	8.887	0.000	48081	0	14.424	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO110821\
Data File : PO082609.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 16:55
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:25:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

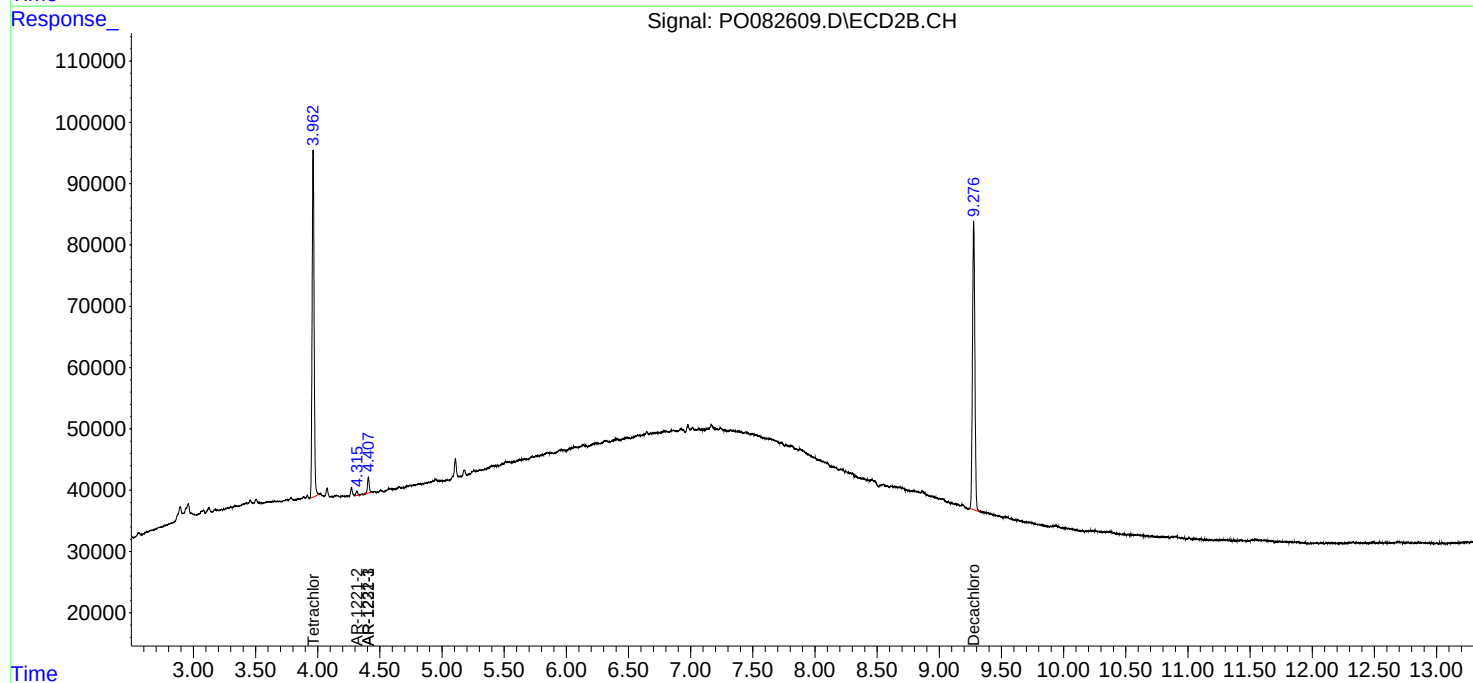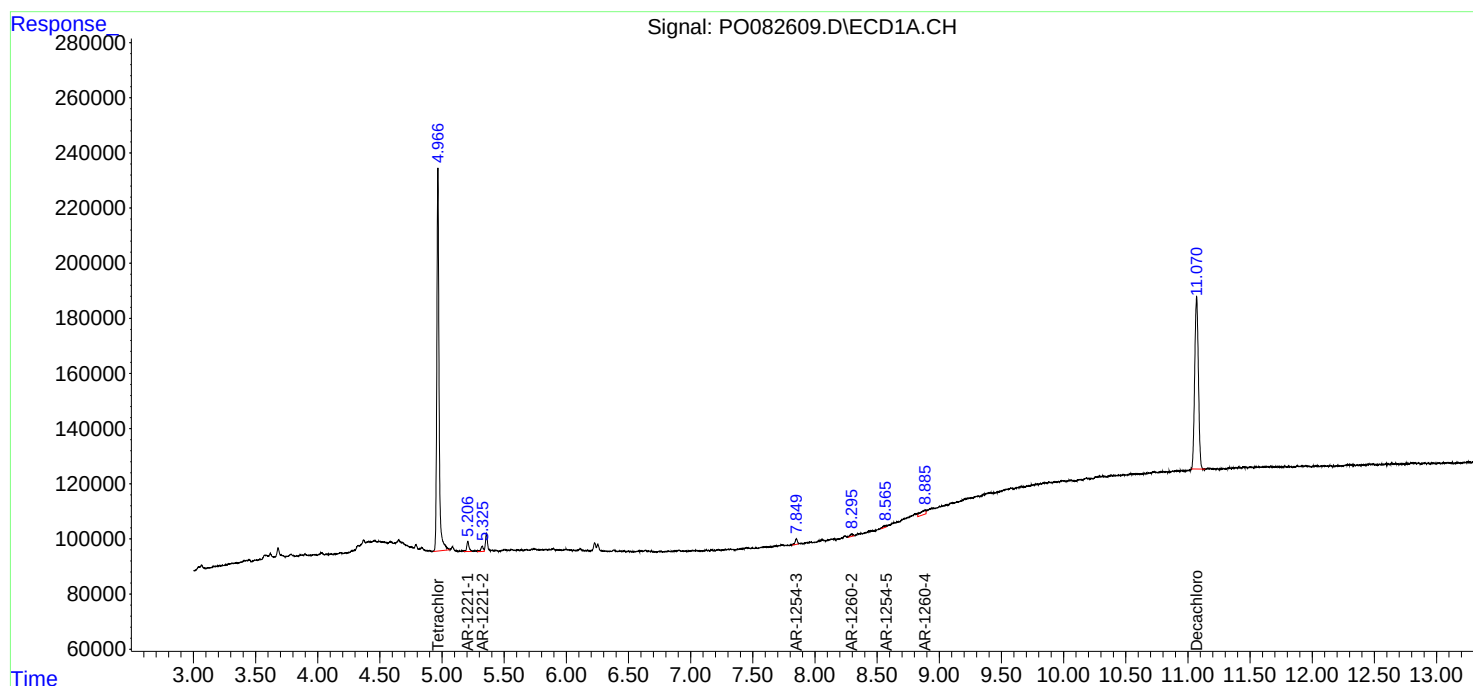


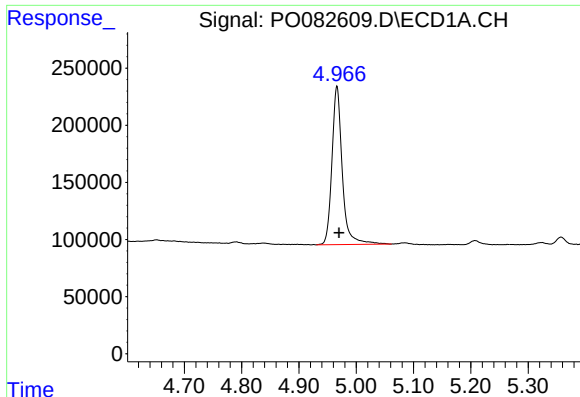

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: -0.004 min
Response: 1728367
Conc: 19.75 ng/ml

Instrument :
ECD_O
ClientSampleId :

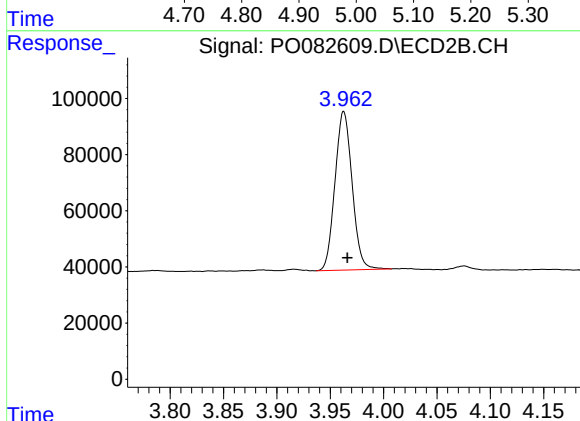


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.003 min
Response: 631967
Conc: 20.42 ng/ml

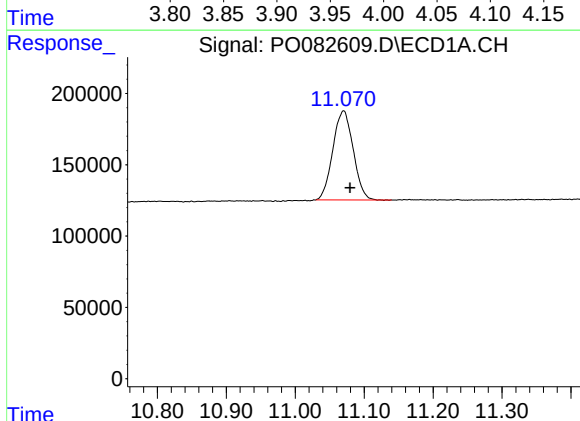


#2 Decachlorobiphenyl

R.T.: 11.070 min
Delta R.T.: -0.009 min
Response: 1281806
Conc: 20.30 ng/ml

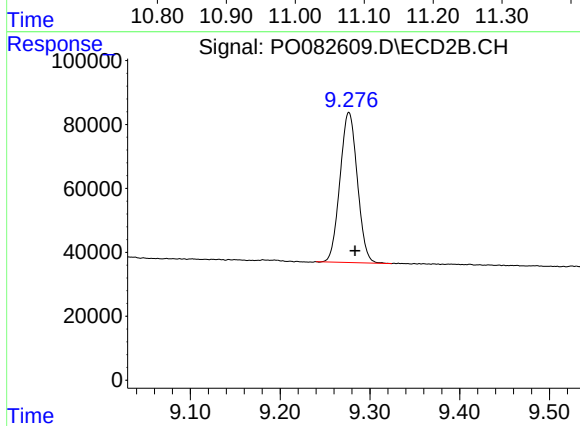

#2 Decachlorobiphenyl


R.T.: 9.277 min
Delta R.T.: -0.007 min
Response: 629783
Conc: 21.87 ng/ml

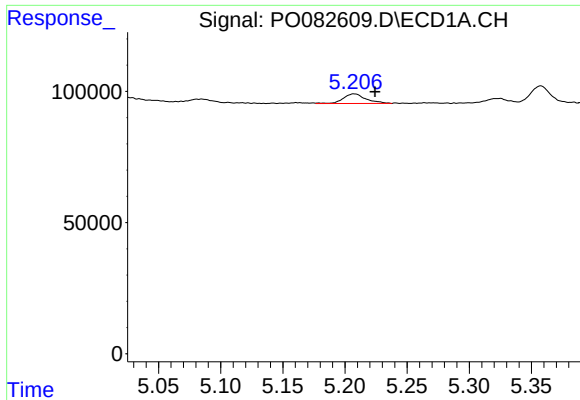

#8 AR-1221-1


R.T.: 5.207 min
Delta R.T.: -0.017 min
Response: 46307
Conc: 49.10 ng/ml

Instrument :
ECD_O
ClientSampleId :

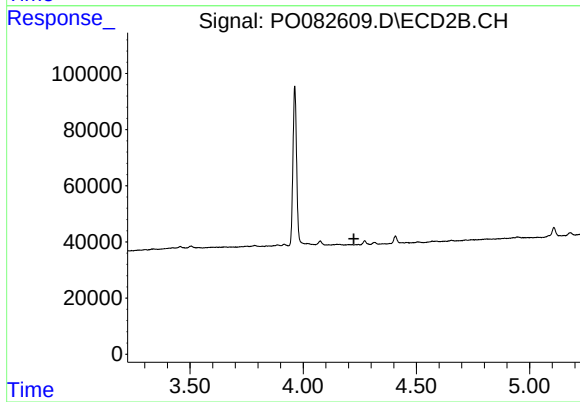


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.224 min
Response: 0
Conc: N.D.

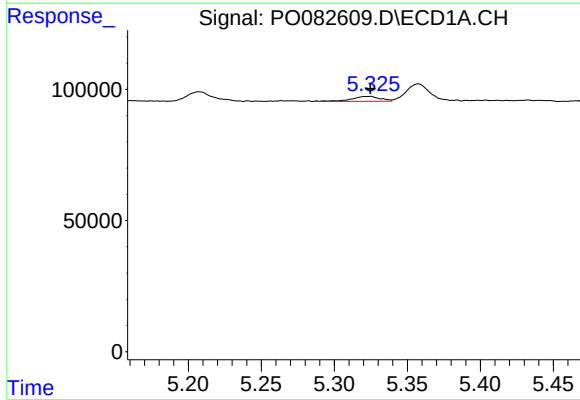


#9 AR-1221-2

R.T.: 5.325 min
Delta R.T.: 0.000 min
Response: 25658
Conc: 39.58 ng/ml

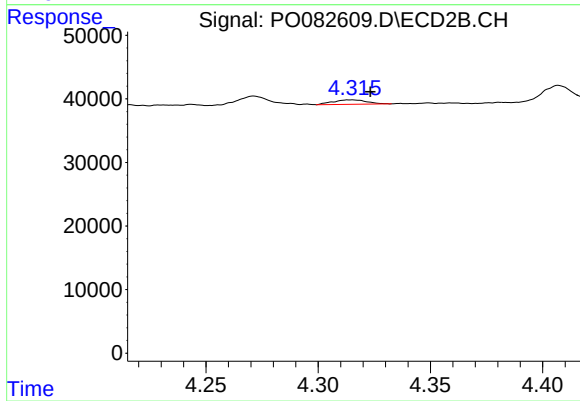

#9 AR-1221-2


R.T.: 4.316 min
Delta R.T.: -0.008 min
Response: 7340
Conc: 25.28 ng/ml

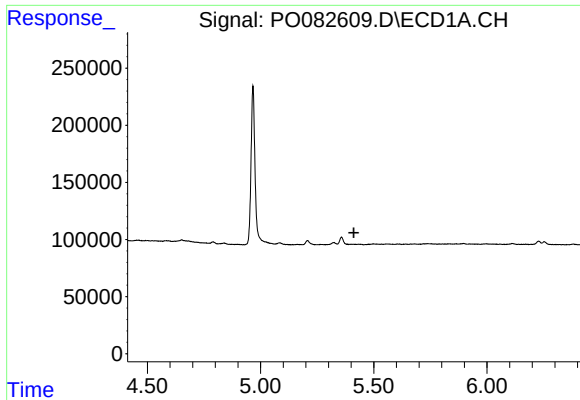

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

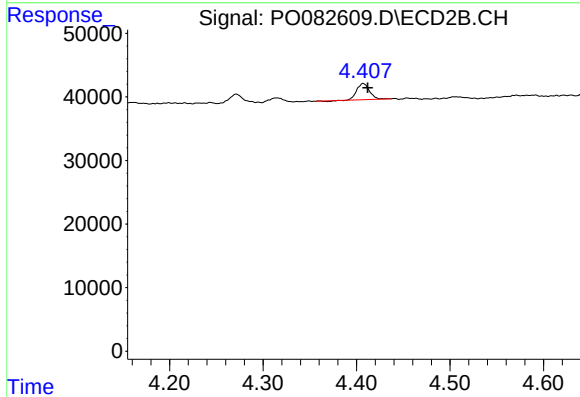


#10 AR-1221-3

R.T.: 4.407 min
Delta R.T.: -0.005 min
Response: 23641
Conc: 25.55 ng/ml

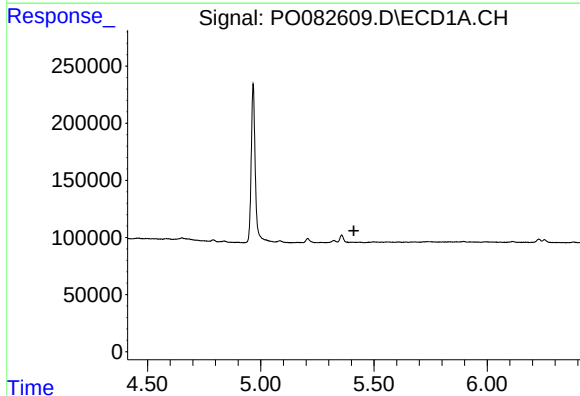


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.

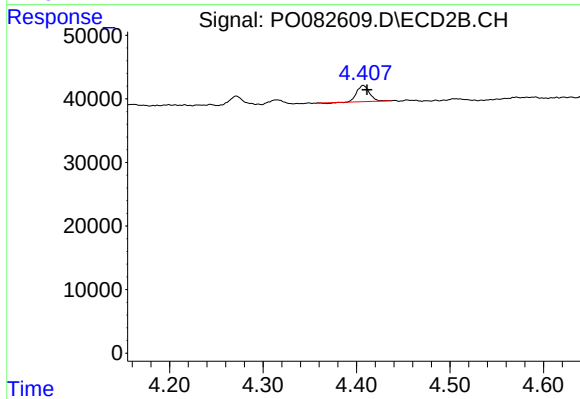

#11 AR-1232-1


R.T.: 4.407 min
Delta R.T.: -0.004 min
Response: 23641
Conc: 29.95 ng/ml

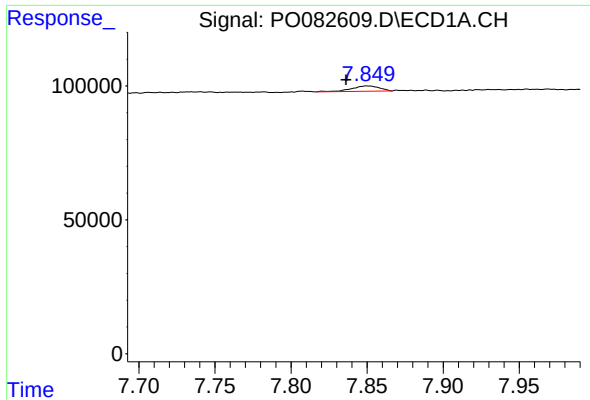

#28 AR-1254-3


R.T.: 7.850 min
Delta R.T.: 0.014 min
Response: 25711
Conc: 6.01 ng/ml

Instrument :
ECD_O
ClientSampleId :

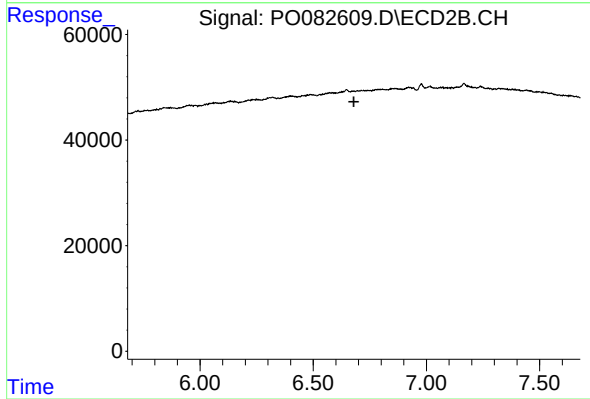


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

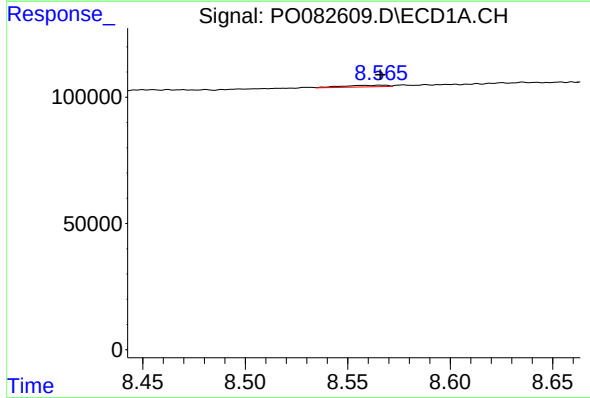


#30 AR-1254-5

R.T.: 8.565 min
Delta R.T.: 0.000 min
Response: 10337
Conc: 3.21 ng/ml

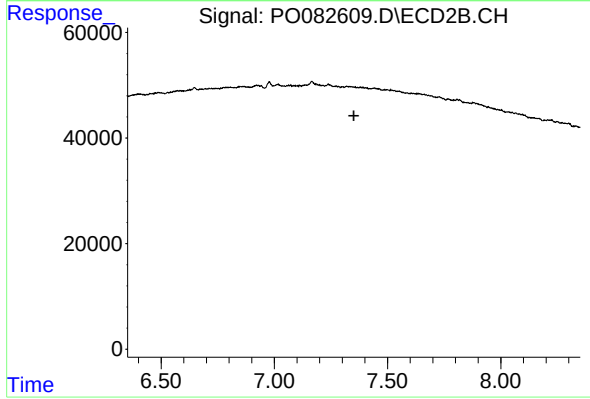

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.351 min
Response: 0
Conc: N.D.

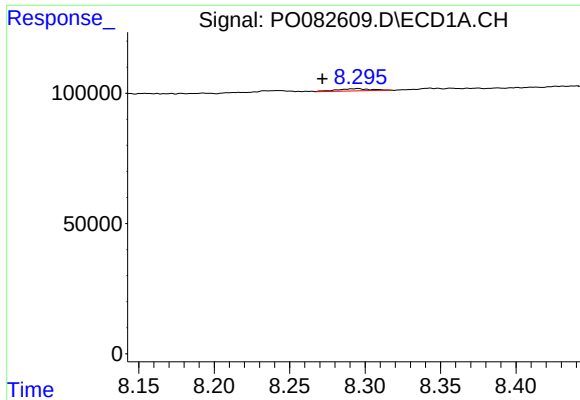

#32 AR-1260-2


R.T.: 8.296 min
Delta R.T.: 0.024 min
Response: 13634
Conc: 3.63 ng/ml

Instrument :
ECD_O
ClientSampleId :

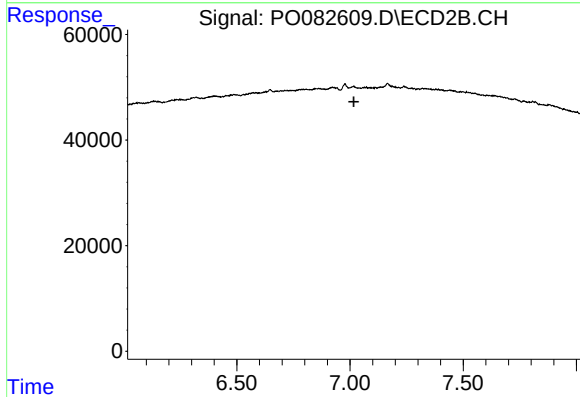


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

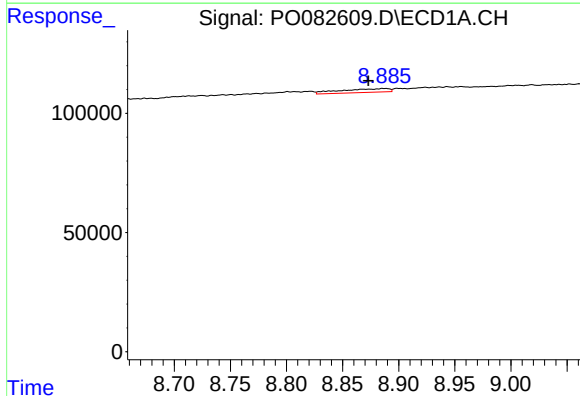

#34 AR-1260-4

R.T.: 8.887 min
Delta R.T.: 0.014 min
Response: 48081
Conc: 14.42 ng/ml

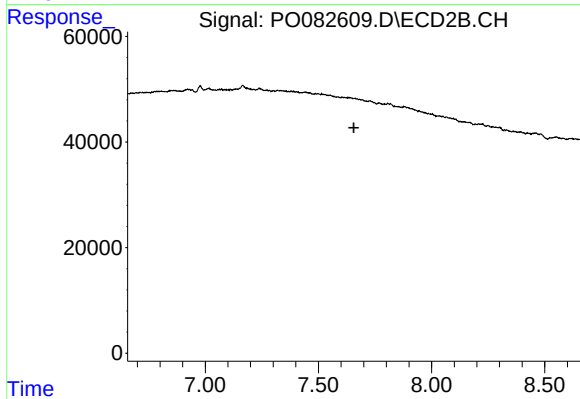

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.657 min
Response: 0
Conc: N.D.